
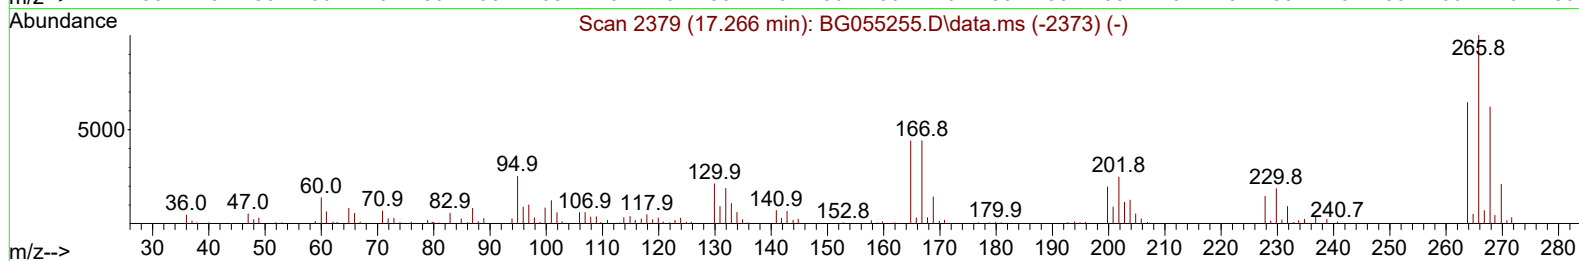
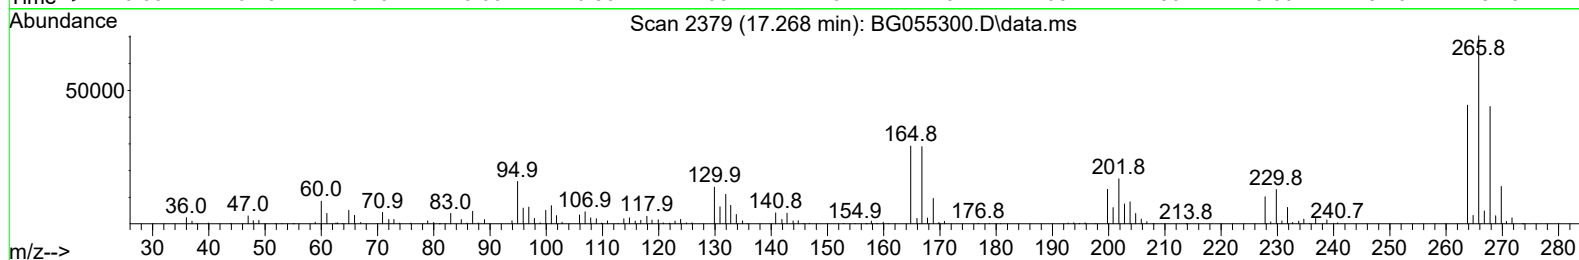


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
Data File : BG055300.D
Acq On : 26 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 10:36:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

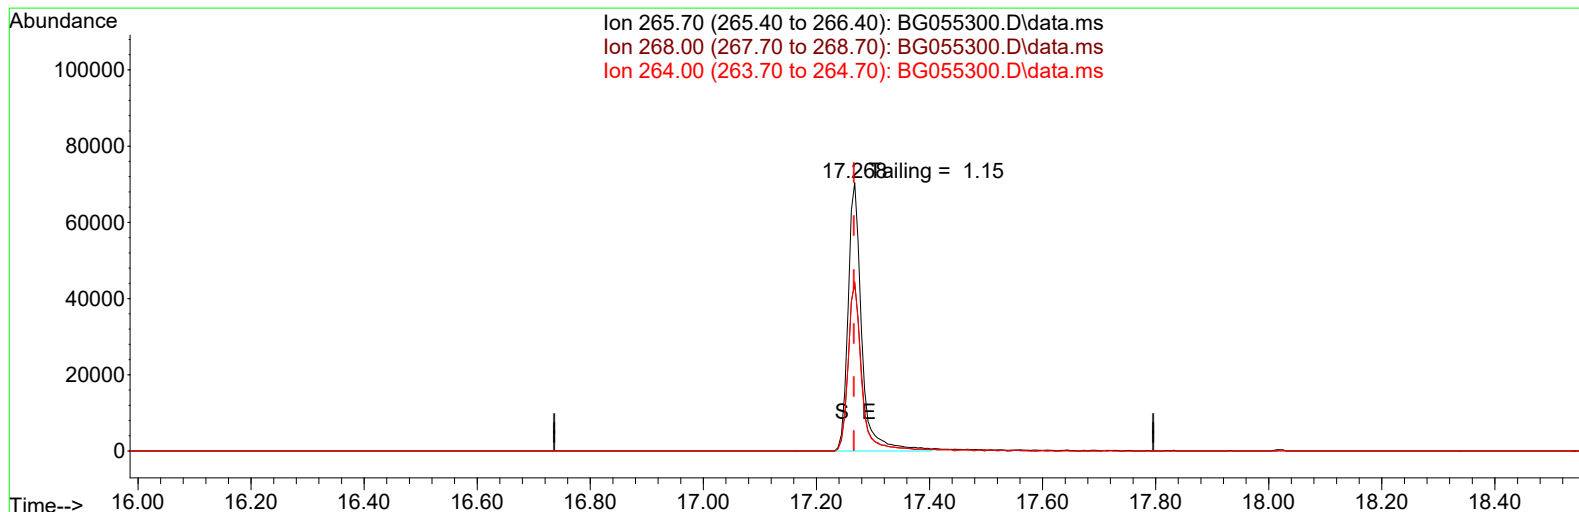

TIC: BG055300.D\data.ms

(70) Pentachlorophenol (C)




17.268min (+ 0.002) 33733.75 ng

response 119560

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	62.49
264.00	64.40	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
Data File : BG055300.D
Acq On : 26 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 10:36:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

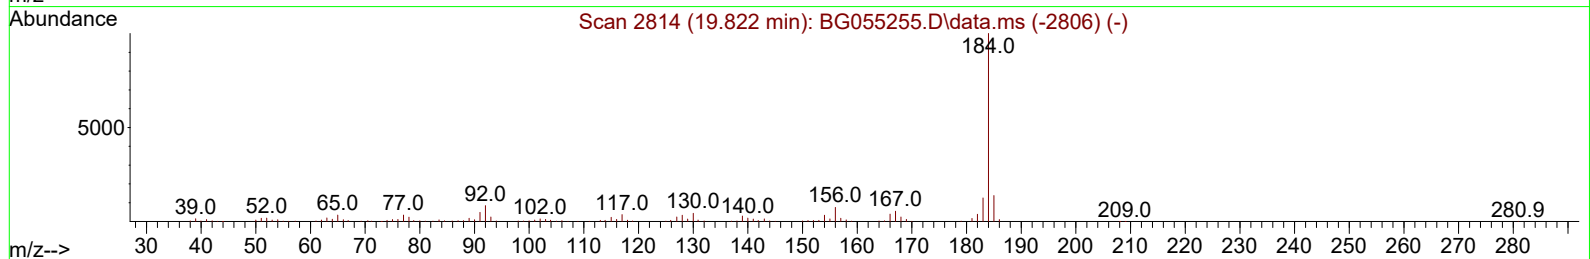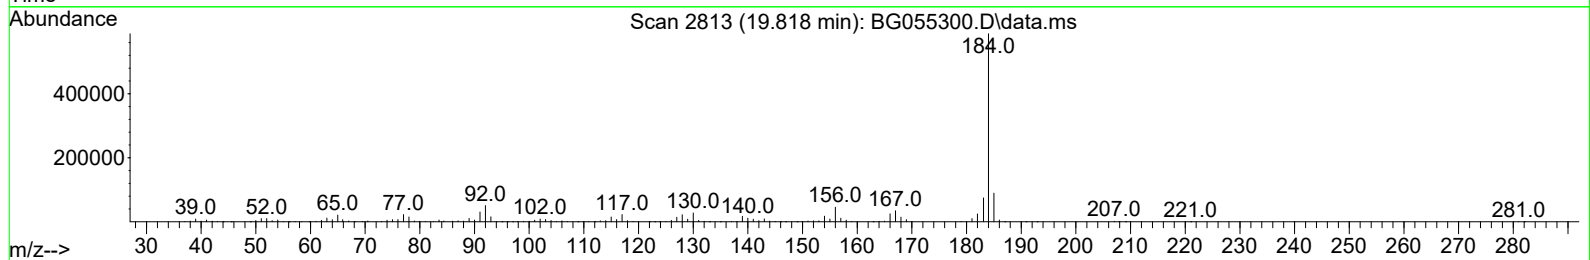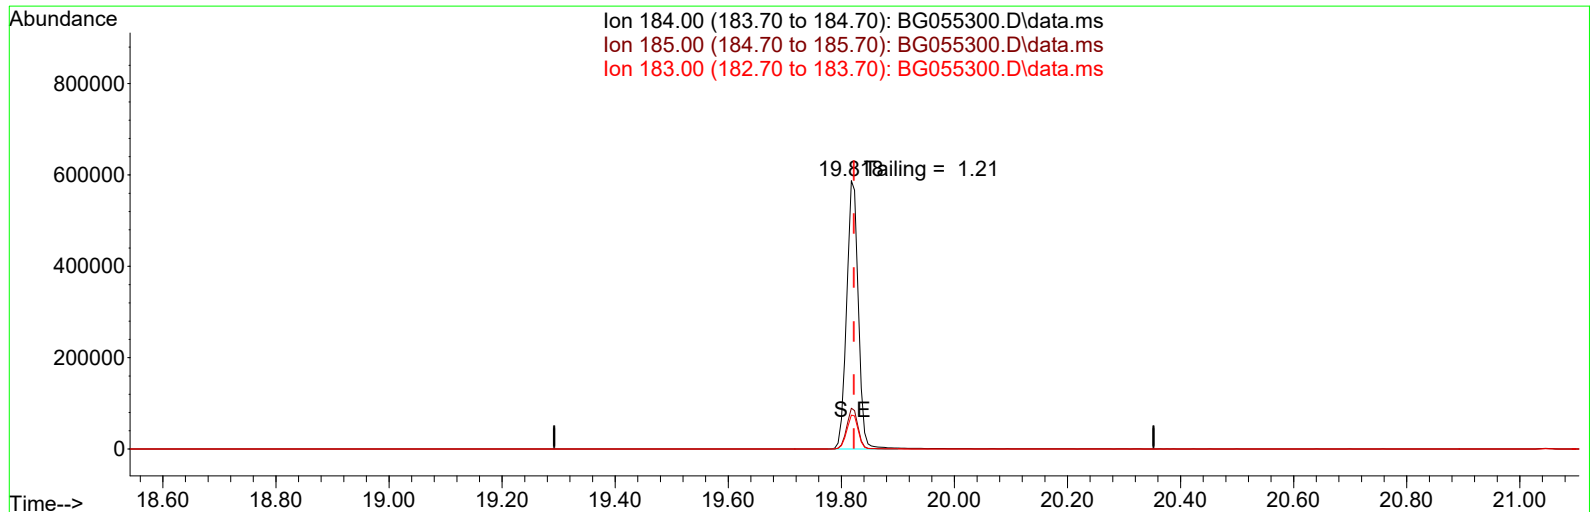

TIC: BG055300.D\data.ms

(77) Benzidine**19.818min (-0.004) 321578.57 ng****response 848710**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	15.25
183.00	12.50	12.68
0.00	0.00	0.00