


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
 Data File : BG055293.D
 Acq On : 26 Oct 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 24 16:54:05 2022

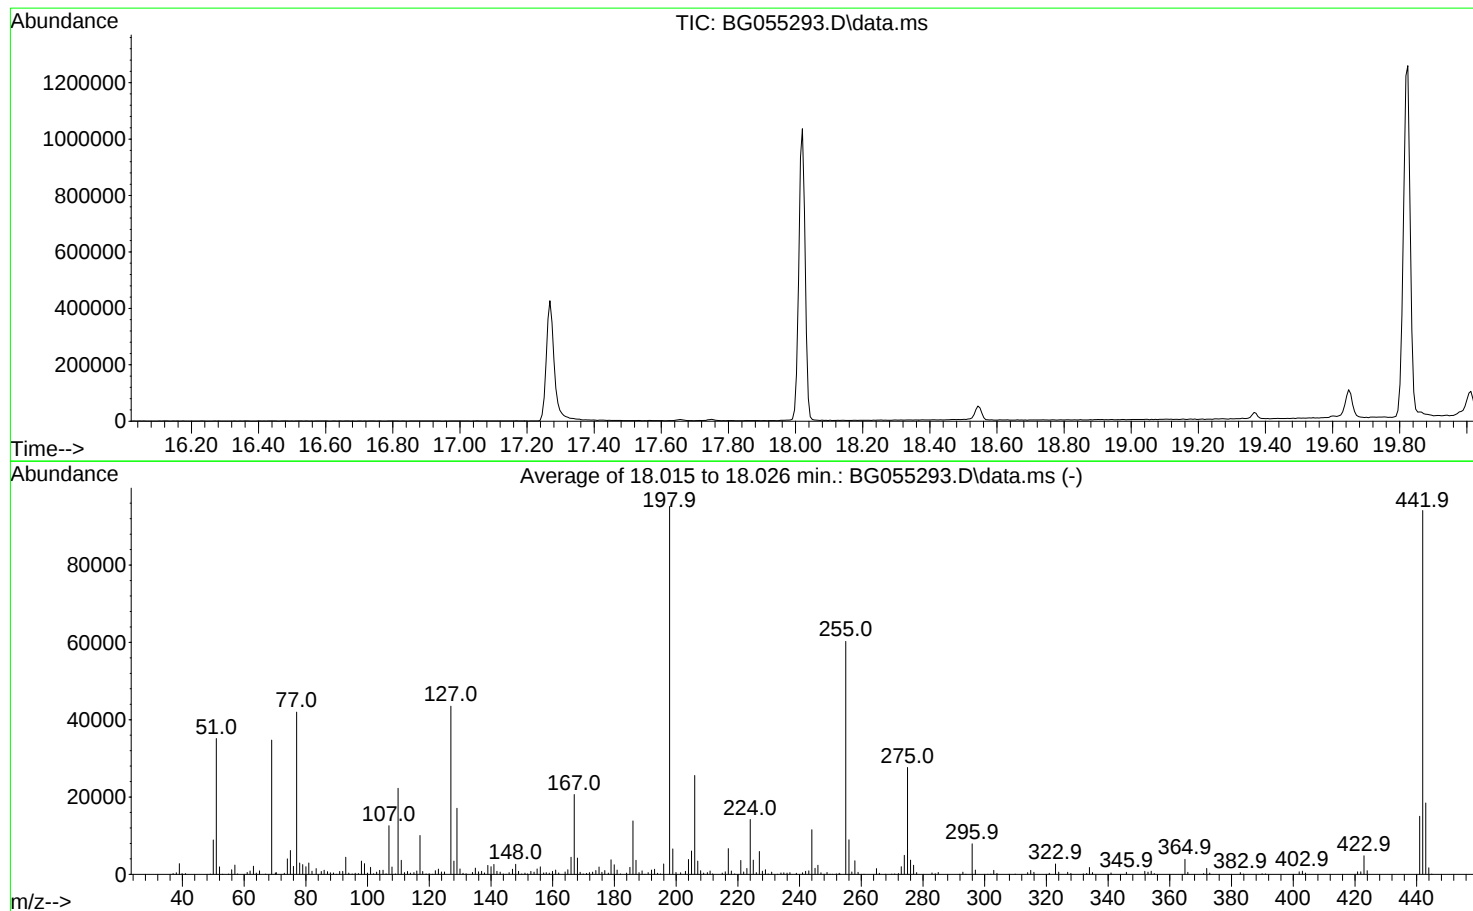




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	35128	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.5	34731	PASS
70	69	0.00	2	1.3	457	PASS
127	198	10	80	45.7	43507	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95152	PASS
199	198	5	9	6.9	6568	PASS
275	198	10	60	29.0	27637	PASS
365	198	1	100	4.1	3894	PASS
441	198	0.01	100	15.8	15035	PASS
442	442	50	100	100.0	94101	PASS
443	442	15	24	19.6	18451	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
 Data File : BG055293.D
 Acq On : 26 Oct 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 28 09:30:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 24 16:54:05 2022
 Response via : Initial Calibration

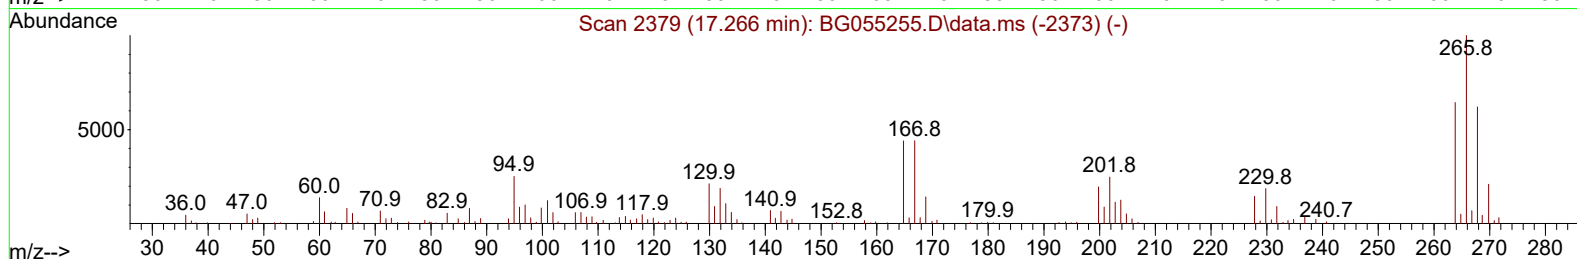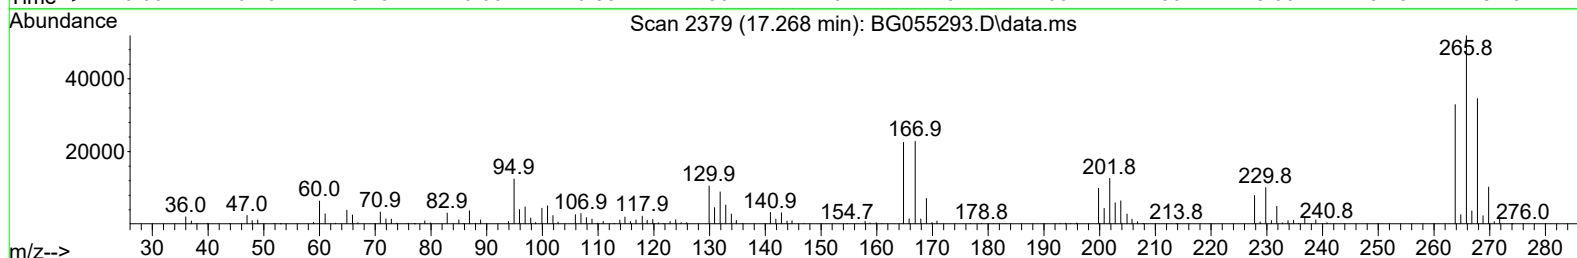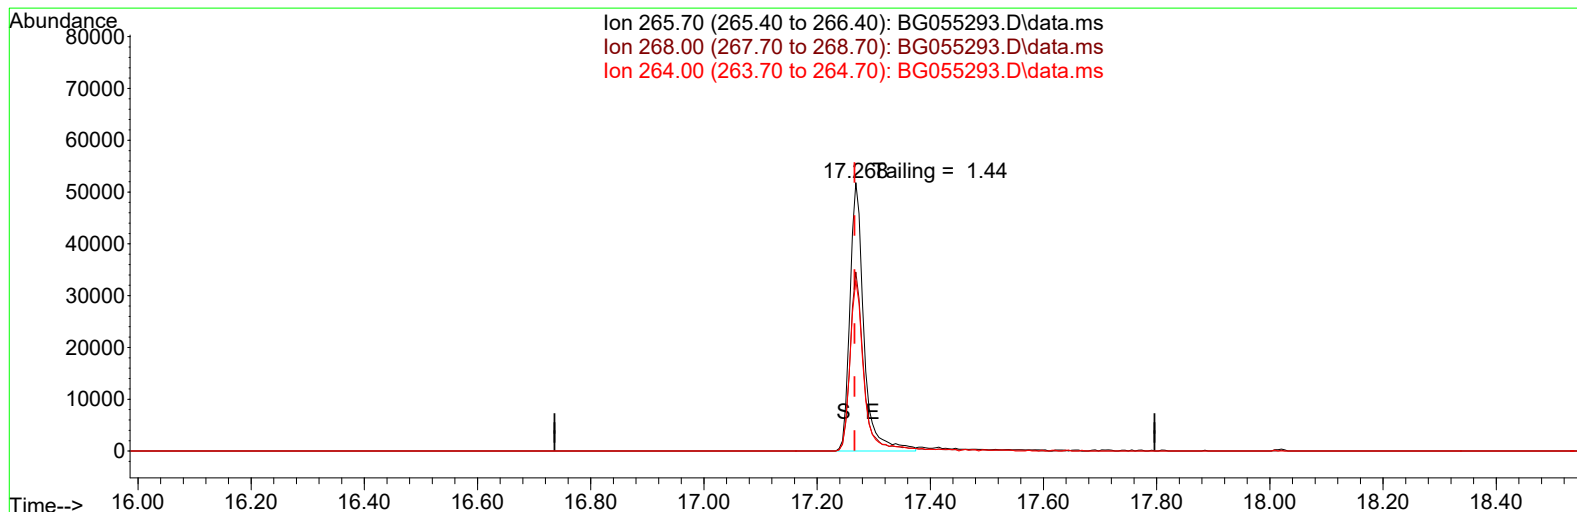

TIC: BG055293.D\data.ms

(70) Pentachlorophenol (C)

17.268min (+ 0.002) 33652.41 ng




response 89292

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	66.67
264.00	64.40	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
Data File : BG055293.D
Acq On : 26 Oct 2022 10:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 28 09:30:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

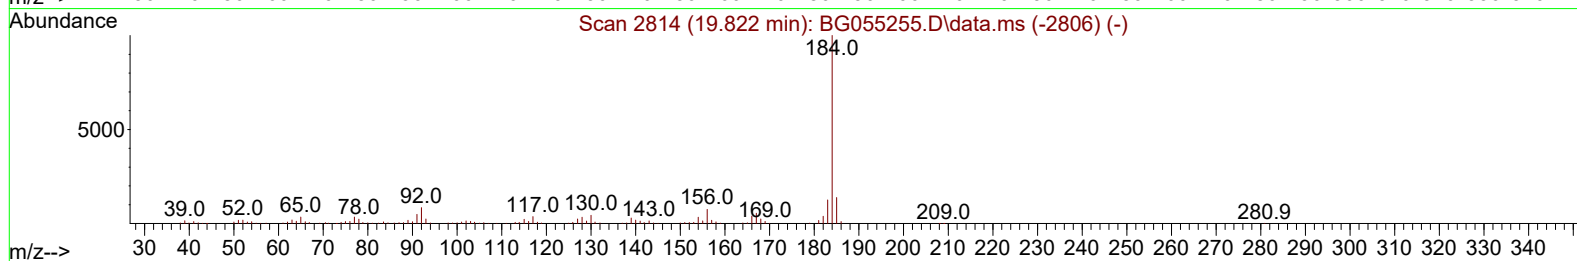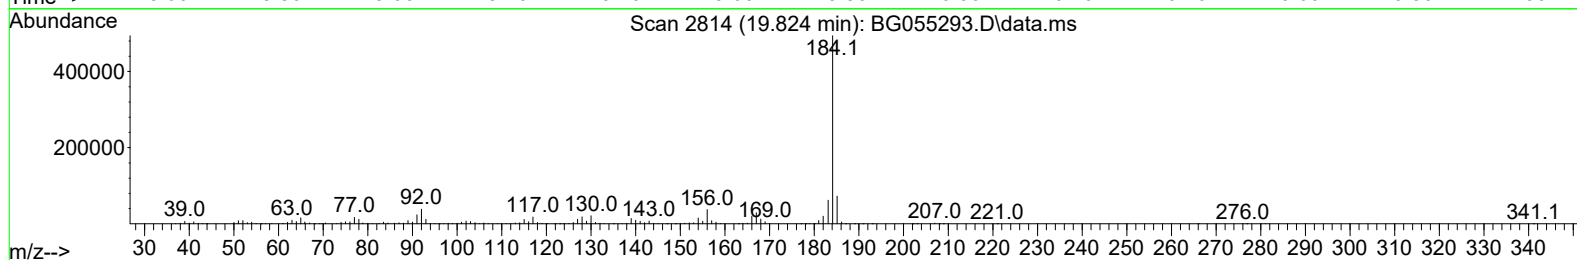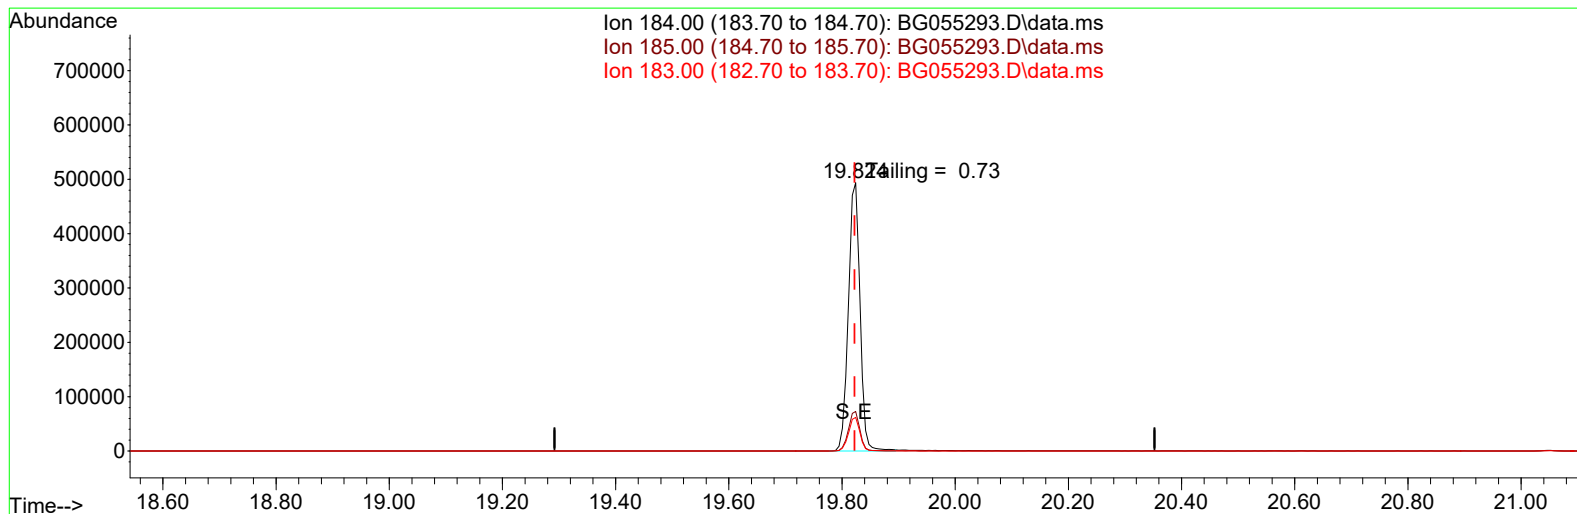

TIC: BG055293.D\data.ms

(77) Benzidine

19.824min (+ 0.002) 34136.01 ng

response 708336

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.71
183.00	12.50	12.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2022	BNA_G	BG055293.D
Compound Name	Response	Retention Time
DDT	338507	21.046
DDD	4332	20.653
DDE	170	20.112
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4502	343009	1.31

Instrument :
BNA_G
ClientSampleId :
DFTPP