


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
Data File : BG055300.D
Acq On : 26 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 24 16:54:05 2022

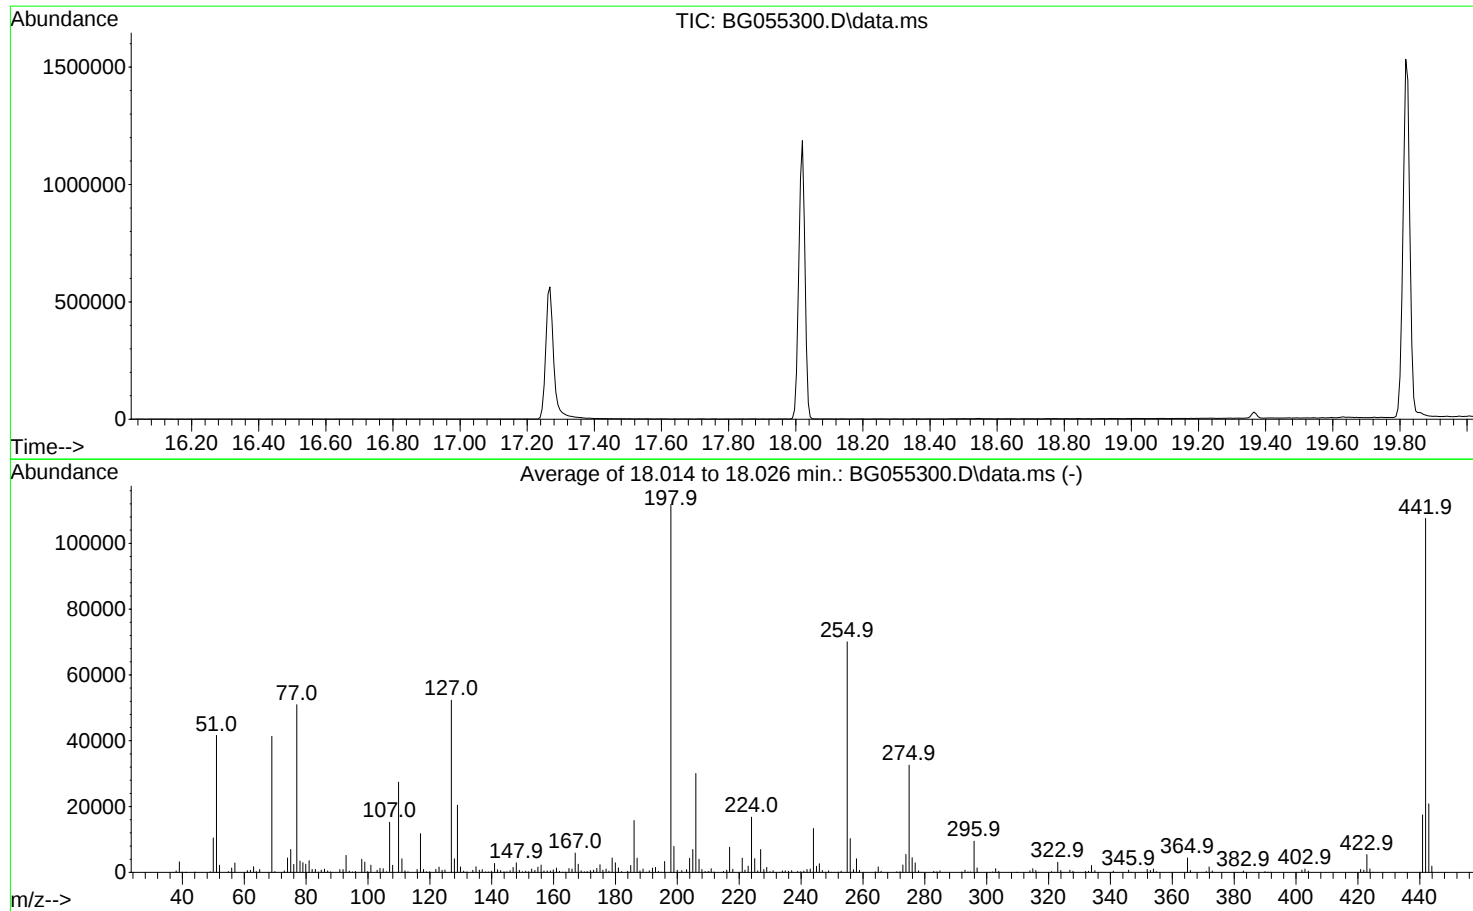




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	41608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.0	41349	PASS
70	69	0.00	2	0.6	241	PASS
127	198	10	80	46.8	52325	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111803	PASS
199	198	5	9	7.0	7858	PASS
275	198	10	60	29.1	32571	PASS
365	198	1	100	3.9	4390	PASS
441	198	0.01	100	15.6	17460	PASS
442	442	50	100	100.0	107549	PASS
443	442	15	24	19.4	20816	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
Data File : BG055300.D
Acq On : 26 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 27 10:36:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

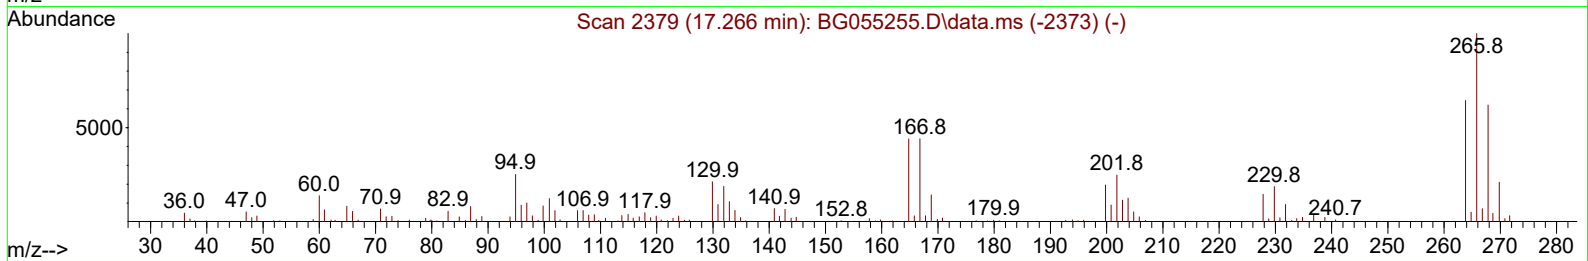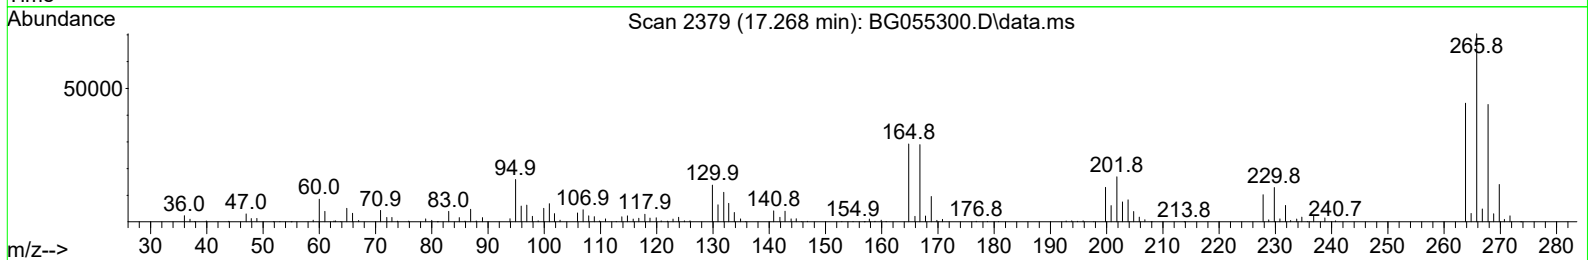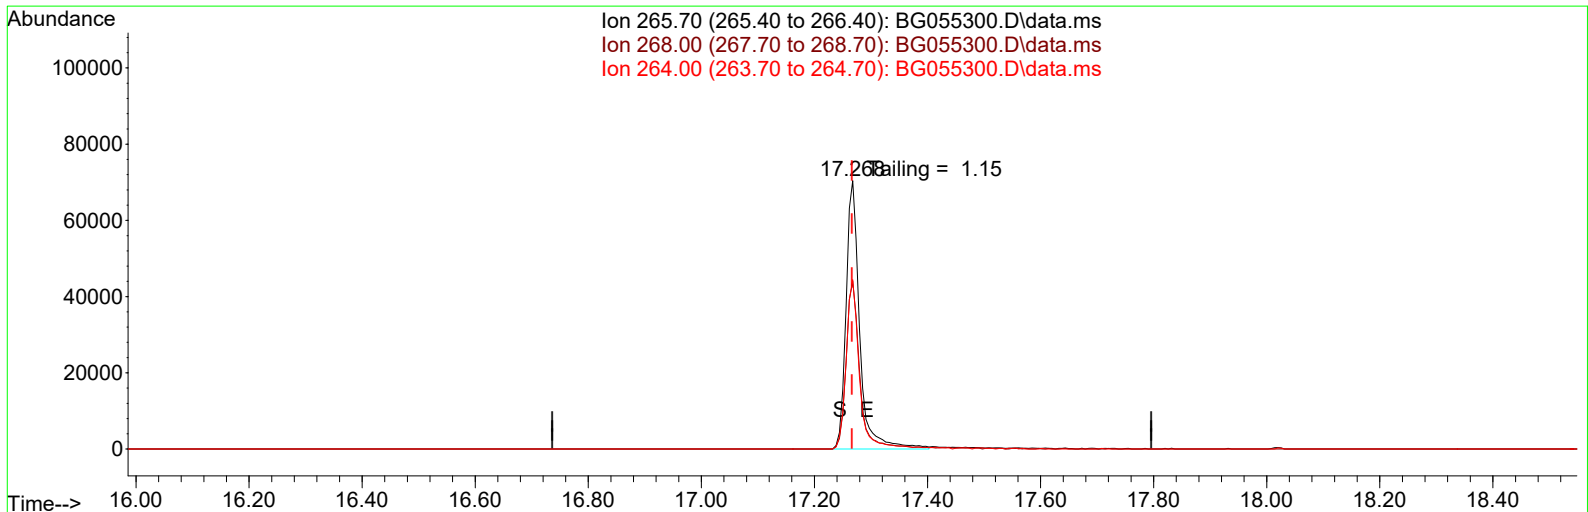

TIC: BG055300.D\data.ms

(70) Pentachlorophenol (C)

17.268min (+ 0.002) 33733.75 ng




response 119560

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	62.49
264.00	64.40	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
Data File : BG055300.D
Acq On : 26 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 27 10:36:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

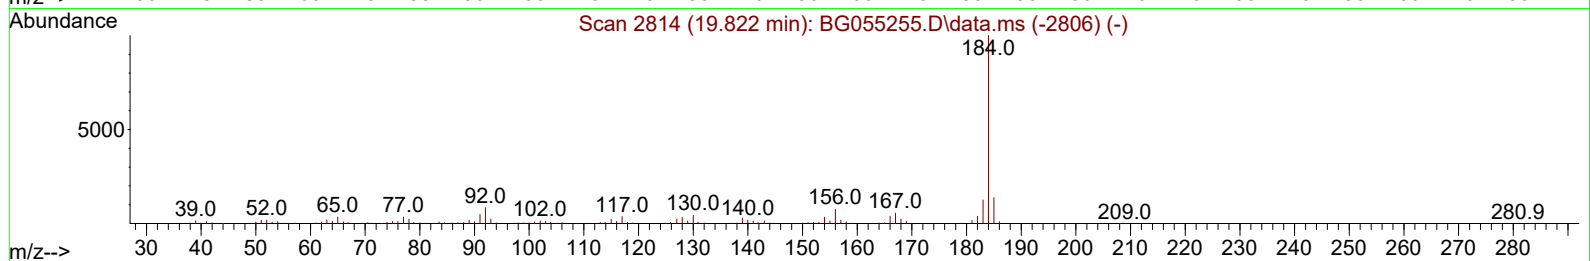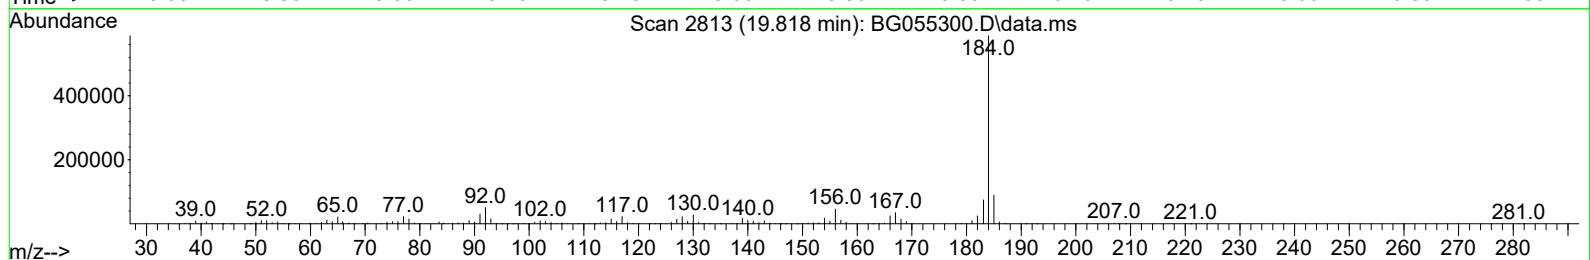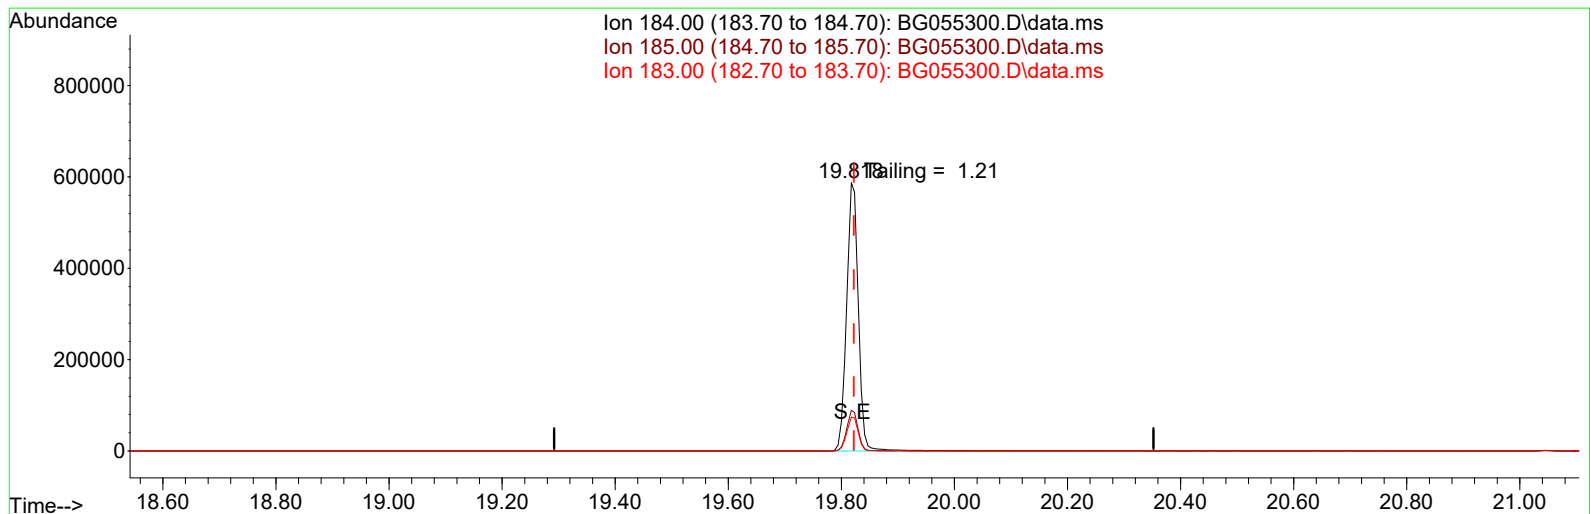

TIC: BG055300.D\data.ms

(77) Benzidine

19.818min (-0.004) 321578.57 ng

response 848710

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	15.25
183.00	12.50	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2022	BNA_G	BG055300.D
Compound Name	Response	Retention Time
DDT	402525	21.046
DDD	4918	20.599
DDE	254	20.106
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5172	407697	1.27

Instrument :
BNA_G
ClientSampleId :
DFTPP