

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102716\
 Data File : BG024528.D
 Acq On : 27 Oct 2016 19:35
 Operator : UM/SJ
 Sample : PB94345BSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB94345BSD

Quant Time: Oct 28 02:12:26 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	118038	20.00	ng	0.00
21) Naphthalene-d8	11.10	136	454241	20.00	ng	0.00
38) Acenaphthene-d10	14.89	164	339584	20.00	ng	0.00
63) Phenanthrene-d10	17.63	188	724688	20.00	ng	0.00
75) Chrysene-d12	21.93	240	1011156	20.00	ng	0.00
86) Perylene-d12	25.35	264	1085463	20.00	ng	-0.01

System Monitoring Compounds

5) 2-Fluorophenol	5.80	112	482225	66.96	ng	0.00
7) Phenol-d6	7.40	99	691327	69.98	ng	0.00
23) Nitrobenzene-d5	9.45	82	880788	88.28	ng	0.00
41) 2,4,6-Tribromophenol	16.37	330	353417	69.66	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	1728926	84.62	ng	0.00
78) Terphenyl-d14	20.21	244	2880380	85.12	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.66	88	96579	32.82	ng	# 90
3) Pyridine	4.08	79	293957	33.37	ng	85
4) n-Nitrosodimethylamine	3.99	42	168348	36.92	ng	89
6) Aniline	7.59	93	275495	22.01	ng	97
8) 2-Chlorophenol	7.83	128	301262	41.14	ng	90
9) Benzaldehyde	7.40	77	66475	10.89	ng	94
10) Phenol	7.43	94	438689	43.08	ng	97
11) bis(2-Chloroethyl)ether	7.68	93	308467	40.32	ng	91
12) 1,3-Dichlorobenzene	8.16	146	353557	39.00	ng	95
13) 1,4-Dichlorobenzene	8.31	146	353004	39.43	ng	97
14) 1,2-Dichlorobenzene	8.63	146	339158	39.40	ng	91
15) Benzyl Alcohol	8.50	79	371332	40.41	ng	96
16) 2,2'-oxybis(1-Chloropropan	8.80	45	527189	37.14	ng	97
17) 2-Methylphenol	8.70	107	278321	41.25	ng	95
18) Hexachloroethane	9.36	117	134399	39.05	ng	92
19) n-Nitroso-di-n-propylamine	9.07	70	295002	40.52	ng	97
20) 3+4-Methylphenols	9.03	107	375678	41.47	ng	98
22) Acetophenone	9.10	105	476157	40.81	ng	96
24) Nitrobenzene	9.49	77	439049	39.56	ng	99
25) Isophorone	10.01	82	761007	41.01	ng	99
26) 2-Nitrophenol	10.20	139	164491	39.93	ng	96
27) 2,4-Dimethylphenol	10.24	122	317674	44.05	ng	94
28) bis(2-Chloroethoxy)methane	10.48	93	415464	43.27	ng	98
29) 2,4-Dichlorophenol	10.74	162	335881	44.37	ng	91
30) 1,2,4-Trichlorobenzene	10.95	180	358350	39.91	ng	97
31) Naphthalene	11.15	128	899748	39.71	ng	98
32) Benzoic acid	10.35	122	211137	35.15	ng	91
33) 4-Chloroaniline	11.25	127	176608	17.95	ng	94
34) Hexachlorobutadiene	11.42	225	280079	39.85	ng	93
35) Caprolactam	12.01	113	66392	23.96	ng	# 84
36) 4-Chloro-3-methylphenol	12.34	107	389414	42.61	ng	95
37) 2-Methylnaphthalene	12.73	142	652902	39.49	ng	97
39) 1,2,4,5-Tetrachlorobenzene	13.09	216	442288	38.62	ng	99
40) Hexachlorocyclopentadiene	13.06	237	661906	102.62	ng	96


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102716\
 Data File : BG024528.D
 Acq On : 27 Oct 2016 19:35
 Operator : UM/SJ
 Sample : PB94345BSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB94345BSD

Quant Time: Oct 28 02:12:26 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) 2,4,6-Trichlorophenol	13.32	196	291089	42.28	ng	98
43) 2,4,5-Trichlorophenol	13.40	196	316713	42.55	ng	97
45) 1,1'-Biphenyl	13.73	154	917145	38.92	ng	98
46) 2-Chloronaphthalene	13.77	162	732922	40.84	ng	99
47) 2-Nitroaniline	13.97	65	300987	40.97	ng	98
48) Acenaphthylene	14.61	152	1093828	39.75	ng	98
49) Dimethylphthalate	14.33	163	978162	40.57	ng	99
50) 2,6-Dinitrotoluene	14.46	165	222864	43.30	ng	87
51) Acenaphthene	14.95	154	733249	35.74	ng	95
52) 3-Nitroaniline	14.79	138	109362	20.53	ng	100
53) 2,4-Dinitrophenol	14.99	184	306604	82.21	ng	94
54) Dibenzofuran	15.28	168	1148212	40.49	ng	100
55) 4-Nitrophenol	15.08	139	392360	84.56	ng	# 84
56) 2,4-Dinitrotoluene	15.24	165	317760	42.49	ng	# 96
57) Fluorene	15.93	166	940998	40.01	ng	99
58) 2,3,4,6-Tetrachlorophenol	15.50	232	333838	43.26	ng	# 94
59) Diethylphthalate	15.68	149	999907	39.56	ng	99
60) 4-Chlorophenyl-phenylether	15.91	204	534689	40.52	ng	95
61) 4-Nitroaniline	15.95	138	214377	36.85	ng	96
62) Azobenzene	16.21	77	1058667	42.00	ng	95
64) 4,6-Dinitro-2-methylphenol	16.00	198	223292	44.72	ng	97
65) n-Nitrosodiphenylamine	16.13	169	871065	43.97	ng	98
66) 4-Bromophenyl-phenylether	16.81	248	388630	44.18	ng	99
67) Hexachlorobenzene	16.93	284	420771	43.29	ng	# 90
68) Atrazine	17.06	200	383884	45.17	ng	98
69) Pentachlorophenol	17.27	266	586180	91.38	ng	99
70) Phenanthrene	17.67	178	1577205	42.70	ng	96
71) Anthracene	17.76	178	1603657	43.03	ng	99
72) Carbazole	18.03	167	1422414	41.85	ng	99
73) Di-n-butylphthalate	18.56	149	1682649	42.94	ng	97
74) Fluoranthene	19.67	202	2020792	43.28	ng	95
76) Benzidine	19.84	184	784985	32.95	ng	97
77) Pyrene	20.02	202	2059116	41.66	ng	98
79) Butylbenzylphthalate	20.89	149	882135	42.81	ng	98
80) Benzo(a)anthracene	21.91	228	2335548	42.05	ng	96
81) 3,3'-Dichlorobenzidine	21.81	252	501769	22.39	ng	93
82) Chrysene	21.98	228	2166469	40.95	ng	98
83) Bis(2-ethylhexyl)phthalate	21.77	149	1229712	41.72	ng	99
84) Di-n-octyl phthalate	23.04	149	2121564	43.37	ng	95
85) Indeno(1,2,3-cd)pyrene	29.31	276	3061711	41.93	ng	98
87) Benzo(b)fluoranthene	24.26	252	2418654	41.22	ng	98
88) Benzo(k)fluoranthene	24.33	252	2407855	42.49	ng	100
89) Benzo(a)pyrene	25.19	252	2354697	41.07	ng	98
90) Dibenzo(a,h)anthracene	29.37	278	2549126	40.51	ng	97
91) Benzo(g,h,i)perylene	30.54	276	2516588	40.03	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.27 min Scan# 925
Delta R.T. 0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Instrument :
BNA_G
ClientSampleId :
PB94345BSD

Tgt Ion	Ratio	Lower	Upper
152	100		
150	164.7	114.0	171.0
115	62.8	48.1	72.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E





#2


1,4-Dioxane
Concen: 32.82 ng
RT: 3.66 min Scan# 140
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Tgt Ion	Ratio	Lower	Upper
88	100		
58	91.3	79.4	119.2
43	32.0	33.8	50.6



Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 58.00 (57.70 to 58.70): BGC
Ion 43.00 (42.70 to 43.70): BGC





#3

Pyridine

Concen: 33.37 ng

RT: 4.08 min Scan# 211

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35

Instrument :

BNA_G

ClientSampleId :

PB94345BSD





Tgt Ion: 79 Resp: 293957

Ion Ratio Lower Upper

79 100

52 80.3 77.8 116.6

51 46.9 43.2 64.8



#4

n-Nitrosodimethylamine

Concen: 36.92 ng

RT: 3.99 min Scan# 196

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35




Tgt Ion: 42 Resp: 168348


Ion Ratio Lower Upper

42 100

74 107.9 76.7 115.1

44 8.0 6.1 9.1





#5

2-Fluorophenol

Concen: 66.96 ng

RT: 5.80 min Scan# 504

Delta R.T. 0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35

Instrument :

BNA_G

ClientSampleId :

PB94345BSD


Tgt Ion: 112 Resp: 482225

Ion Ratio Lower Upper




112 100

64 75.3 61.8 92.6

63 46.3 37.2 55.8



Abundance Ion 112.00 (111.70 to 112.70): BGC
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC



#6

Aniline

Concen: 22.01 ng

RT: 7.59 min Scan# 808

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35


Tgt Ion: 93 Resp: 275495

Ion Ratio Lower Upper



93 100


66 45.0 35.4 53.2

65 23.1 21.2 31.8



Abundance Ion 93.00 (92.70 to 93.70): BGC
Ion 66.00 (65.70 to 66.70): BGC
Ion 65.00 (64.70 to 65.70): BGC





#7

Phenol-d6

Concen: 69.98 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35

Instrument :

BNA_G

ClientSampleId :

PB94345BSD


Tgt Ion: 99 Resp: 691327

Ion Ratio Lower Upper




99 100

42 20.4 20.5 30.7#

71 44.8 37.6 56.4



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC



#8

2-Chlorophenol

Concen: 41.14 ng

RT: 7.83 min Scan# 849

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35


Tgt Ion: 128 Resp: 301262

Ion Ratio Lower Upper



128 100


130 30.9 11.4 51.4

64 55.6 46.6 86.6



Abundance Ion 128.00 (127.70 to 128.70): BGC
Ion 130.00 (129.70 to 130.70): BGC
Ion 64.00 (63.70 to 64.70): BGC





#9

Benzaldehyde

Concen: 10.89 ng

RT: 7.40 min Scan# 777

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35

Instrument :

BNA_G

ClientSampleId :

PB94345BSD


Tgt Ion: 77 Resp: 66475

Ion Ratio Lower Upper

77 100

105 83.5 60.9 100.9




106 67.0 55.1 95.1



Abundance Ion 77.00 (76.70 to 77.70): BGC

Ion 105.00 (104.70 to 105.70): BGC

Ion 106.00 (105.70 to 106.70): BGC

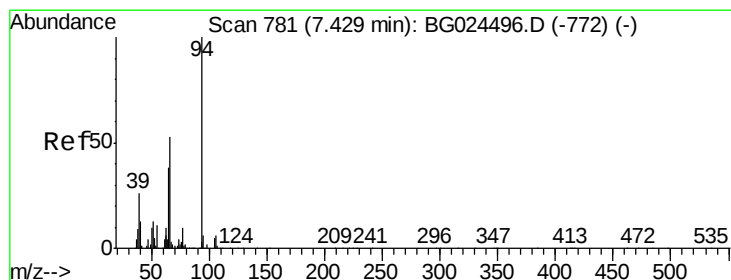

#10

Phenol

Concen: 43.08 ng

RT: 7.43 min Scan# 782

Delta R.T. 0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35


Tgt Ion: 94 Resp: 438689

Ion Ratio Lower Upper

94 100

65 38.7 20.6 60.6



66 53.7 35.5 75.5




Abundance Ion 94.00 (93.70 to 94.70): BGC

Ion 65.00 (64.70 to 65.70): BGC

Ion 66.00 (65.70 to 66.70): BGC









#11
bis(2-Chloroethyl)ether
Concen: 40.32 ng
RT: 7.68 min Scan# 824
Delta R.T. 0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35




Instrument :
BNA_G
ClientSampleId :
PB94345BSD

Tgt Ion: 93 Resp: 308467
Ion Ratio Lower Upper
93 100
63 88.1 78.5 118.5
95 32.3 9.8 49.8



#12
1,3-Dichlorobenzene
Concen: 39.00 ng
RT: 8.16 min Scan# 906
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Tgt Ion: 146 Resp: 353557
Ion Ratio Lower Upper
146 100
148 63.1 49.2 73.8
75 36.7 33.4 50.2









#13
 1,4-Dichlorobenzene
 Concen: 39.43 ng
 RT: 8.31 min Scan# 931
 Delta R.T. -0.00 min
 Lab File: BG024528.D
 Acq: 27 Oct 2016 19:35




Instrument :
 BNA_G
 ClientSampleId :
 PB94345BSD


Tgt Ion:146 Resp: 353004
 Ion Ratio Lower Upper
 146 100
 148 62.6 52.2 78.2
 111 47.6 37.0 55.6



#14
 1,2-Dichlorobenzene
 Concen: 39.40 ng
 RT: 8.63 min Scan# 985
 Delta R.T. -0.00 min
 Lab File: BG024528.D
 Acq: 27 Oct 2016 19:35

Tgt Ion:146 Resp: 339158
 Ion Ratio Lower Upper
 146 100
 148 58.7 54.6 81.8
 111 45.5 39.7 59.5





#15

Benzyl Alcohol

Concen: 40.41 ng

RT: 8.50 min Scan# 964

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35

Instrument :

BNA_G

ClientSampleId :

PB94345BSD





Tgt Ion: 79 Resp: 371332

Ion Ratio Lower Upper

79 100

108 53.6 45.5 68.3

77 65.7 54.3 81.5



#16

2,2'-oxybis(1-Chloropropane)

Concen: 37.14 ng

RT: 8.80 min Scan# 1014

Delta R.T. 0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35




Tgt Ion: 45 Resp: 527189

Ion Ratio Lower Upper

45 100

77 12.0 0.0 30.6

79 9.4 0.0 28.5









#17
2-Methylphenol
Concen: 41.25 ng
RT: 8.70 min Scan# 997
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Instrument :
BNA_G
ClientSampleId :
PB94345BSD

Tgt Ion:	107	Resp:	278321
Ion	Ratio	Lower	Upper
107	100		
108	114.1	85.6	128.4
77	59.0	51.4	77.2
79	62.1	49.2	73.8




Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BG
Ion 79.00 (78.70 to 79.70): BG






#18
Hexachloroethane
Concen: 39.05 ng
RT: 9.36 min Scan# 1110
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Tgt Ion:	117	Resp:	134399
Ion	Ratio	Lower	Upper
117	100		
119	98.9	69.8	104.6
201	113.9	95.4	143.0



Abundance Ion 117.00 (116.70 to 117.70): E
Ion 119.00 (118.70 to 119.70): E
Ion 201.00 (200.70 to 201.70): E









#19
n-Nitroso-di-n-propylamine
Concen: 40.52 ng
RT: 9.07 min Scan# 1061
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35




Instrument :
BNA_G
ClientSampleId :
PB94345BSD

Tgt Ion:	70	Resp:	295002
Ion	Ratio	Lower	Upper
70	100		
42	67.5	56.1	84.1
101	10.7	7.5	11.3
130	18.8	14.6	21.8



#20
3+4-Methylphenols
Concen: 41.47 ng
RT: 9.03 min Scan# 1053
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Tgt Ion:	107	Resp:	375678
Ion	Ratio	Lower	Upper
107	100		
108	91.6	70.8	110.8
77	44.2	25.8	65.8
79	43.4	20.1	60.1





#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.10 min Scan# 1406

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35

Instrument :

BNA_G

ClientSampleId :

PB94345BSD

Tgt Ion:136 Resp: 454241


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 10.1 9.3 13.9

68 7.3 5.1 7.7






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



#22

Acetophenone

Concen: 40.81 ng

RT: 9.10 min Scan# 1065

Delta R.T. -0.00 min

Lab File: BG024528.D

Acq: 27 Oct 2016 19:35

Tgt Ion:105 Resp: 476157


Ion Ratio Lower Upper

105 100

71 0.9 0.9 1.3

51 38.5 34.0 51.0

120 21.7 17.3 25.9






Abundance Ion 105.00 (104.70 to 105.70): E

Ion 71.00 (70.70 to 71.70): BGC

Ion 51.00 (50.70 to 51.70): BGC

Ion 120.00 (119.70 to 120.70): E









#23
 Nitrobenzene-d5
 Concen: 88.28 ng
 RT: 9.45 min Scan# 1125
 Delta R.T. -0.00 min
 Lab File: BG024528.D
 Acq: 27 Oct 2016 19:35




Instrument :
 BNA_G
 ClientSampleId :
 PB94345BSD


Tgt Ion: 82 Resp: 880788
 Ion Ratio Lower Upper
 82 100
 128 35.6 26.4 39.6
 54 57.7 49.4 74.2



#24
 Nitrobenzene
 Concen: 39.56 ng
 RT: 9.49 min Scan# 1132
 Delta R.T. -0.00 min
 Lab File: BG024528.D
 Acq: 27 Oct 2016 19:35

Tgt Ion: 77 Resp: 439049
 Ion Ratio Lower Upper
 77 100
 123 32.3 26.1 39.1
 65 14.7 12.4 18.6









#25
Isophorone
Concen: 41.01 ng
RT: 10.01 min Scan# 1220
Delta R.T. 0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35




Instrument :
BNA_G
ClientSampleId :
PB94345BSD


Tgt Ion: 82 Resp: 761007
Ion Ratio Lower Upper
82 100
95 8.5 7.5 11.3
138 15.3 12.3 18.5



#26
2-Nitrophenol
Concen: 39.93 ng
RT: 10.20 min Scan# 1253
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Tgt Ion: 139 Resp: 164491
Ion Ratio Lower Upper
139 100
109 45.9 38.6 58.0
65 75.6 57.1 85.7









#27
2,4-Dimethylphenol
Concen: 44.05 ng
RT: 10.24 min Scan# 1260
Delta R.T. 0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Instrument :
BNA_G
ClientSampleId :
PB94345BSD

Tgt Ion	Ratio	Lower	Upper
122	100		
107	122.2	104.2	156.4
121	60.9	46.0	69.0



#28
bis(2-Chloroethoxy)methane
Concen: 43.27 ng
RT: 10.48 min Scan# 1301
Delta R.T. -0.00 min
Lab File: BG024528.D
Acq: 27 Oct 2016 19:35

Tgt Ion	Ratio	Lower	Upper
93	100		
95	33.3	25.7	38.5
123	10.9	8.3	12.5

