
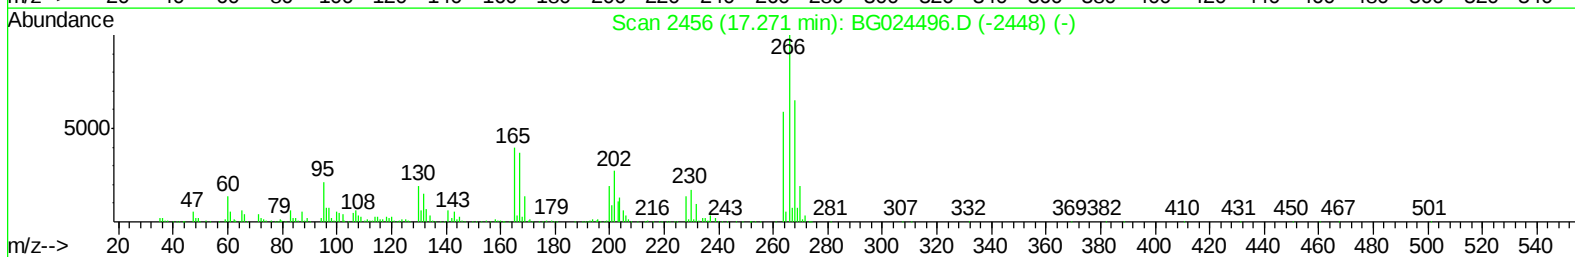
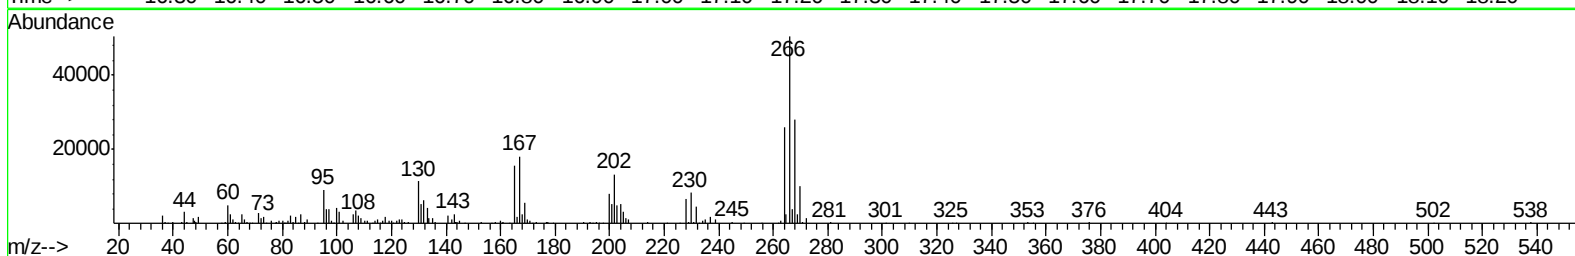


Data Path : Z:\HPCHEM1\BNA_G\Data\BG102716\
Data File : BG024520.D
Acq On : 27 Oct 2016 8:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 08:20:21 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

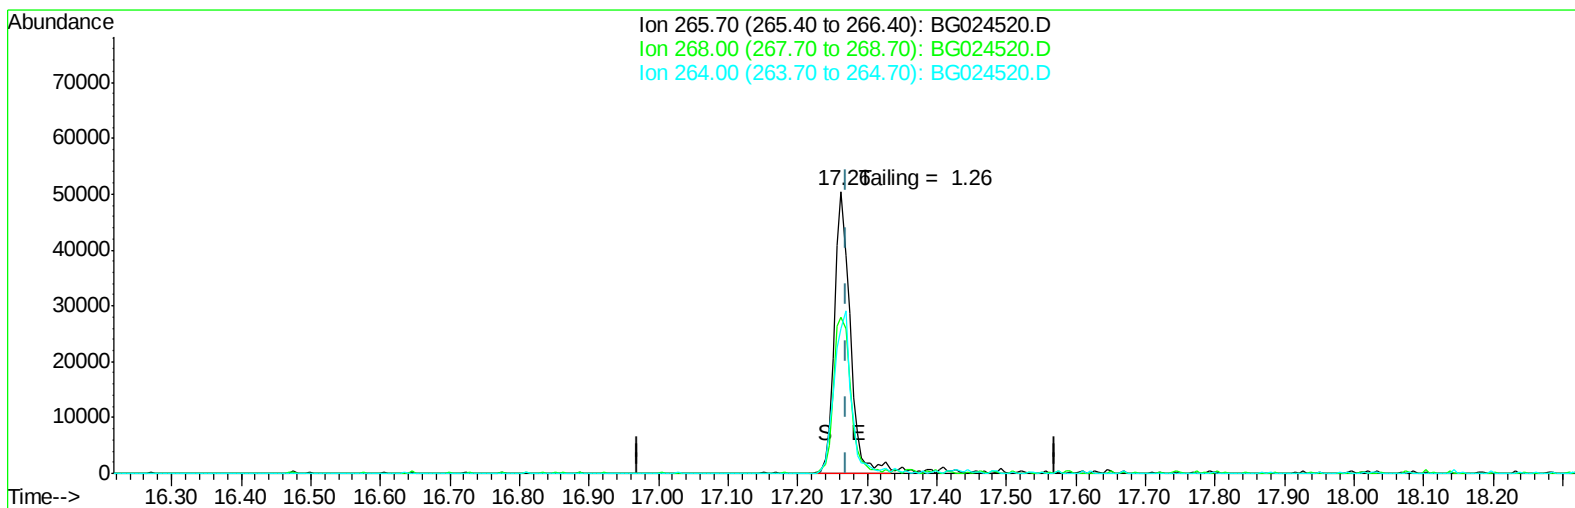

TIC: BG024520.D

(69) Pentachlorophenol (C)




17.263min (-0.008) 152636.41ng

response 77009

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	55.62
264.00	62.60	51.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG102716\
Data File : BG024520.D
Acq On : 27 Oct 2016 8:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 08:20:21 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

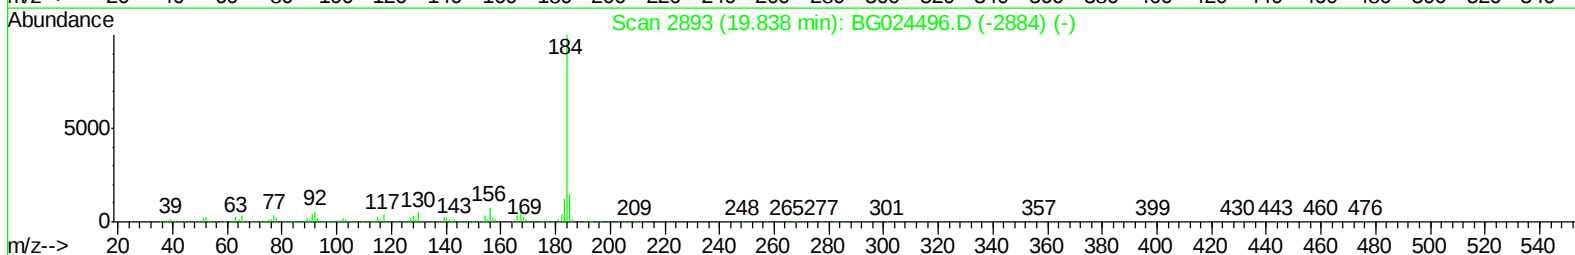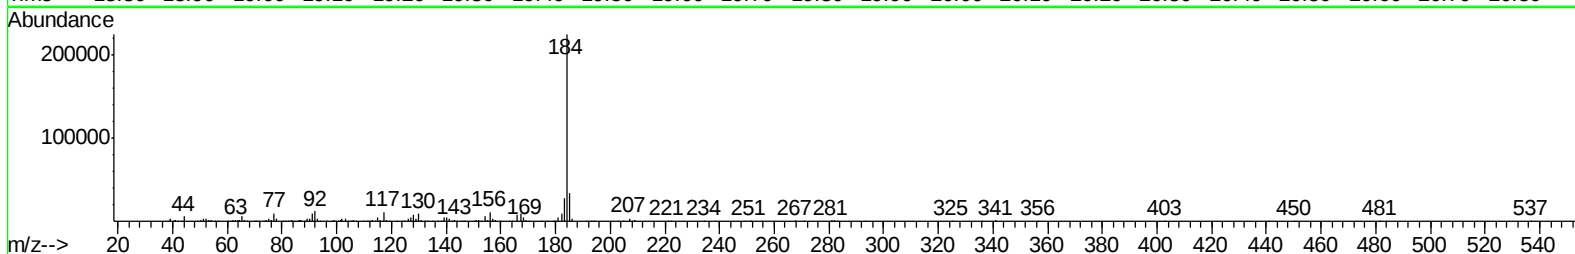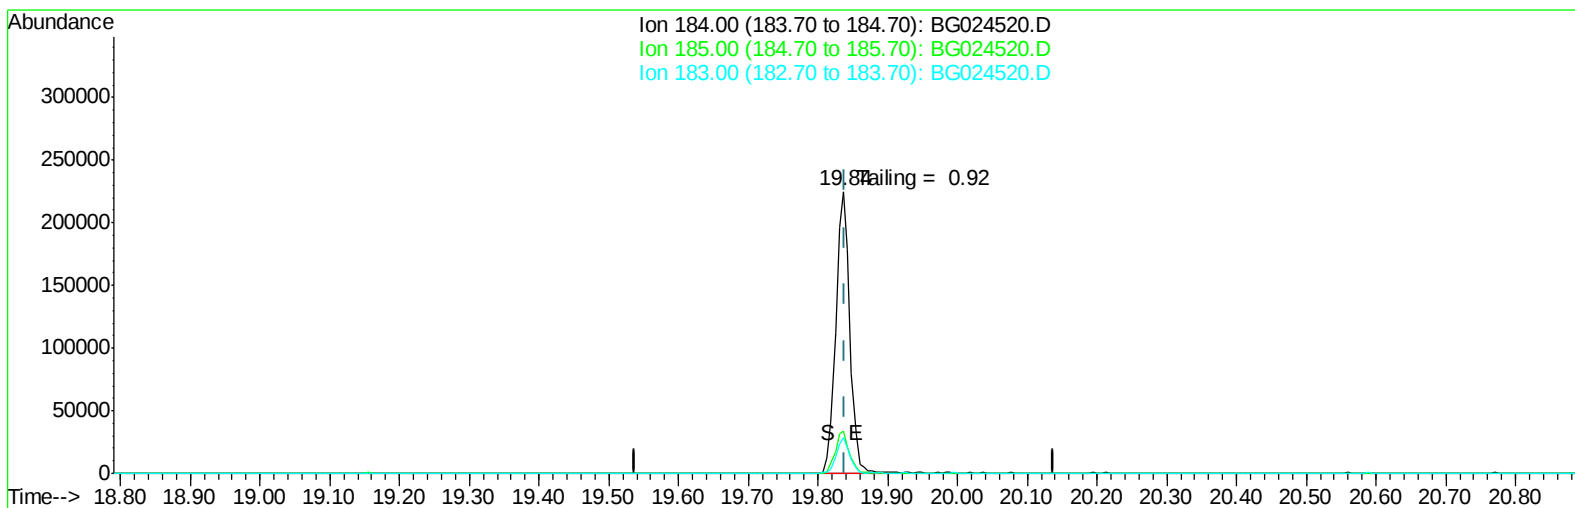

TIC: BG024520.D

(76) Benzidine

19.836min (-0.002) 46925.92ng

response 316210

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.11
183.00	13.80	12.58
0.00	0.00	0.00