
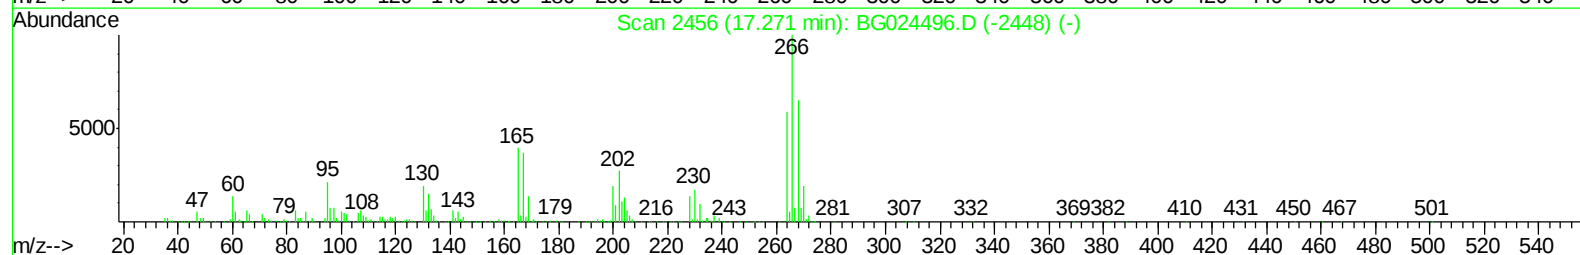
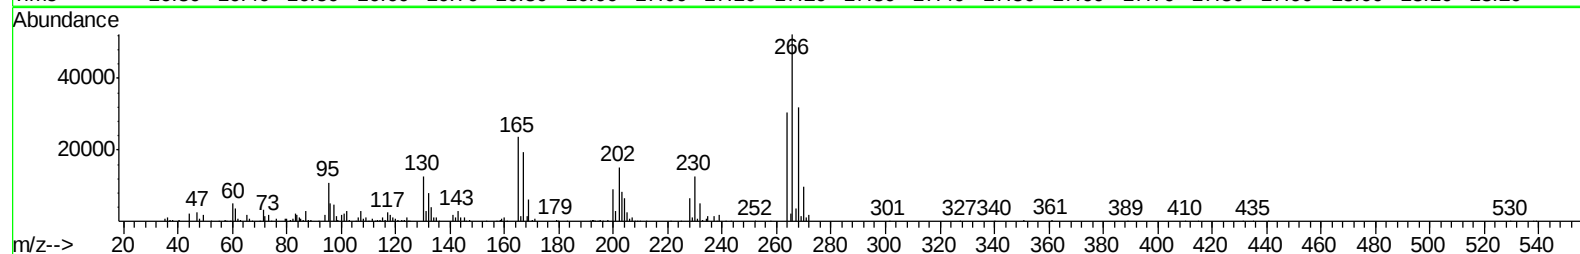


Data Path : Z:\HPCHEM1\BNA_G\Data\BG102716\
Data File : BG024524.D
Acq On : 27 Oct 2016 15:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 08:21:05 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

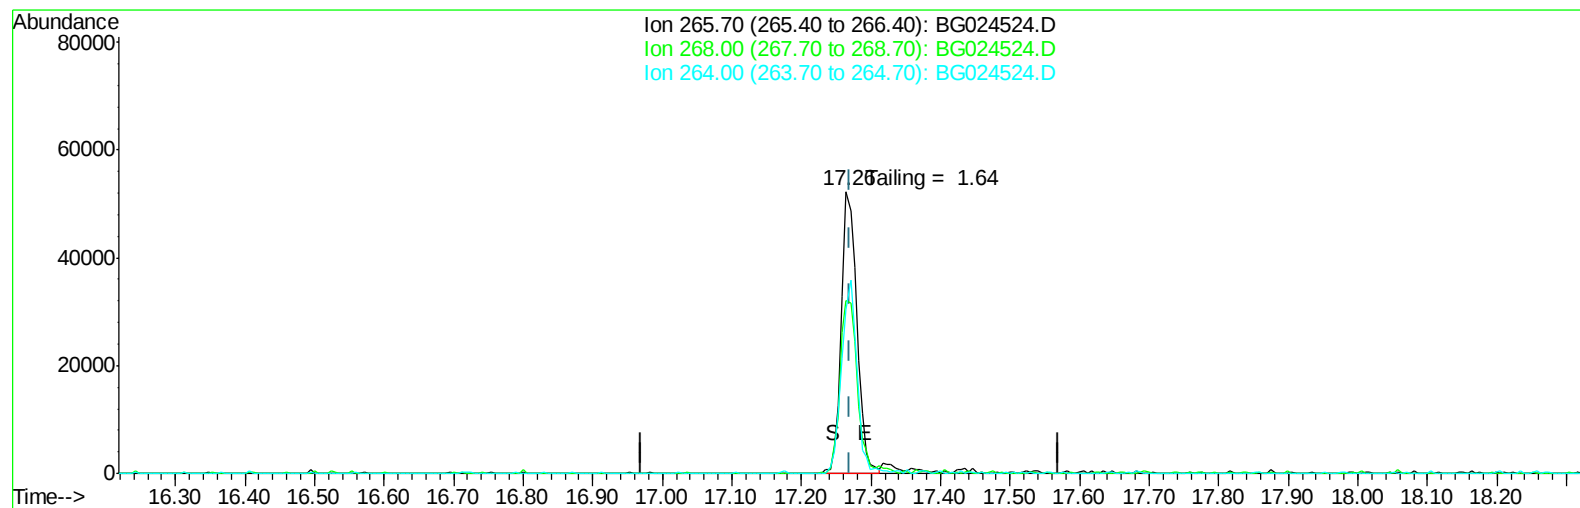

TIC: BG024524.D

(69) Pentachlorophenol (C)




17.264min (-0.006) 106586.28ng

response 81135

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	61.40
264.00	62.60	58.32
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_G\Data\BG102716\  
Data File : BG024524.D  
Acq On    : 27 Oct 2016  15:18  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Oct 28 08:21:05 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

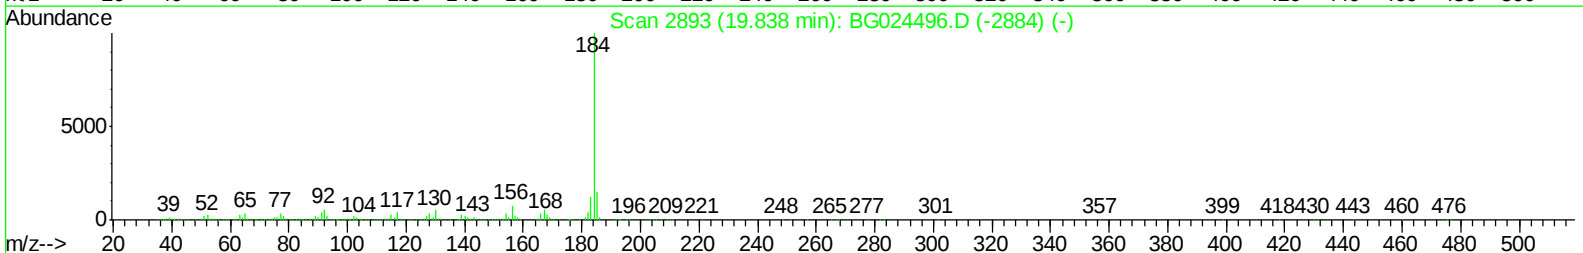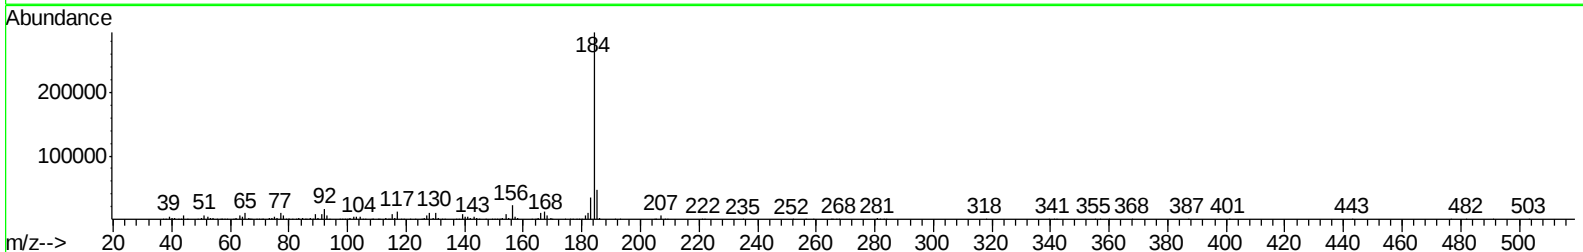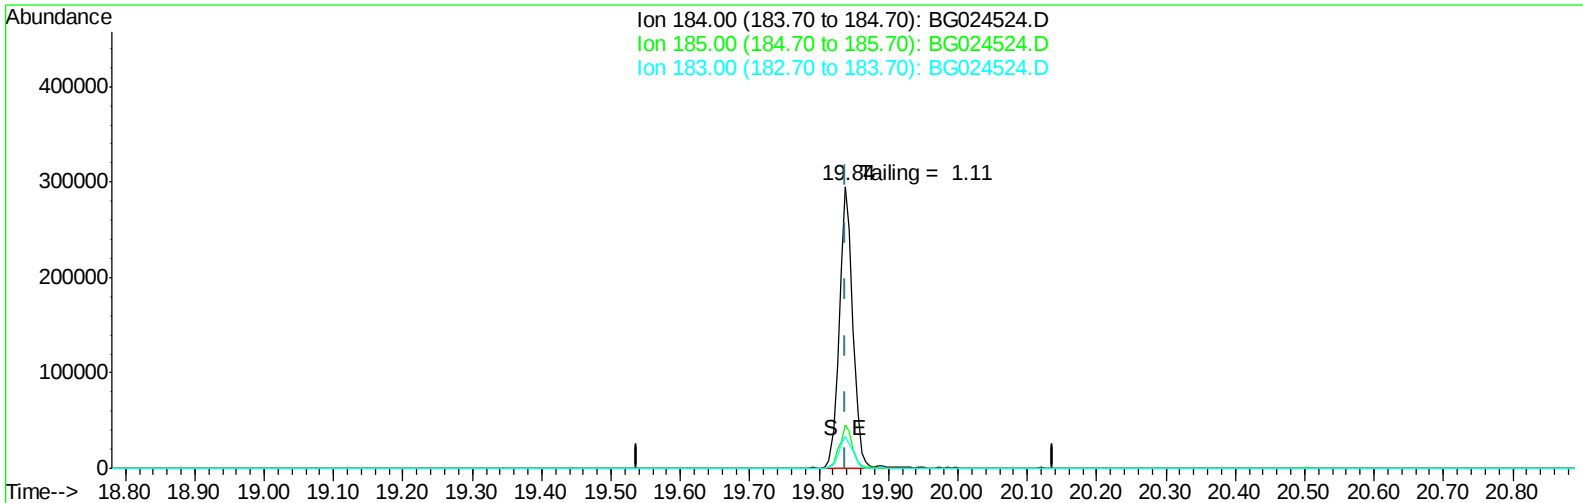

TIC: BG024524.D

(76) Benzidine

19.838min (-0.001) 53405.50ng

response 403913

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.67
183.00	13.80	11.41
0.00	0.00	0.00