


Data Path : Z:\HPCHEM1\BNA_G\Data\BG102716\
 Data File : BG024520.D
 Acq On : 27 Oct 2016 8:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

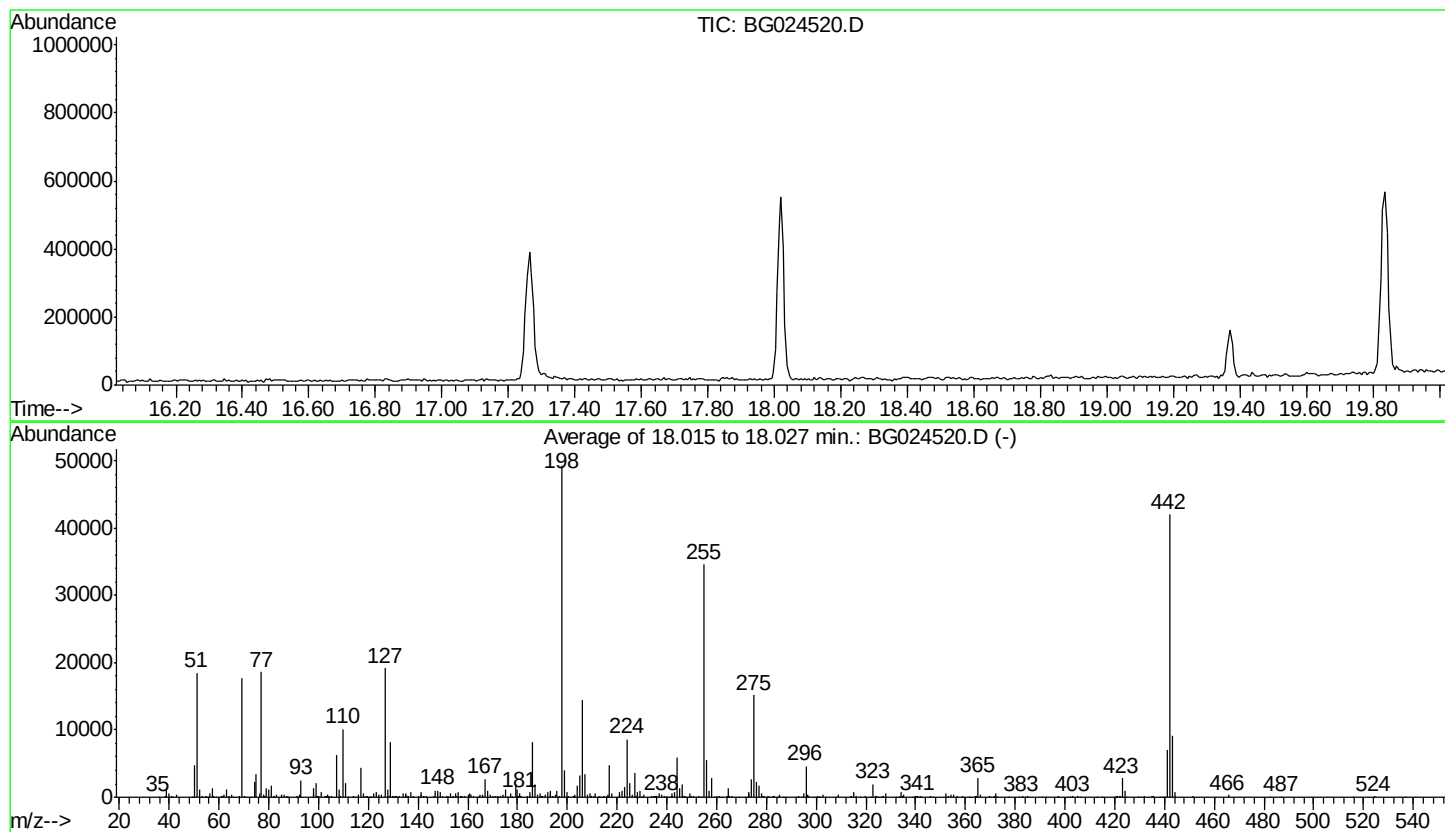

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	18489	PASS
68	69	0.00	2	1.1	195	PASS
69	198	0.00	100	35.8	17643	PASS
70	69	0.00	2	0.6	102	PASS
127	198	10	80	38.9	19174	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49274	PASS
199	198	5	9	8.1	4008	PASS
275	198	10	60	30.8	15175	PASS
365	198	1	100	6.0	2948	PASS
441	442	0.01	24	17.0	7132	PASS
442	198	50	100	85.3	42032	PASS
443	442	15	24	21.9	9184	PASS