


Data Path : Z:\HPCHEM1\BNA_G\Data\BG102716\
 Data File : BG024524.D
 Acq On : 27 Oct 2016 15:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

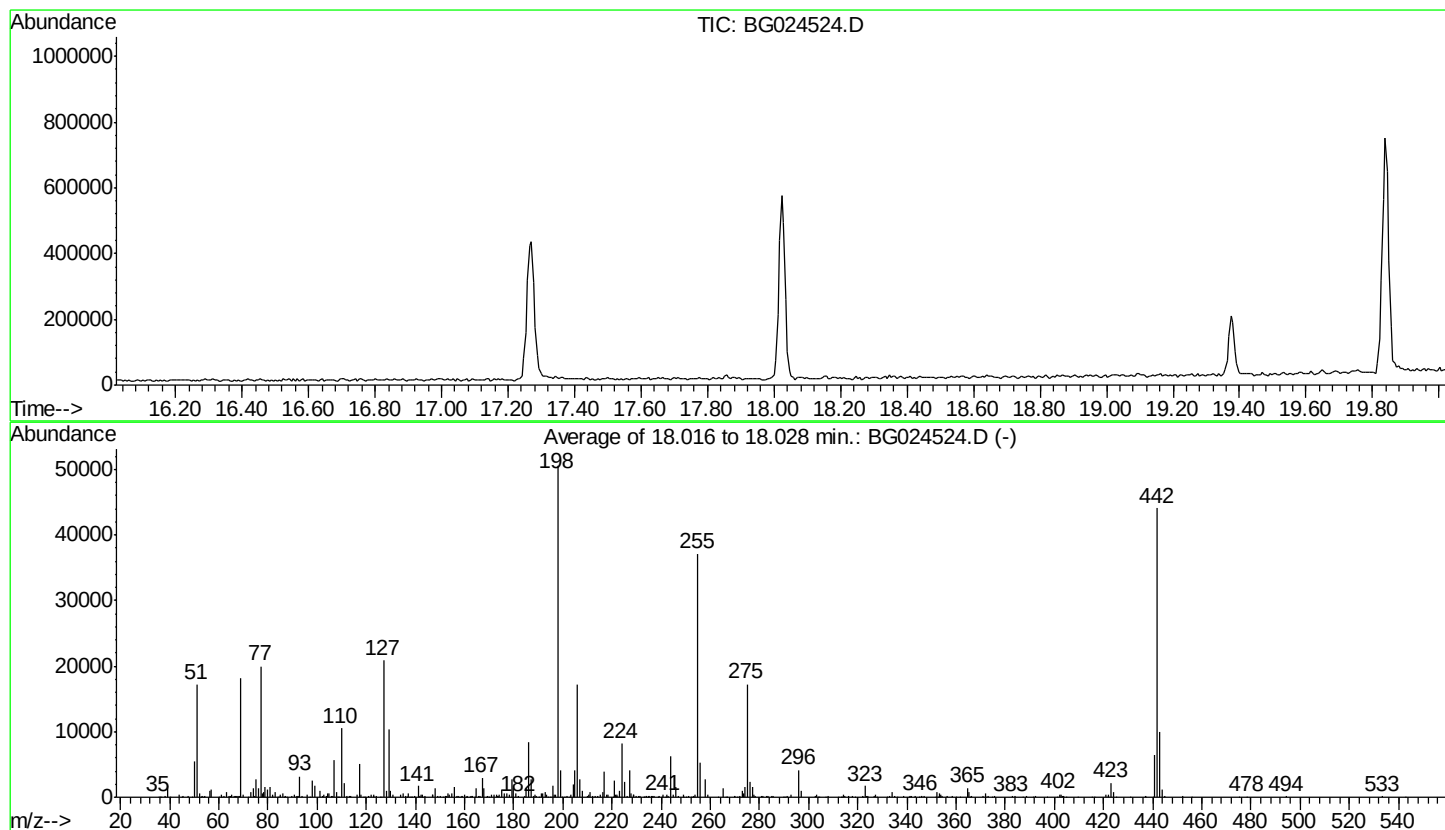

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	17177	PASS
68	69	0.00	2	0.8	155	PASS
69	198	0.00	100	36.1	18242	PASS
70	69	0.00	2	1.9	345	PASS
127	198	10	80	41.3	20866	PASS
197	198	0.00	2	0.9	480	PASS
198	198	100	100	100.0	50562	PASS
199	198	5	9	8.2	4122	PASS
275	198	10	60	34.1	17242	PASS
365	198	1	100	2.8	1415	PASS
441	442	0.01	24	14.7	6495	PASS
442	198	50	100	87.1	44050	PASS
443	442	15	24	22.6	9935	PASS