

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102717\
 Data File : BG030497.D
 Acq On : 27 Oct 2017 14:47
 Operator : SJ/JU
 Sample : I6024-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-12-COMP

Quant Time: Oct 27 16:16:07 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 17:32:15 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	63009	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	303052	20.00	ng	0.00
38) Acenaphthene-d10	14.79	164	196211	20.00	ng	0.00
63) Phenanthrene-d10	17.52	188	460913	20.00	ng	0.00
75) Chrysene-d12	21.80	240	487327	20.00	ng	0.00
86) Perylene-d12	25.11	264	483252	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	426297	113.02	ng	0.00
7) Phenol-d6	7.32	99	582419	110.01	ng	0.00
23) Nitrobenzene-d5	9.33	82	351612	73.73	ng	0.00
41) 2,4,6-Tribromophenol	16.27	330	278799	110.05	ng	0.00
44) 2-Fluorobiphenyl	13.41	172	963097	71.99	ng	0.00
78) Terphenyl-d14	20.12	244	1457459	68.04	ng	0.00
Target Compounds						
10) Phenol	7.35	94	14999	2.628	ng	Qvalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102717\
Data File : BG030497.D
Acq On : 27 Oct 2017 14:47
Operator : SJ/JU
Sample : I6024-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-12-COMP

Quant Time: Oct 27 16:16:07 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

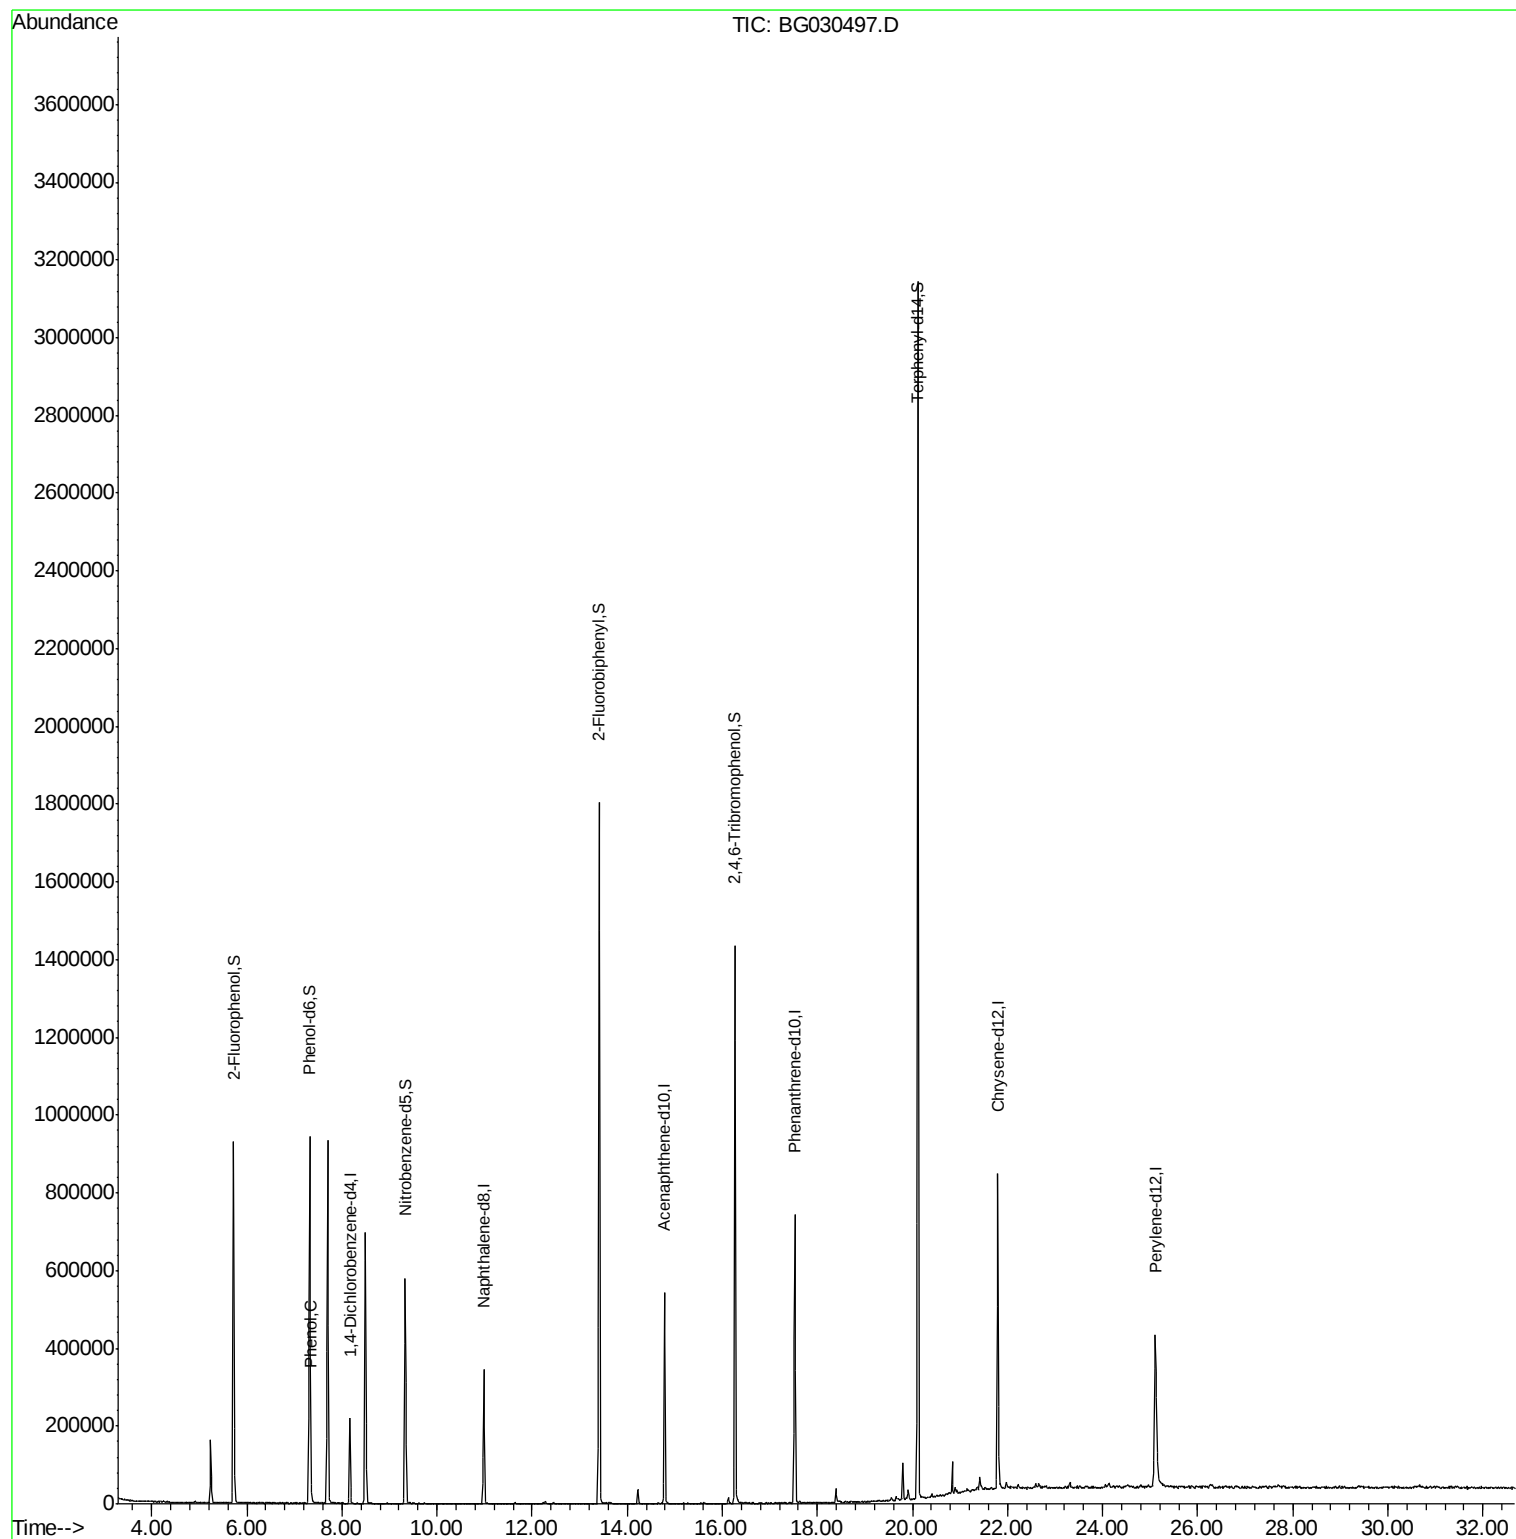




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 831
Delta R.T. -0.00 min
Lab File: BG030497.D
Acq: 27 Oct 2017 14:47

Instrument :
BNA_G
ClientSampleId :
SB-12-COMP

Tot Ion:152 Resp: 63009
Ion Ratio Lower Upper
152 100
150 156.2 126.6 189.8
115 58.9 53.0 79.4

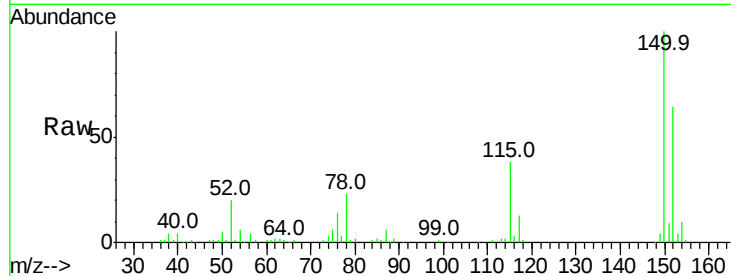


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

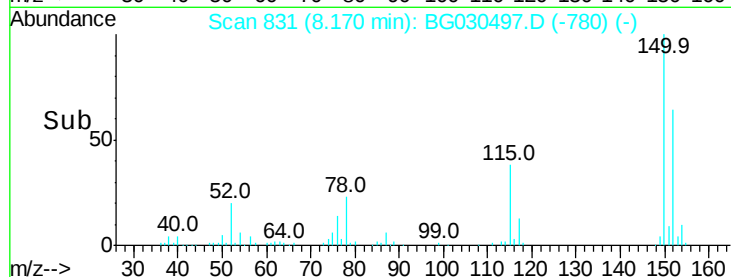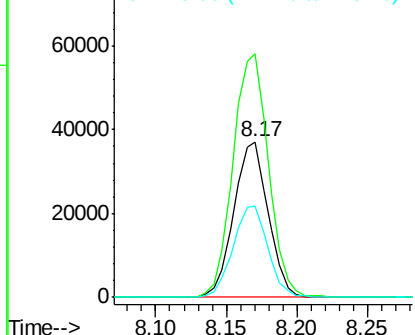



#5


2-Fluorophenol
Concen: 113.024 ng
RT: 5.72 min Scan# 414
Delta R.T. 0.00 min
Lab File: BG030497.D
Acq: 27 Oct 2017 14:47

Tgt Ion:112 Resp: 426297
Ion Ratio Lower Upper
112 100
64 59.0 56.3 84.5
63 30.6 30.1 45.1

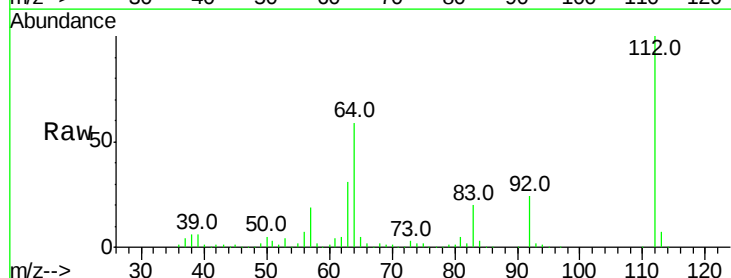

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

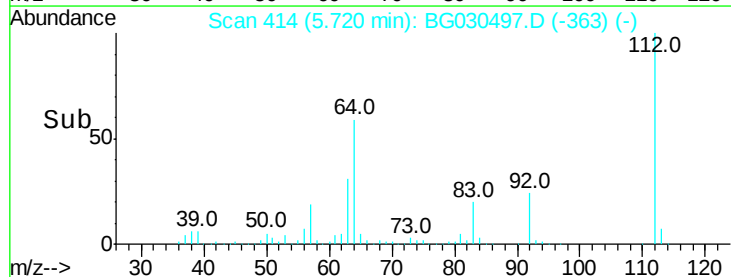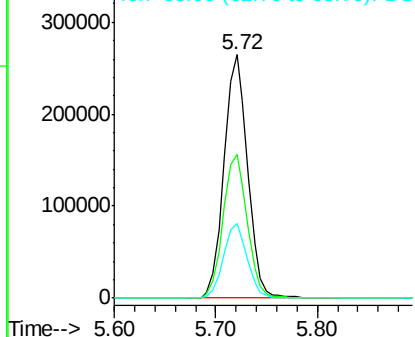

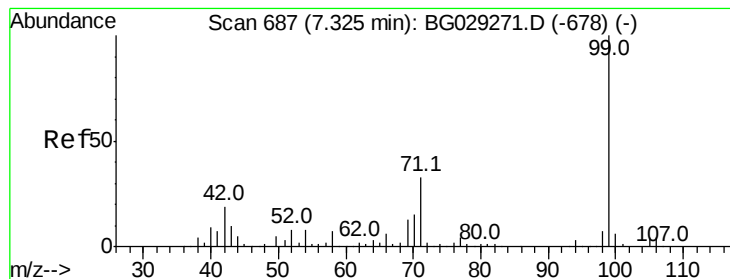

#7

Phenol-d6

Concen: 110.010 ng

RT: 7.32 min Scan# 686

Delta R.T. -0.01 min

Lab File: BG030497.D

Acq: 27 Oct 2017 14:47

Instrument :

BNA_G

ClientSampleId :

SB-12-COMP


Tot Ion: 99 Resp: 582419

Ion Ratio Lower Upper




99 100

42 19.6 14.1 21.1

71 34.2 26.1 39.1

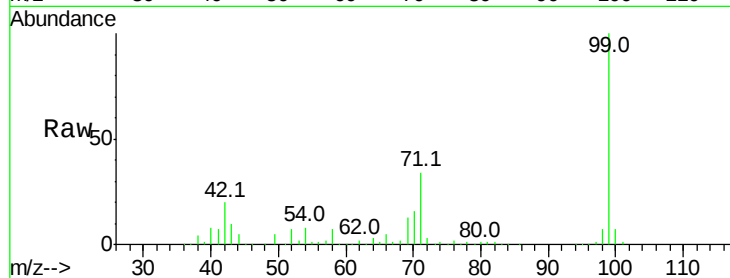

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

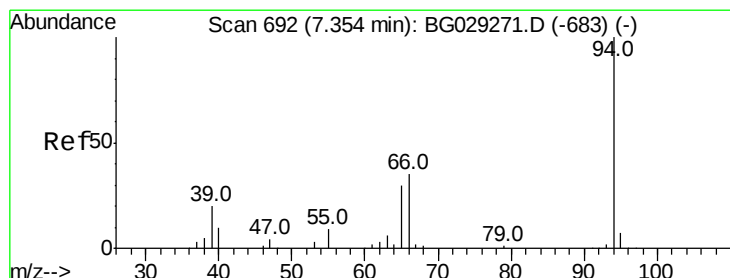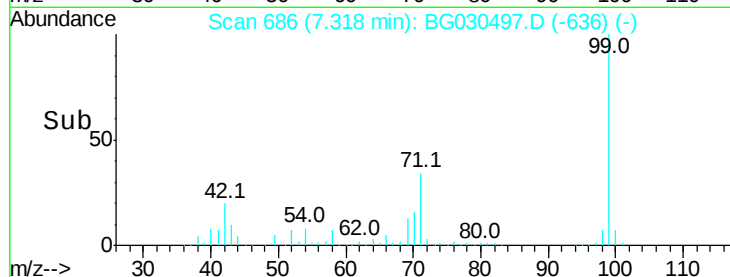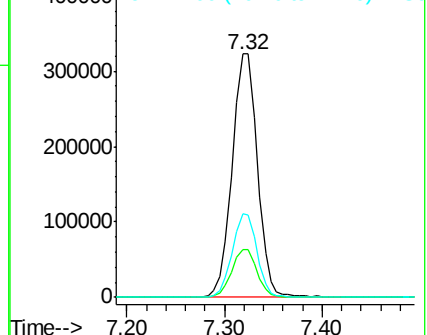

#10

Phenol

Concen: 2.628 ng

RT: 7.35 min Scan# 691

Delta R.T. -0.01 min

Lab File: BG030497.D

Acq: 27 Oct 2017 14:47


Tgt Ion: 94 Resp: 14999

Ion Ratio Lower Upper



94 100

65 28.7 11.9 51.9

66 52.6 22.2 62.2

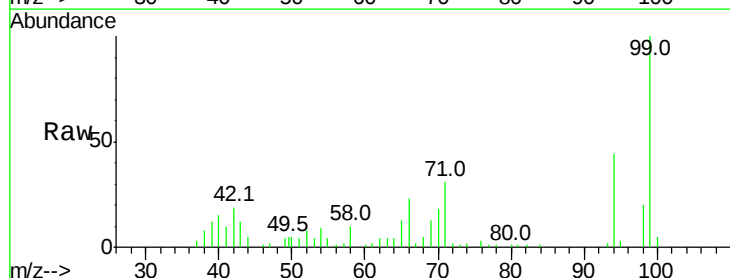

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

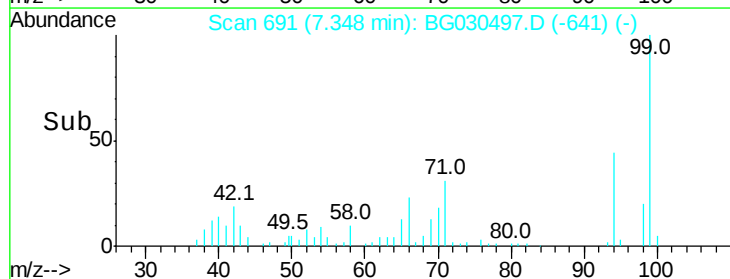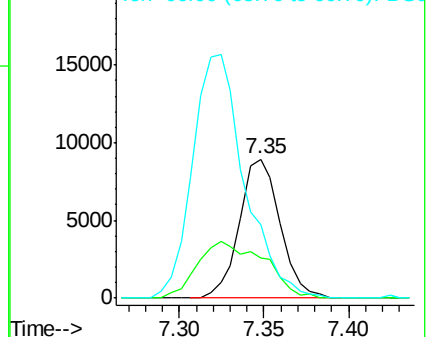







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.98 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BG030497.D
Acq: 27 Oct 2017 14:47

Instrument :
BNA_G
ClientSampleId :
SB-12-COMP

Tot Ion:	136	Resp:	303052
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.2	13.8
54	8.0	10.3	15.5#
68	5.8	4.5	6.7

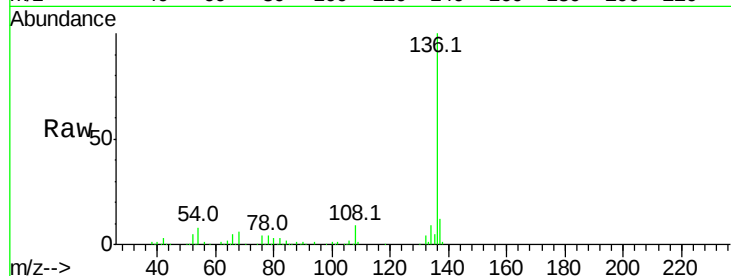


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

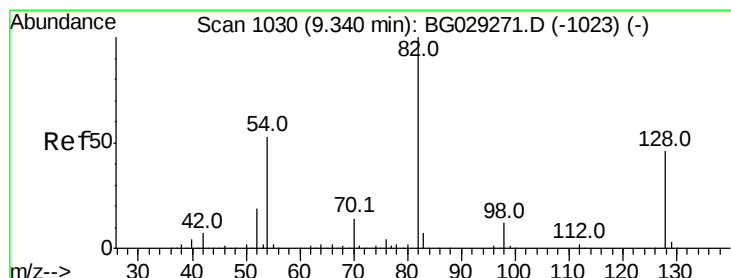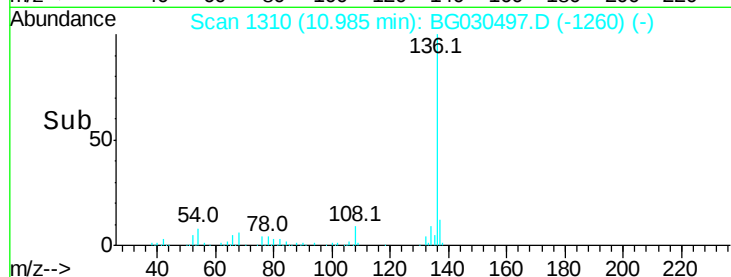
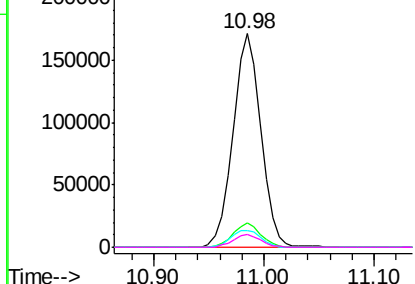


#23
Nitrobenzene-d5
Concen: 73.730 ng
RT: 9.33 min Scan# 1029
Delta R.T. -0.01 min
Lab File: BG030497.D
Acq: 27 Oct 2017 14:47

Tgt Ion:	82	Resp:	351612
Ion	Ratio	Lower	Upper
82	100		
128	44.9	29.7	44.5#
54	54.2	43.1	64.7

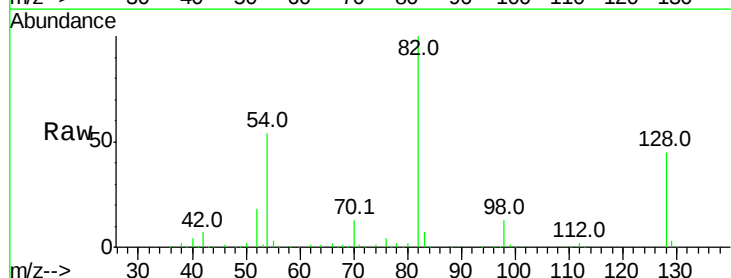

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

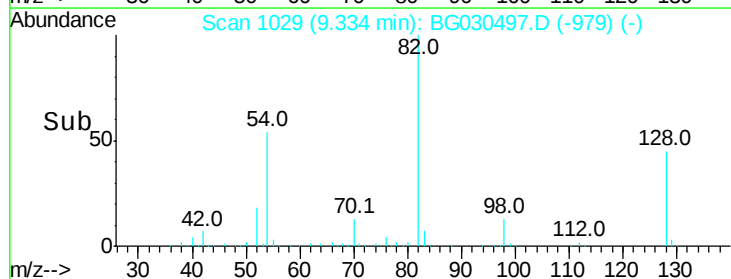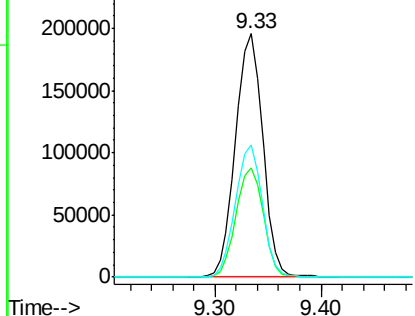



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.79 min Scan# 1957

Delta R.T. -0.01 min

Lab File: BG030497.D

Acq: 27 Oct 2017 14:47

Instrument :

BNA_G

ClientSampleId :

SB-12-COMP


Tot Ion:164 Resp: 196211

Ion Ratio Lower Upper

164 100

162 104.4 78.8 118.2




160 47.5 35.4 53.0

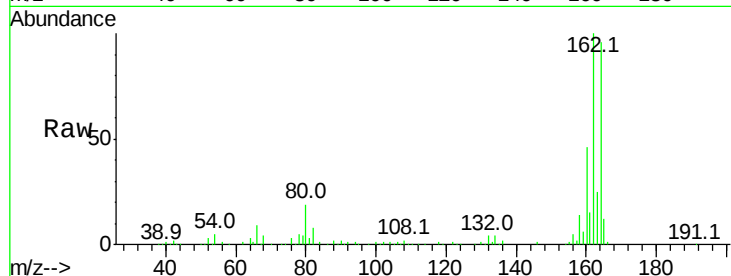

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

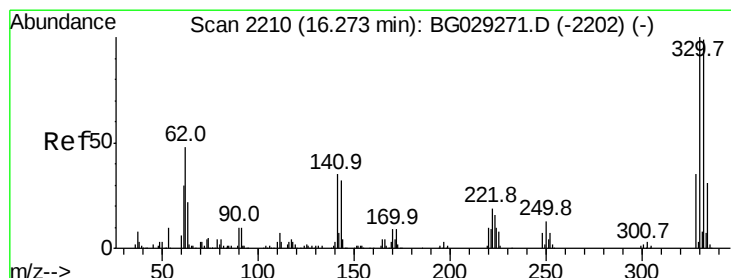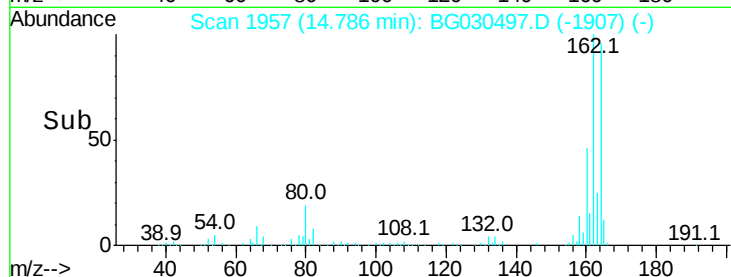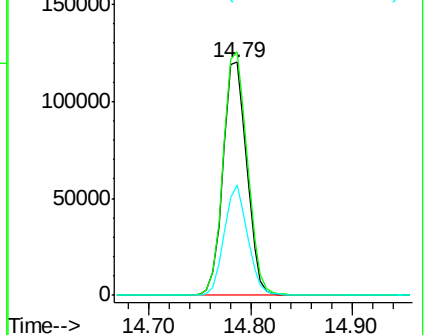

#41

2,4,6-Tribromophenol

Concen: 110.054 ng

RT: 16.27 min Scan# 2209

Delta R.T. -0.01 min

Lab File: BG030497.D

Acq: 27 Oct 2017 14:47


Tgt Ion:330 Resp: 278799

Ion Ratio Lower Upper

330 100

332 96.9 77.0 115.6



141 34.2 25.2 37.8

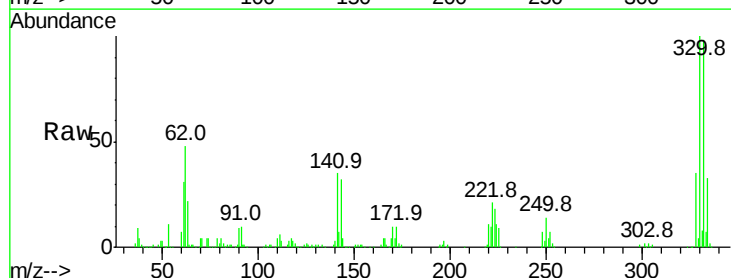

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



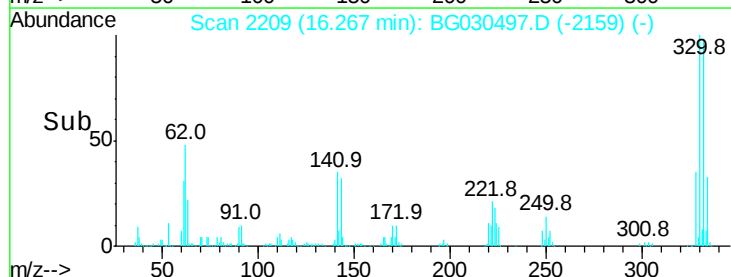
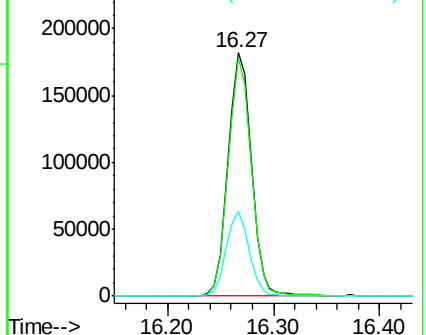




#44
 2-Fluorobiphenyl
 Concen: 71.990 ng
 RT: 13.41 min Scan# 1723
 Delta R.T. -0.01 min
 Lab File: BG030497.D
 Acq: 27 Oct 2017 14:47




Instrument :
 BNA_G
 ClientSampleId :
 SB-12-COMP


Tot Ion	Ratio	Lower	Upper
172	100		
171	37.3	30.0	45.0
170	24.5	19.5	29.3

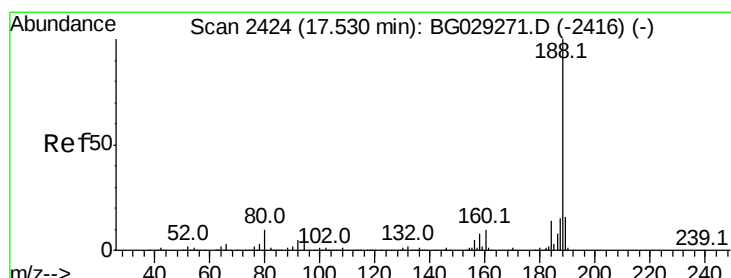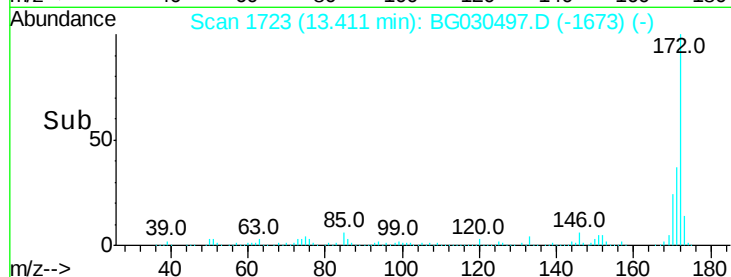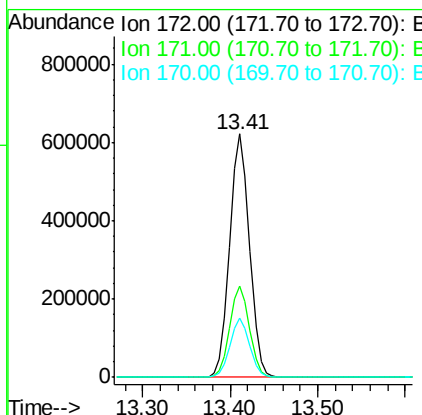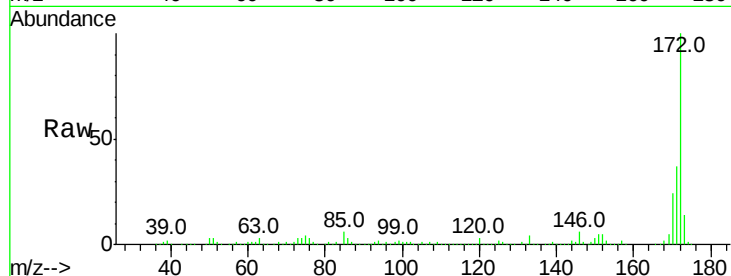

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.52 min Scan# 2423
 Delta R.T. -0.01 min
 Lab File: BG030497.D
 Acq: 27 Oct 2017 14:47

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.6	6.9	10.3
80	8.8	7.7	11.5

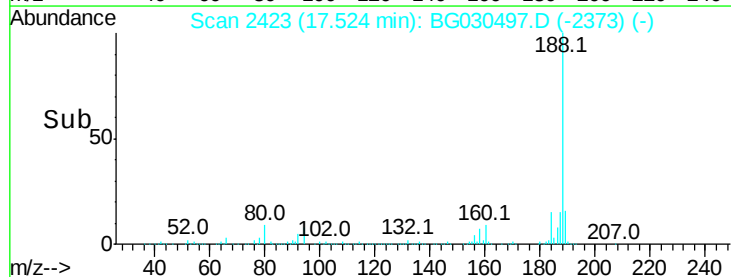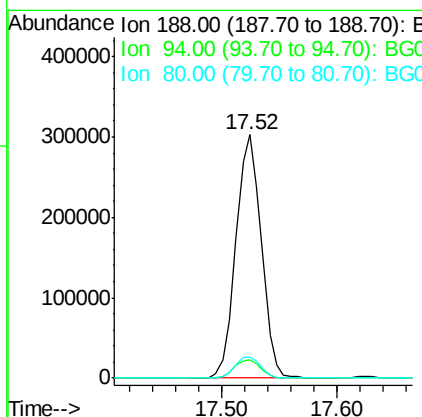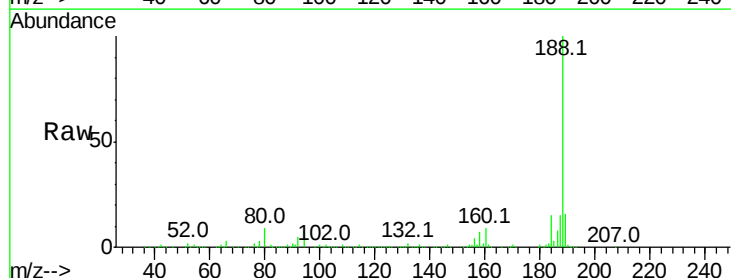

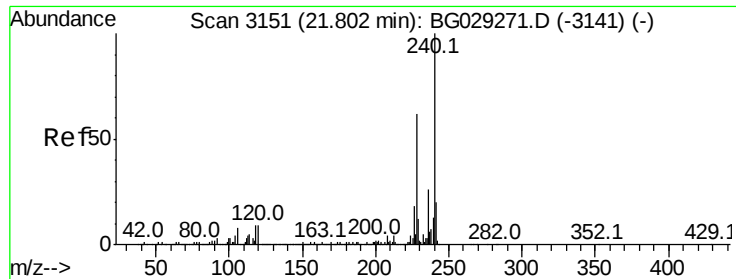

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.80 min Scan# 3150

Delta R.T. -0.01 min

Lab File: BG030497.D

Acq: 27 Oct 2017 14:47

Instrument :

BNA_G

ClientSampleId :

SB-12-COMP


Tot Ion:240 Resp: 487327

Ion Ratio Lower Upper

240 100

120 8.9 6.8 10.2




236 26.2 20.9 31.3

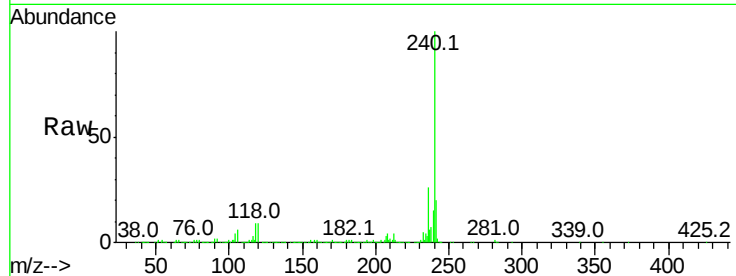

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

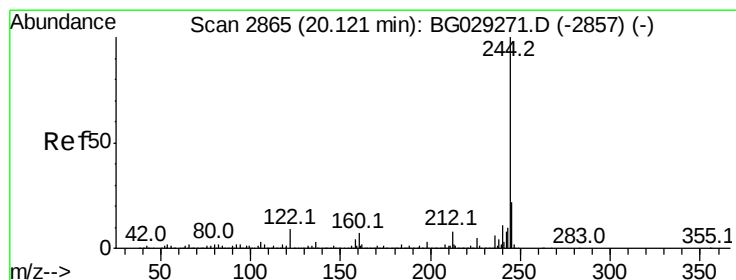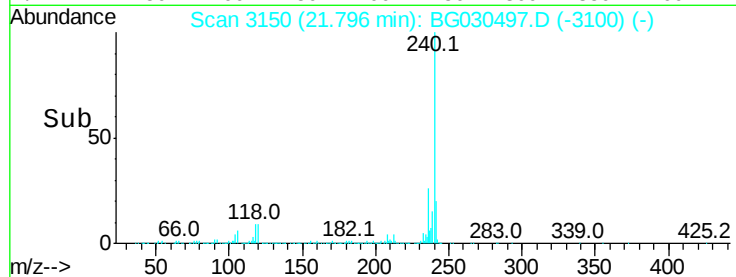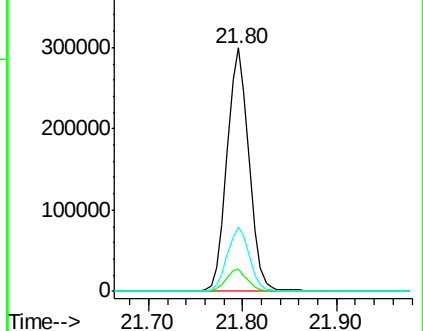

#78

Terphenyl-d14

Concen: 68.037 ng

RT: 20.12 min Scan# 2864

Delta R.T. -0.01 min

Lab File: BG030497.D

Acq: 27 Oct 2017 14:47


Tgt Ion:244 Resp: 1457459

Ion Ratio Lower Upper

244 100

212 7.9 5.8 8.8



122 9.3 7.0 10.4

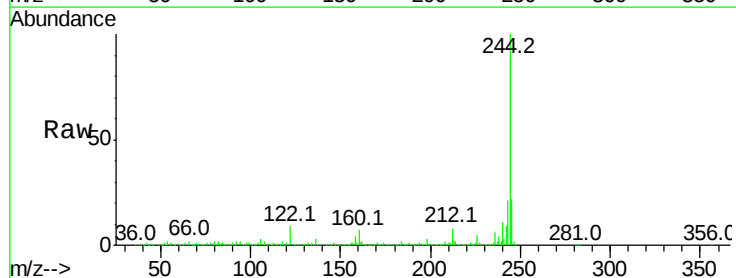


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

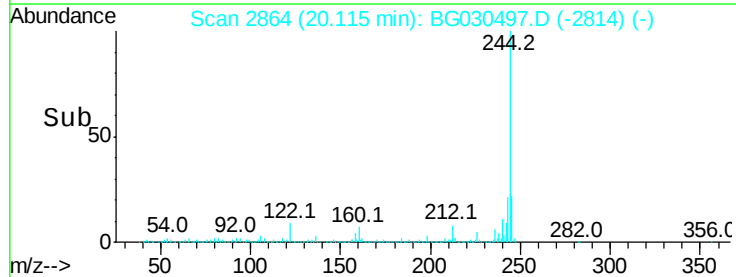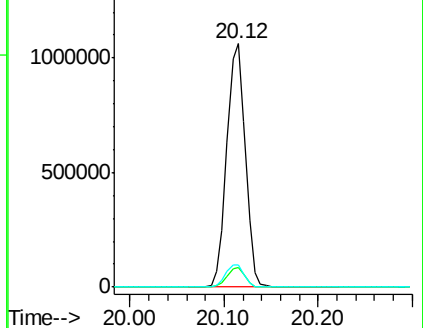


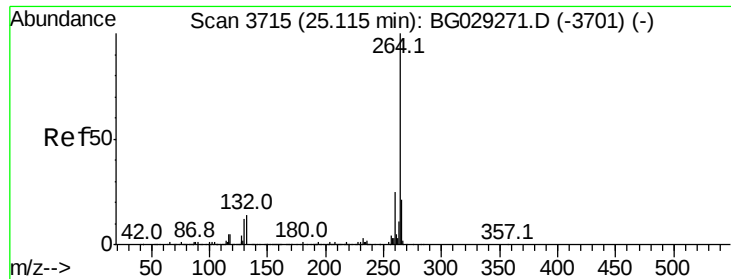

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.11 min Scan# 3714
 Delta R.T. -0.01 min
 Lab File: BG030497.D
 Acq: 27 Oct 2017 14:47

Instrument :
 BNA_G
 ClientSampleId :
 SB-12-COMP

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.8	17.4	26.0
265	21.3	17.7	26.5

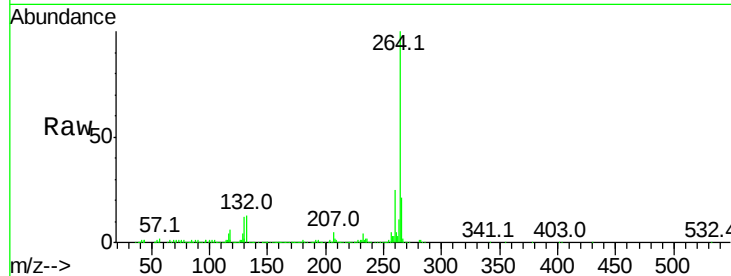

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

