
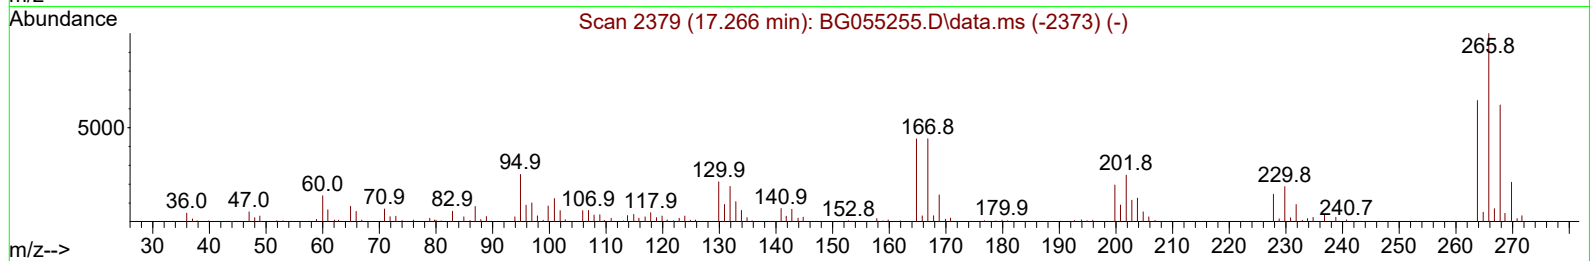
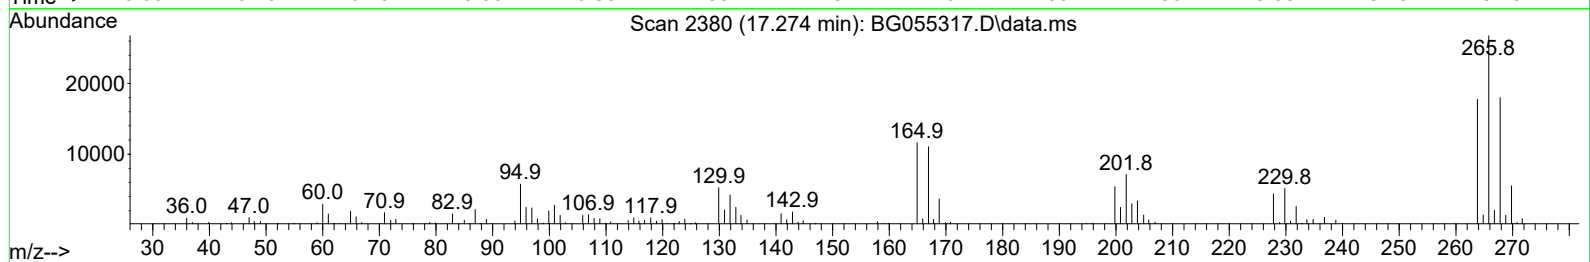


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102722\  
Data File : BG055317.D  
Acq On : 27 Oct 2022 10:12  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 06:40:30 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Oct 24 16:54:05 2022  
Response via : Initial Calibration

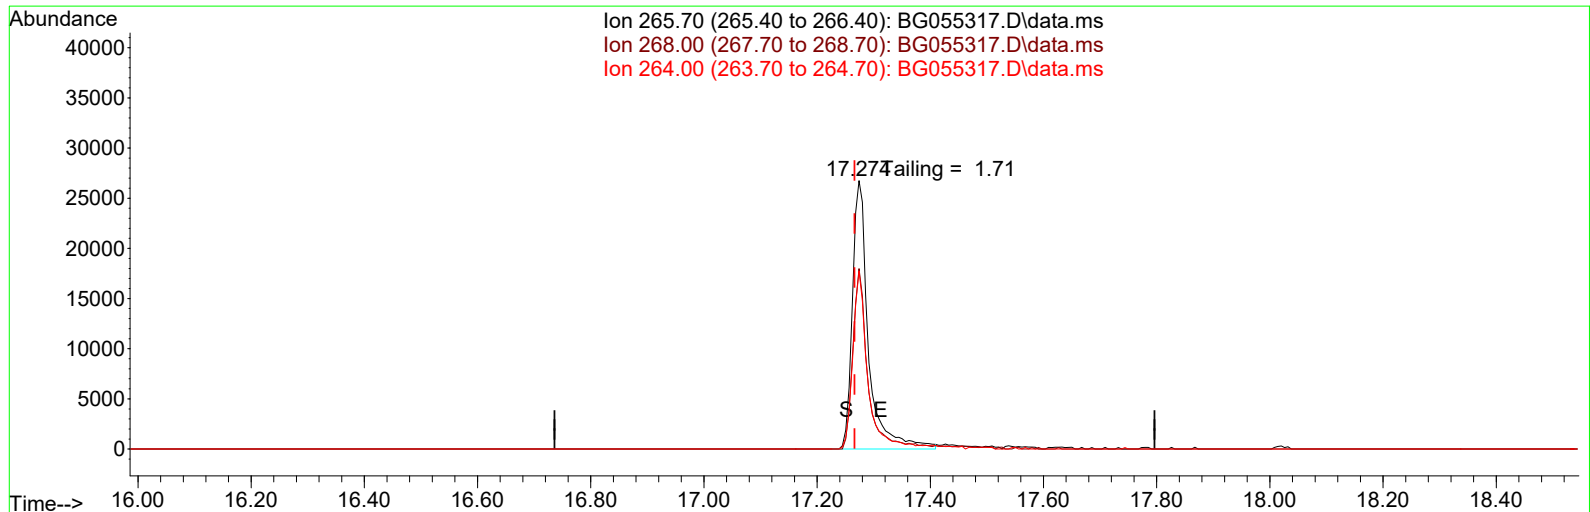

TIC: BG055317.D\data.ms

**(70) Pentachlorophenol (C)**




**17.274min (+ 0.008) 42439.09 ng**

**response 53312**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.50  | 67.22  |
| 264.00 | 64.40  | 66.33  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102722\  
Data File : BG055317.D  
Acq On : 27 Oct 2022 10:12  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 06:40:30 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG102422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Oct 24 16:54:05 2022  
Response via : Initial Calibration

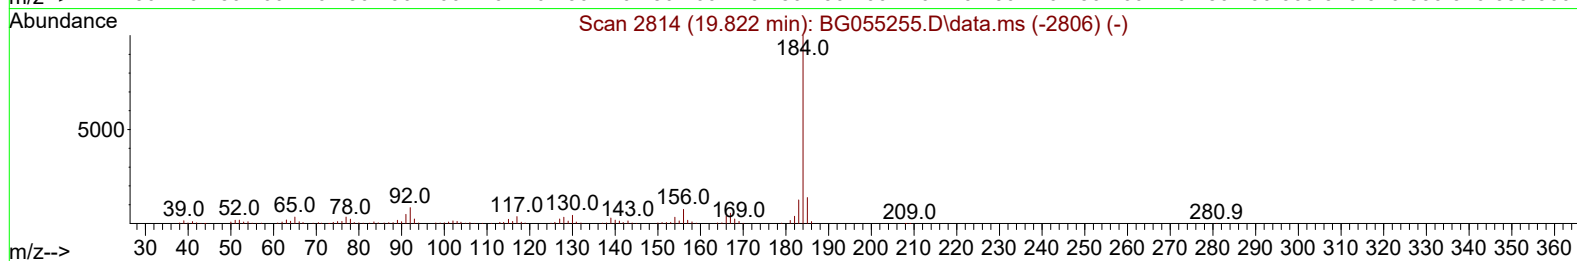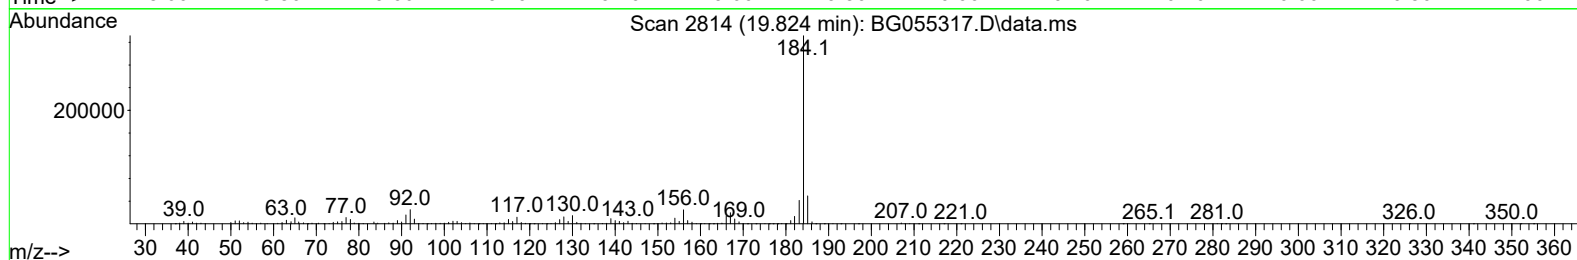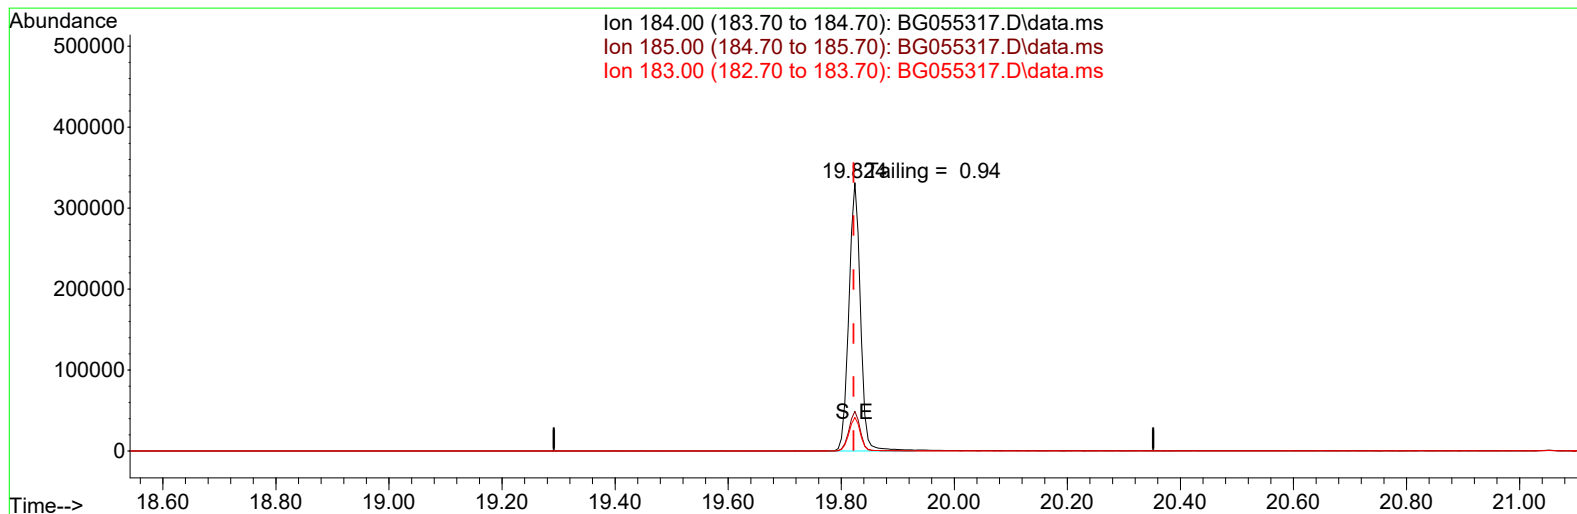

TIC: BG055317.D\data.ms

**(77) Benzidine****19.824min (+ 0.002) 171482.53 ng****response 473337**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.82  |
| 183.00 | 12.50  | 12.51  |
| 0.00   | 0.00   | 0.00   |