


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102722\
 Data File : BG055317.D
 Acq On : 27 Oct 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 24 16:54:05 2022

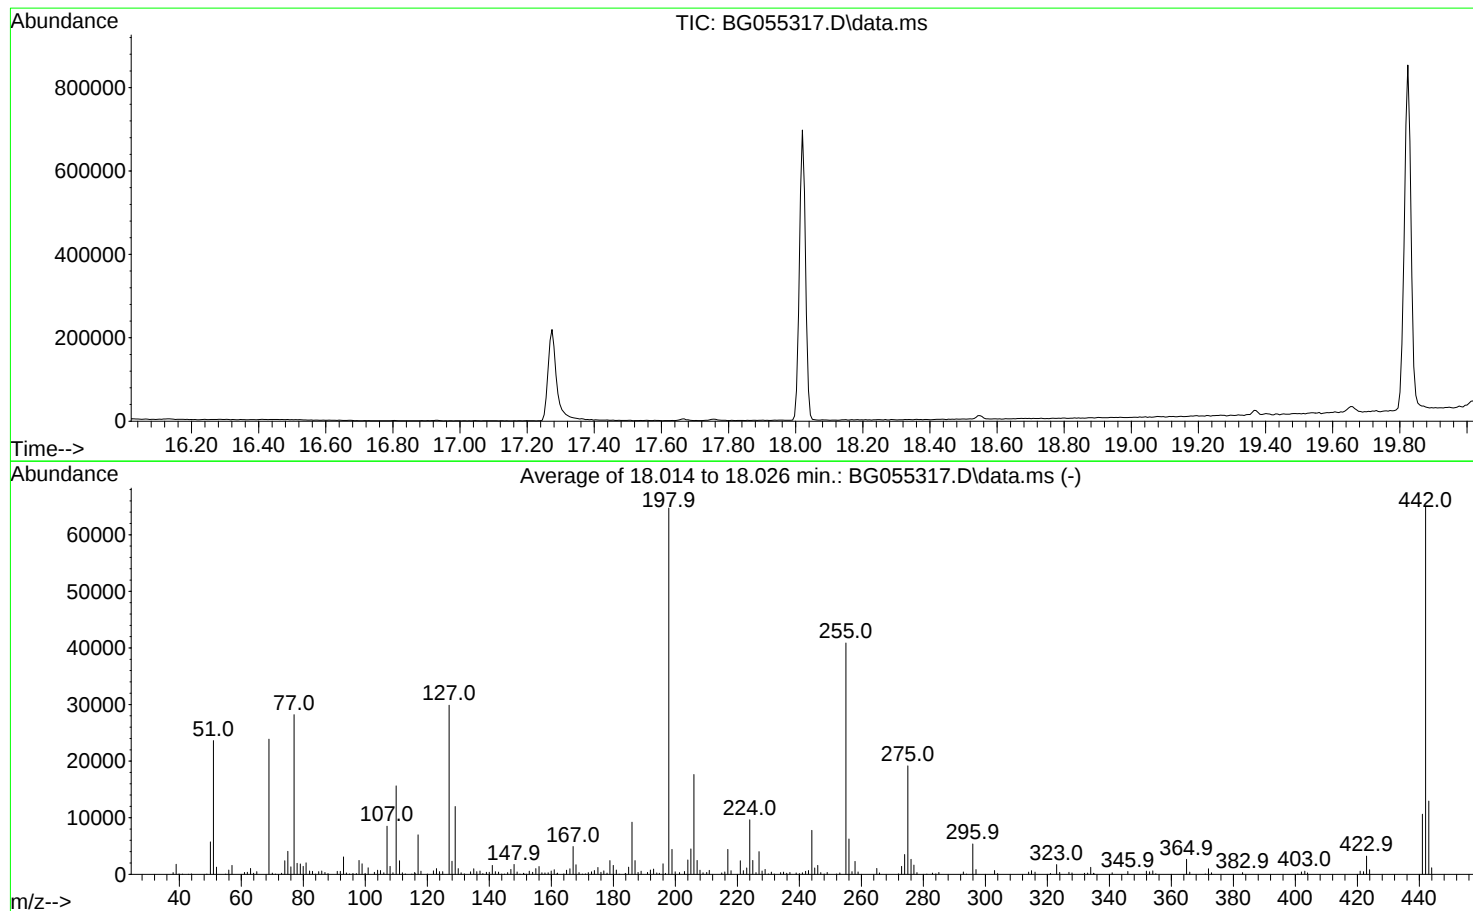




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	23629	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.9	23880	PASS
70	69	0.00	2	0.9	225	PASS
127	198	10	80	46.1	29867	PASS
197	198	0.00	2	0.3	167	PASS
198	198	100	100	100.0	64728	PASS
199	198	5	9	6.8	4390	PASS
275	198	10	60	29.6	19165	PASS
365	198	1	100	4.1	2636	PASS
441	198	0.01	100	16.4	10619	PASS
442	442	50	100	100.0	65013	PASS
443	442	15	24	19.9	12944	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102722\
Data File : BG055317.D
Acq On : 27 Oct 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 28 06:40:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

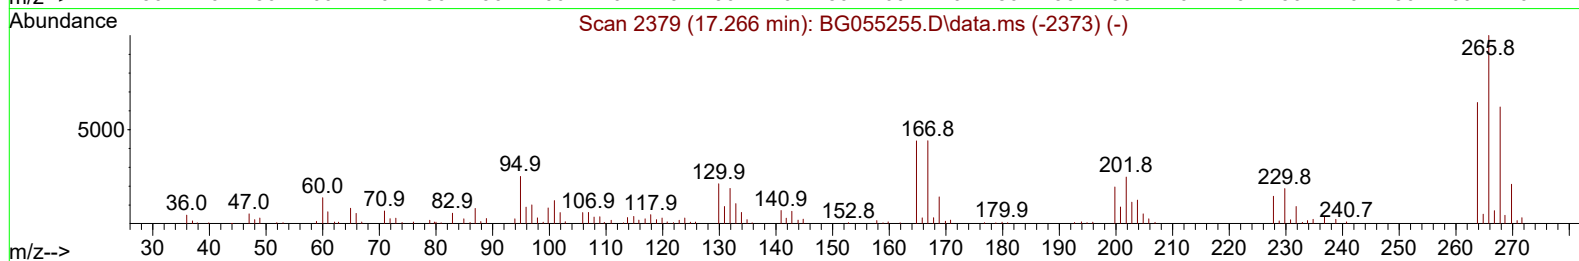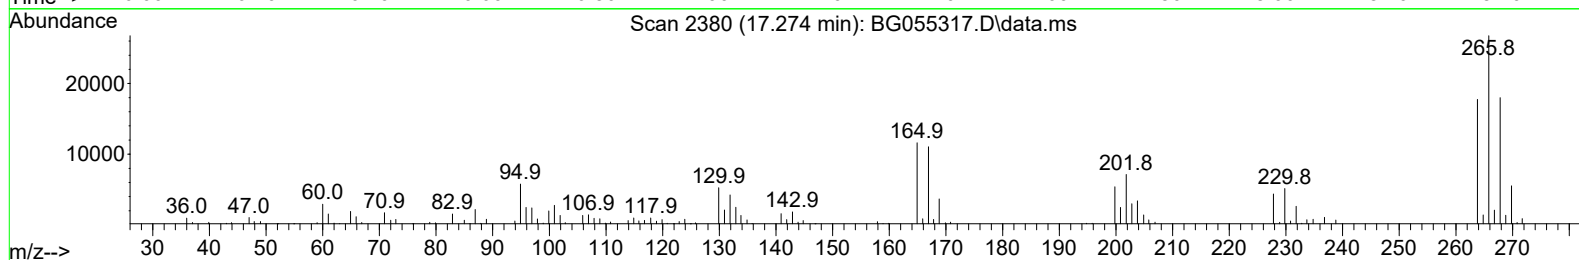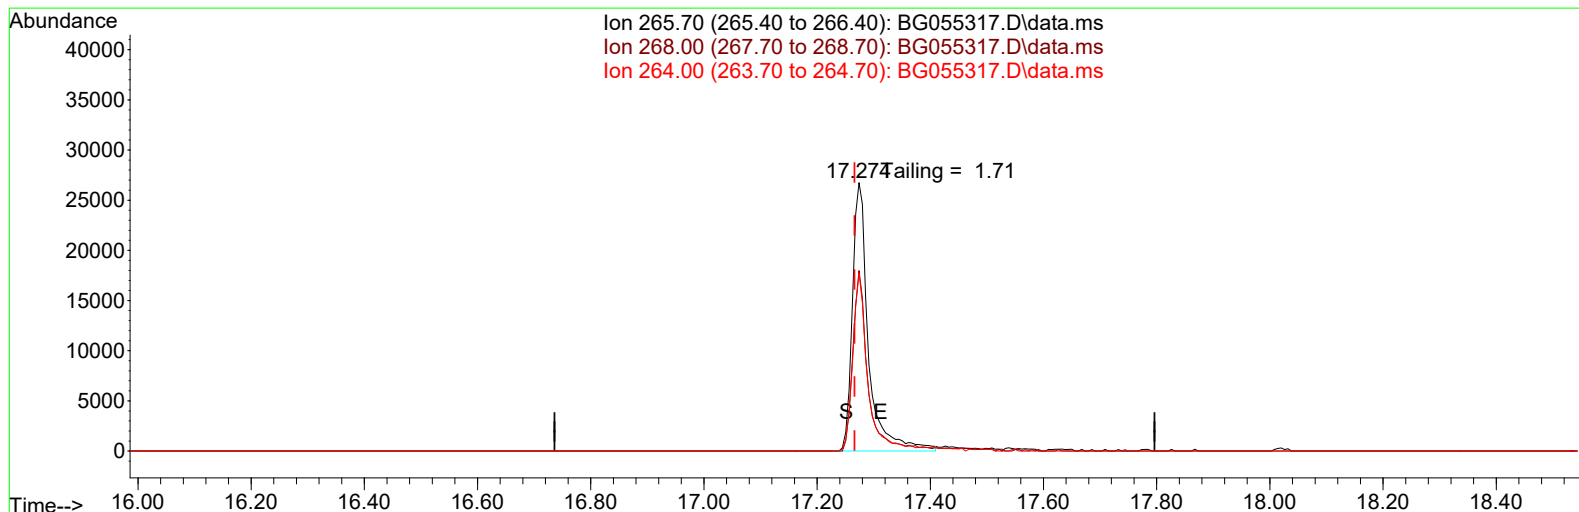

TIC: BG055317.D\data.ms

(70) Pentachlorophenol (C)

17.274min (+ 0.008) 42439.09 ng




response 53312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	67.22
264.00	64.40	66.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102722\
Data File : BG055317.D
Acq On : 27 Oct 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 28 06:40:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

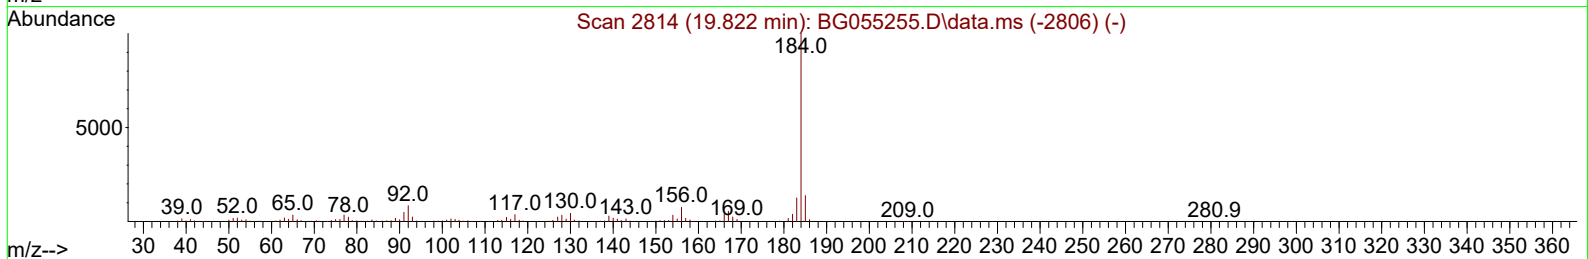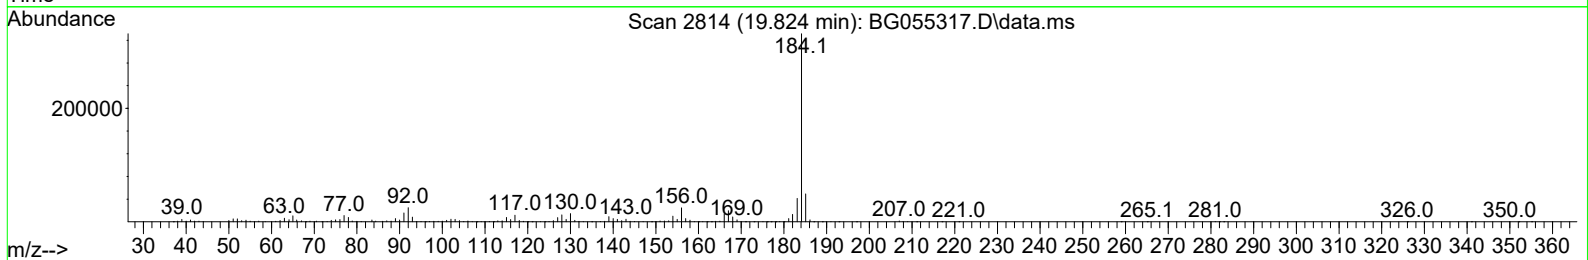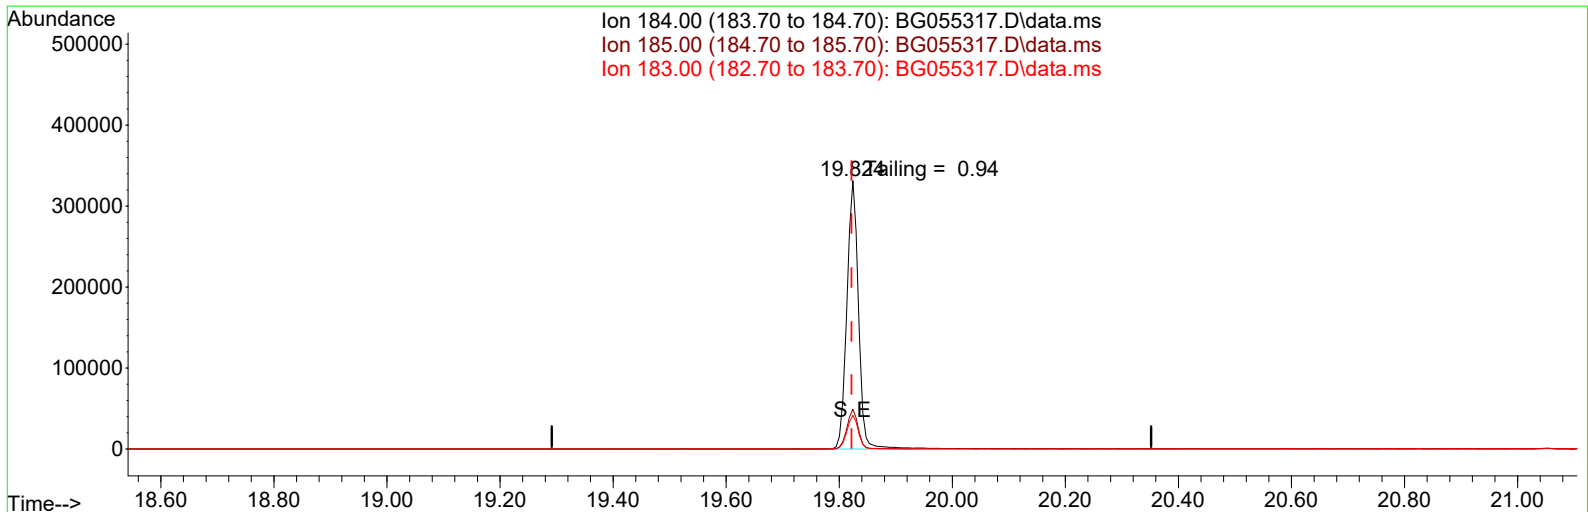

TIC: BG055317.D\data.ms

(77) Benzidine

19.824min (+ 0.002) 171482.53 ng

response 473337

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.82
183.00	12.50	12.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/27/2022	BNA_G	BG055317.D
Compound Name	Response	Retention Time
DDT	221921	21.052
DDD	4369	20.6
DDE	178	20.094
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4547	226468	2.01

Instrument :
BNA_G
ClientSampleId :
DFTPP