

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102815\
 Data File : BG019383.D
 Acq On : 28 Oct 2015 16:14
 Operator : UM/NP
 Sample : PB86317BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK17

Quant Time: Oct 29 01:33:33 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 29 01:04:20 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	21176	20.00	ng/ul	0.00
18) Naphthalene-d8	11.03	136	92078	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.83	164	73930	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	214465	20.00	ng/ul	0.00
78) Chrysene-d12	21.86	240	289359	20.00	ng/ul	0.00
86) Perylene-d12	25.24	264	263314	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.51	96	3633	8.22	ng/uL	0.00
5) Phenol-d5	7.34	99	68782	35.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	47207	38.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.73	132	44305	36.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.91	113	55466	35.82	ng/ul	0.00
19) Nitrobenzene-d5	9.38	128	24138	35.67	ng/ul	0.00
22) 2-Nitrophenol-d4	10.11	143	29552	36.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	57348	32.91	ng/ul	0.00
29) 4-Chloroaniline-d4	11.16	131	70713	40.11	ng/ul	0.00
44) Dimethylphthalate-d6	14.23	166	232207	38.09	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	242660	35.95	ng/ul	0.00
52) 4-Nitrophenol-d4	15.01	143	34830	35.97	ng/ul	0.00
58) Fluorene-d10	15.82	176	199251	35.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.92	200	47371	34.13	ng/ul	0.00
71) Anthracene-d10	17.67	188	365490	37.38	ng/ul	0.00
79) Pyrene-d10	19.95	212	463860	36.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.01	264	498199	37.70	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.91	70	1825	1.07	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102815\
Data File : BG019383.D
Acq On : 28 Oct 2015 16:14
Operator : UM/NP
Sample : PB86317BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK17

Quant Time: Oct 29 01:33:33 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 29 01:04:20 2015
Response via : Initial Calibration

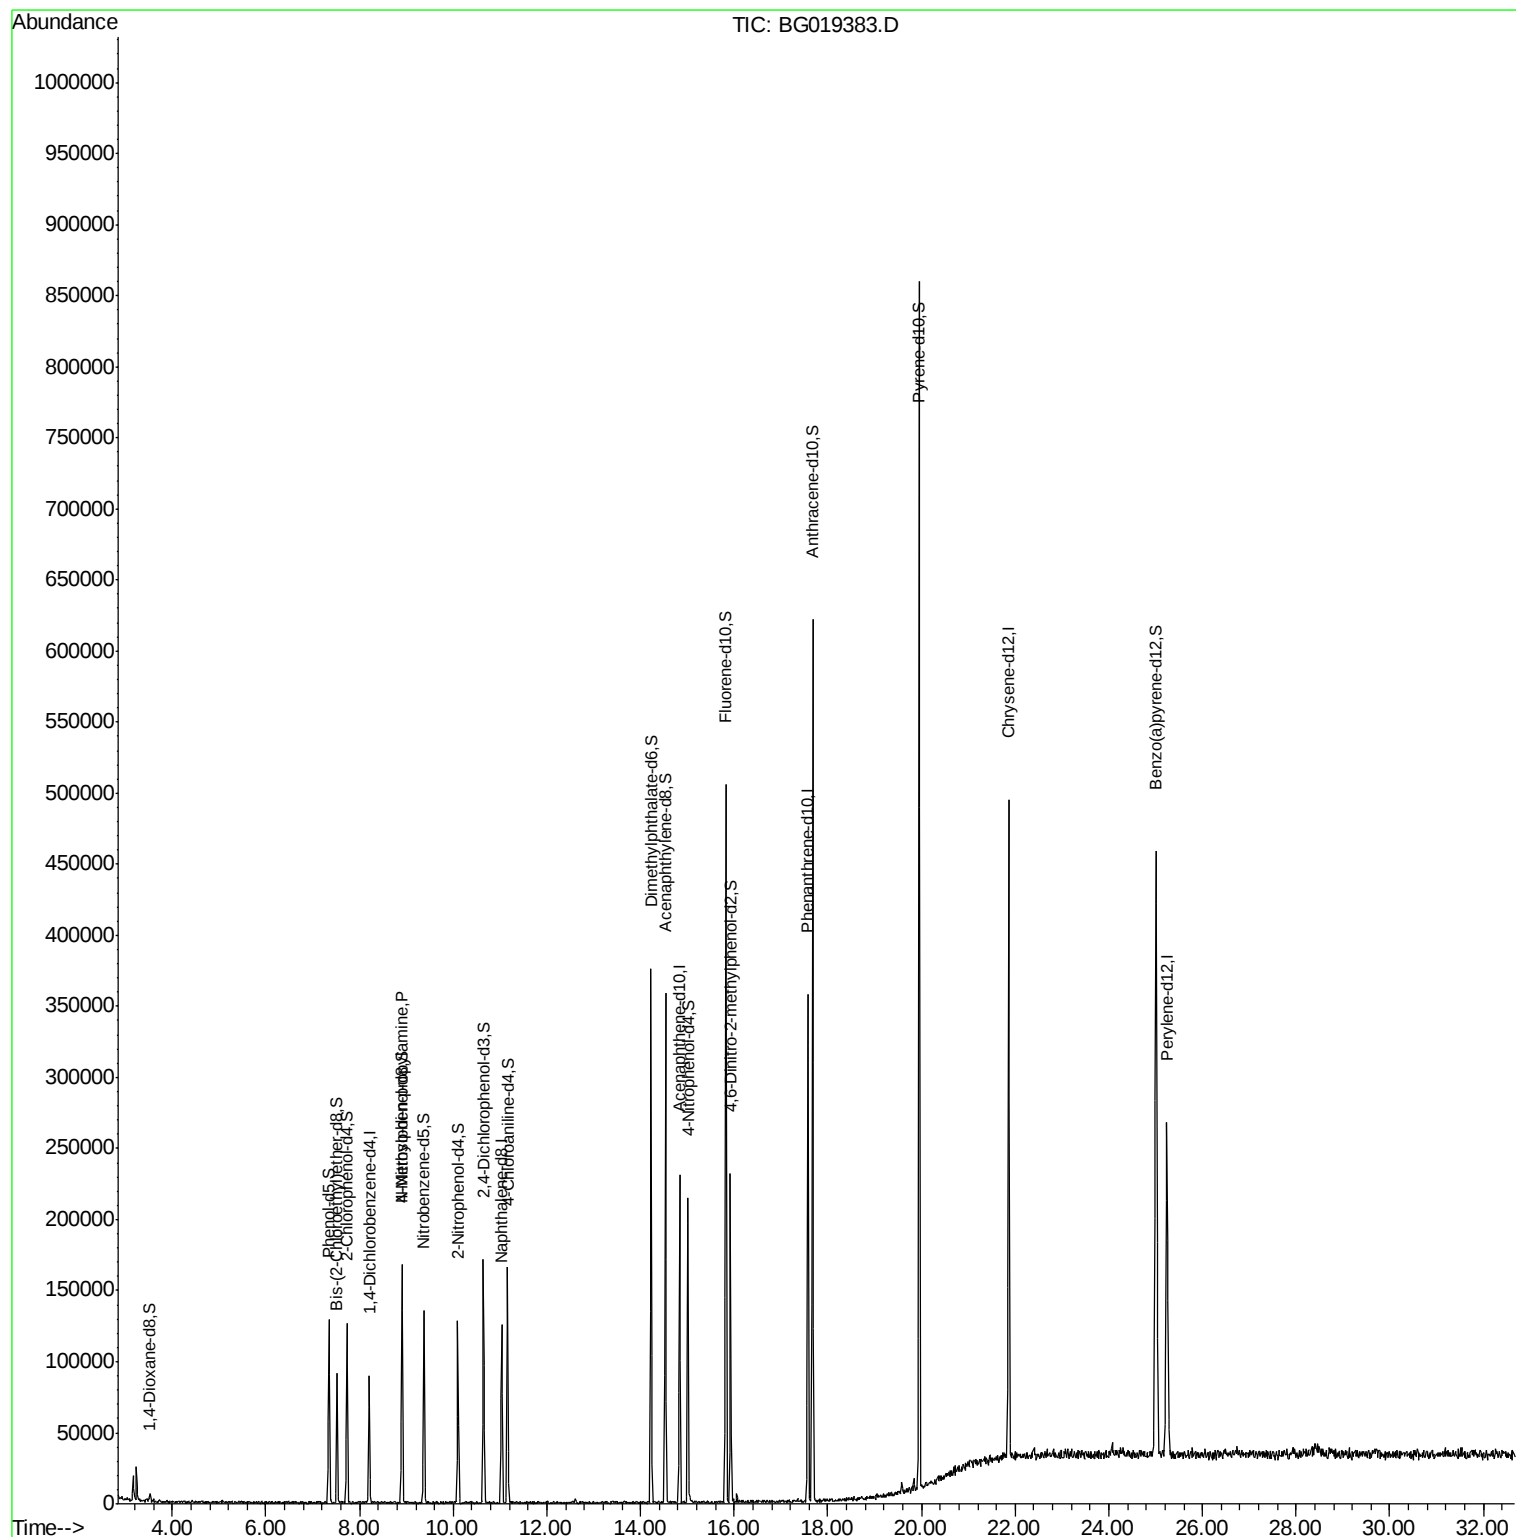

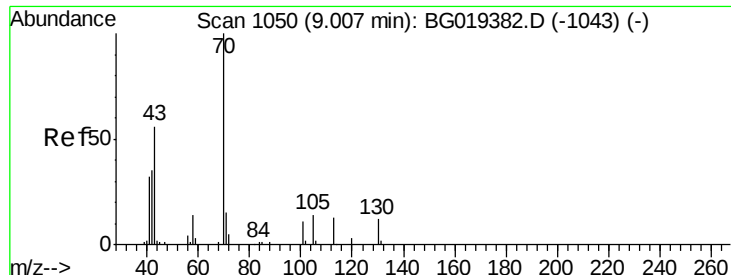

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.07 ng/ul
 RT: 8.91 min Scan# 1033
 Delta R.T. -0.10 min
 Lab File: BG019383.D
 Acq: 28 Oct 2015 16:14

Instrument :
 BNA_G
 ClientSampleId :
 SBLK17

Tot Ion: 70 Resp: 1825
 Ion Ratio Lower Upper
 70 100
 42 240.3 36.6 55.0#
 101 0.0 5.8 8.8#
 130 0.0 14.6 22.0#

