

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102815\
 Data File : BG019408.D
 Acq On : 29 Oct 2015 8:33
 Operator : UM/NP
 Sample : G4075-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9L1

Quant Time: Oct 30 00:33:35 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 29 04:26:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	42545	20.00	ng/ul	0.00
18) Naphthalene-d8	11.03	136	174368	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.84	164	129769	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	321481	20.00	ng/ul	0.00
78) Chrysene-d12	21.86	240	373636	20.00	ng/ul	0.00
86) Perylene-d12	25.25	264	351756	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	2658	2.99	ng/uL	0.01
5) Phenol-d5	7.36	99	90547	23.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	56053	22.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.74	132	56918	23.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.91	113	66572	21.40	ng/ul	0.00
19) Nitrobenzene-d5	9.38	128	29120	22.72	ng/ul	0.00
22) 2-Nitrophenol-d4	10.11	143	35391	23.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	74265	22.50	ng/ul	0.00
29) 4-Chloroaniline-d4	11.16	131	60023	17.98	ng/ul	0.00
44) Dimethylphthalate-d6	14.23	166	232881	21.77	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	279198	23.56	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	34089	20.06	ng/ul	0.01
58) Fluorene-d10	15.82	176	220189	22.25	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.93	200	42175	20.27	ng/ul	0.00
71) Anthracene-d10	17.67	188	344667	23.52	ng/ul	0.00
79) Pyrene-d10	19.95	212	392937	24.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.01	264	432151	24.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.27	163	54498	4.98	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102815\
Data File : BG019408.D
Acq On : 29 Oct 2015 8:33
Operator : UM/NP
Sample : G4075-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9L1

Quant Time: Oct 30 00:33:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 29 04:26:00 2015
Response via : Initial Calibration

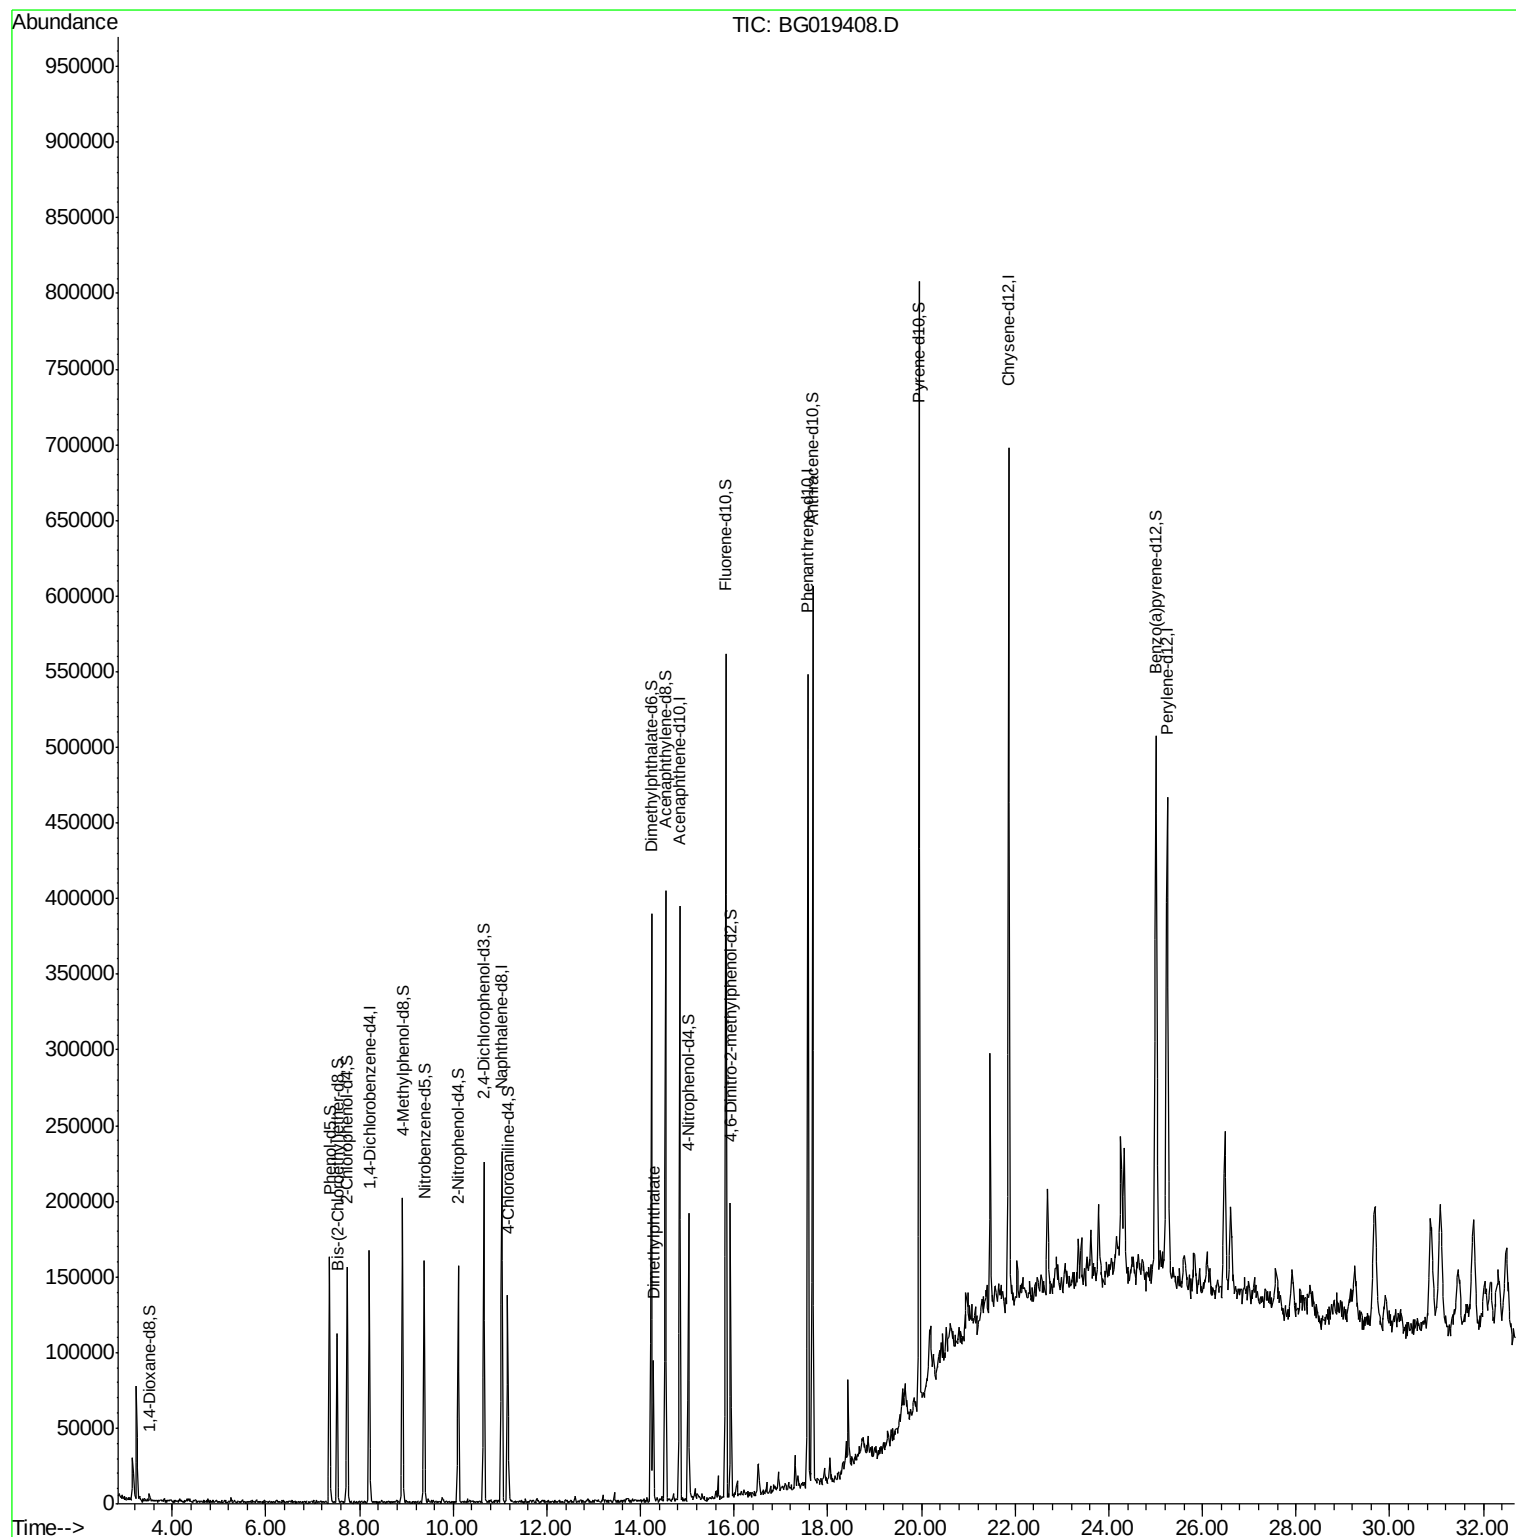

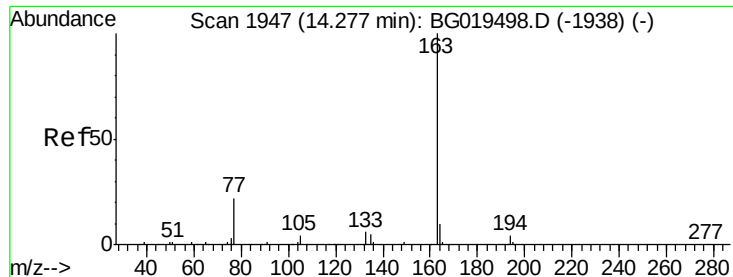

#45

Dimethylphthalate

Concen: 4.98 ng/ul

RT: 14.27 min Scan# 1946

Delta R.T. -0.01 min

Lab File: BG019408.D

Acq: 29 Oct 2015 8:33

Instrument :

BNA_G

ClientSampleId :

JG9L1


Tgt Ion:163 Resp: 54498

Ion Ratio Lower Upper

163 100

194 4.6 4.3 6.5

164 10.7 7.5 11.3

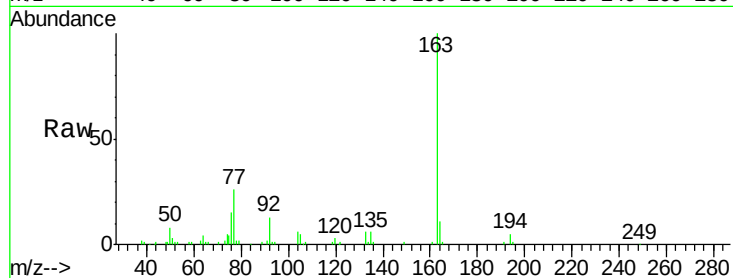

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

