

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102815\
 Data File : BG019409.D
 Acq On : 29 Oct 2015 9:11
 Operator : UM/NP
 Sample : G4075-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9J0

Quant Time: Oct 30 00:33:44 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 29 04:26:00 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	30809	20.00	ng/ul	0.00
18) Naphthalene-d8	11.03	136	128083	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.84	164	98342	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	249220	20.00	ng/ul	0.00
78) Chrysene-d12	21.86	240	285877	20.00	ng/ul	0.00
86) Perylene-d12	25.24	264	274713	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.51	96	3672	5.71	ng/uL	0.00
5) Phenol-d5	7.36	99	107841	38.13	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.52	67	71697	39.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.74	132	71348	40.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.91	113	85661	38.03	ng/ul	0.00
19) Nitrobenzene-d5	9.38	128	35071	37.26	ng/ul	0.00
22) 2-Nitrophenol-d4	10.11	143	43621	39.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	94897	39.15	ng/ul	0.00
29) 4-Chloroaniline-d4	11.16	131	86567	35.30	ng/ul	0.00
44) Dimethylphthalate-d6	14.23	166	293634	36.21	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	355890	39.63	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	38593	29.96	ng/ul	0.01
58) Fluorene-d10	15.82	176	277618	37.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.93	200	55029	34.11	ng/ul	0.00
71) Anthracene-d10	17.67	188	453595	39.93	ng/ul	0.00
79) Pyrene-d10	19.95	212	507916	40.60	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.01	264	548902	39.82	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.91	70	2955	1.19	ng/ul#	1
45) Dimethylphthalate	14.28	163	151784	18.30	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102815\
Data File : BG019409.D
Acq On : 29 Oct 2015 9:11
Operator : UM/NP
Sample : G4075-12
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9J0

Quant Time: Oct 30 00:33:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 29 04:26:00 2015
Response via : Initial Calibration




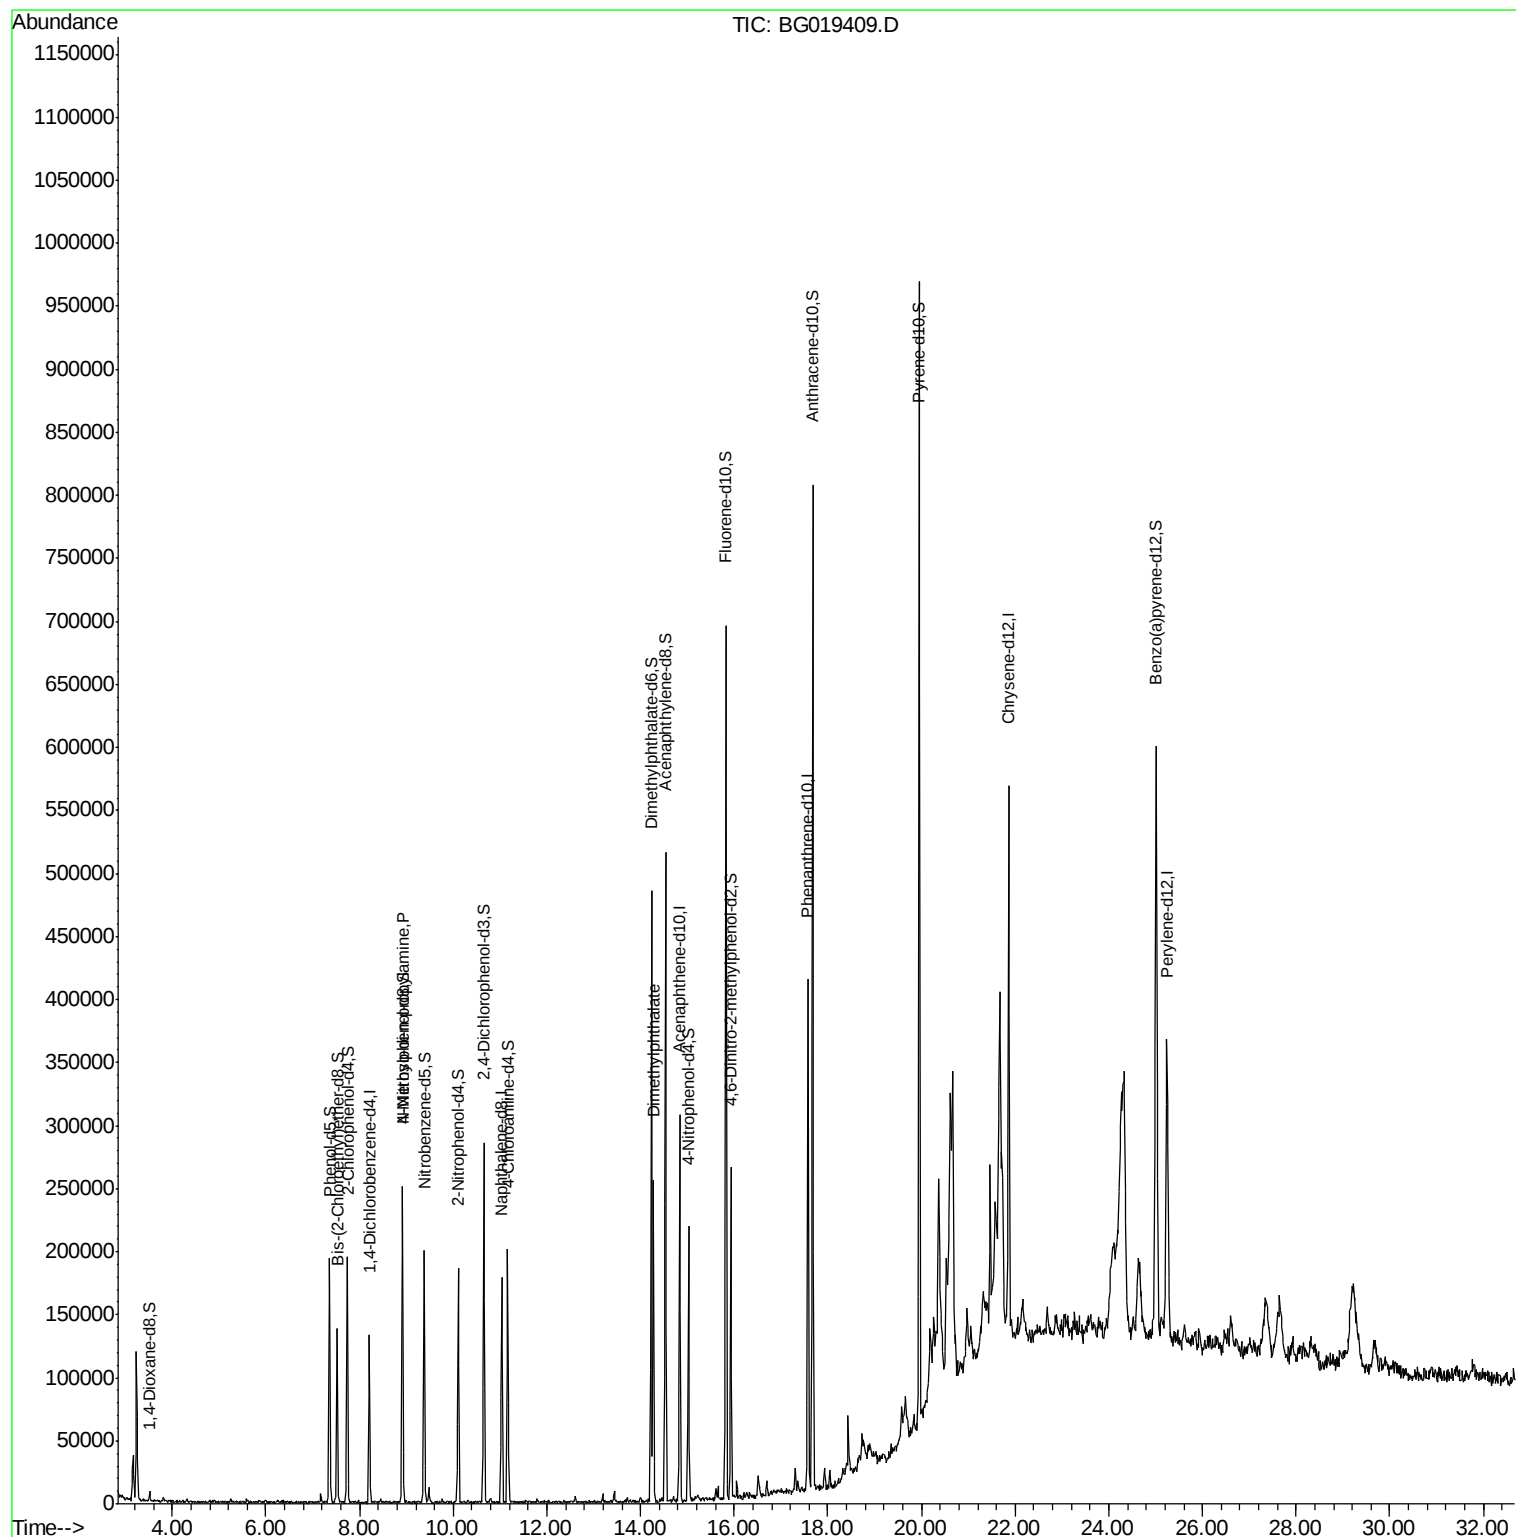


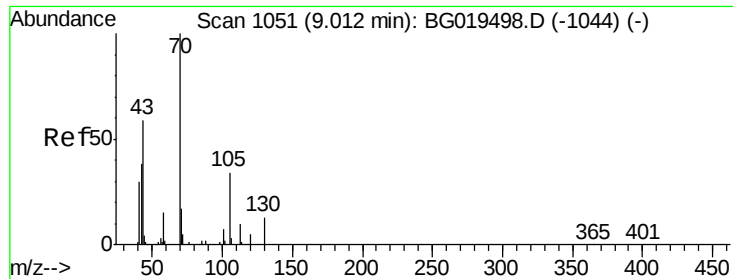

#15
N-Nitroso-di-n-propylamine
Concen: 1.19 ng/ul
RT: 8.91 min Scan# 1034
Delta R.T. -0.10 min
Lab File: BG019409.D
Acq: 29 Oct 2015 9:11

Instrument :
BNA_G
ClientSampleId :
JG9J0

Tgt Ion: 70 Resp: 2955
Ion Ratio Lower Upper
70 100
42 241.1 36.6 55.0#
101 0.0 5.8 8.8#
130 0.0 14.6 22.0#

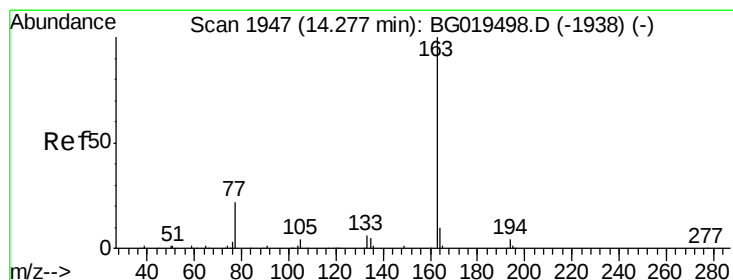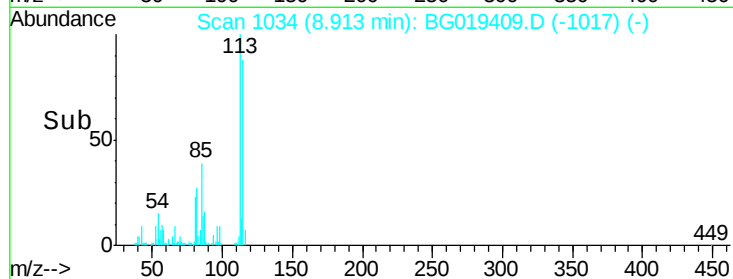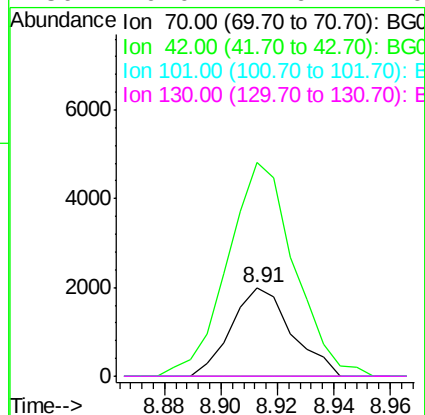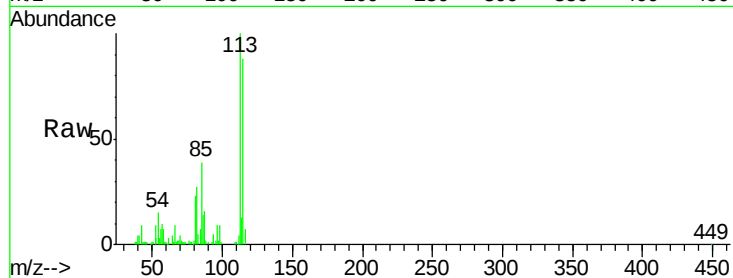

#45
Dimethylphthalate
Concen: 18.30 ng/ul
RT: 14.28 min Scan# 1947
Delta R.T. 0.00 min
Lab File: BG019409.D
Acq: 29 Oct 2015 9:11

Tgt Ion: 163 Resp: 151784
Ion Ratio Lower Upper
163 100
194 4.4 4.3 6.5
164 10.1 7.5 11.3

