

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102815\
 Data File : BG019414.D
 Acq On : 29 Oct 2015 12:39
 Operator : UM/NP
 Sample : PB86289BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK89

Quant Time: Oct 30 01:18:02 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 30 02:14:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	38674	20.00	ng/ul	0.00
18) Naphthalene-d8	11.03	136	153010	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.83	164	115728	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.58	188	299651	20.00	ng/ul	0.00
78) Chrysene-d12	21.87	240	346204	20.00	ng/ul	0.00
86) Perylene-d12	25.25	264	324391	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.51	96	5106	6.32	ng/uL	0.00
5) Phenol-d5	7.36	99	137607	38.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.52	67	85850	38.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.74	132	84464	38.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.91	113	113419	40.11	ng/ul	0.00
19) Nitrobenzene-d5	9.38	128	45042	40.06	ng/ul	0.00
22) 2-Nitrophenol-d4	10.10	143	54333	40.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.65	165	116094	40.09	ng/ul	0.00
29) 4-Chloroaniline-d4	11.17	131	51849	17.70	ng/ul	0.00
44) Dimethylphthalate-d6	14.23	166	359415	37.67	ng/ul	0.00
47) Acenaphthylene-d8	14.53	160	420815	39.82	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	57084	37.66	ng/ul	0.00
58) Fluorene-d10	15.82	176	327894	37.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.93	200	71129	36.67	ng/ul	0.00
71) Anthracene-d10	17.67	188	541026	39.61	ng/ul	0.00
79) Pyrene-d10	19.95	212	625632	41.30	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.02	264	681365	41.86	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.92	70	4402	1.41	ng/ul#	1
21) Isophorone	10.11	82	8231	1.03	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102815\
Data File : BG019414.D
Acq On : 29 Oct 2015 12:39
Operator : UM/NP
Sample : PB86289BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK89

Quant Time: Oct 30 01:18:02 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 30 02:14:45 2015
Response via : Initial Calibration




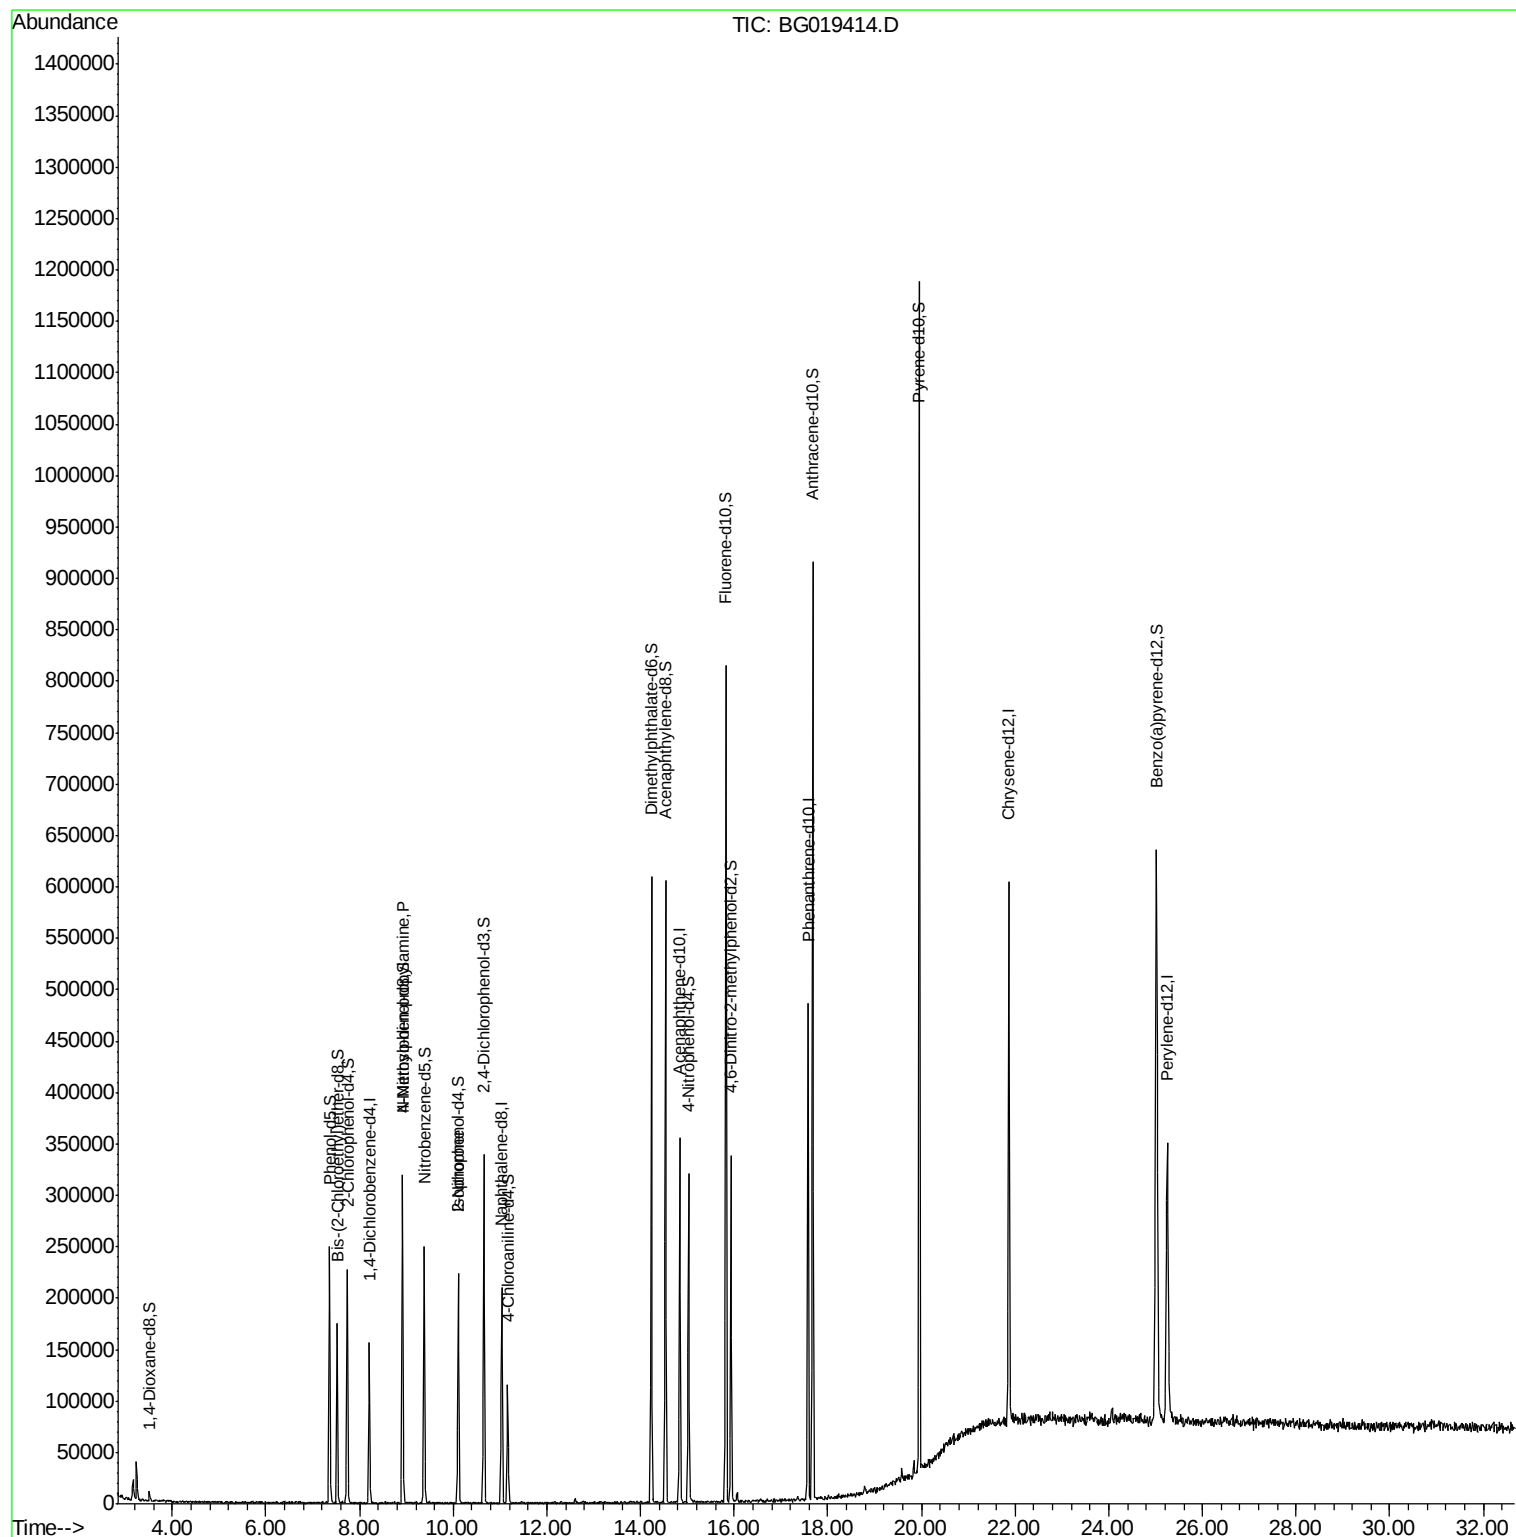


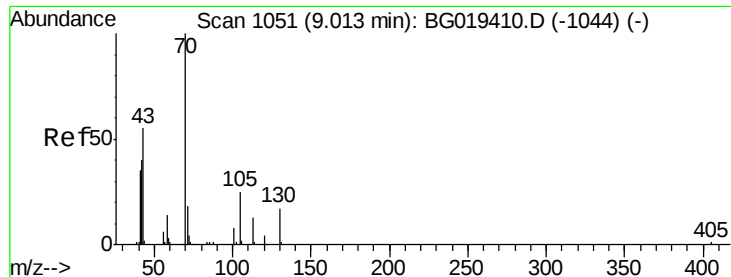

#15
N-Nitroso-di-n-propylamine
Concen: 1.41 ng/ul
RT: 8.92 min Scan# 1035
Delta R.T. -0.09 min
Lab File: BG019414.D
Acq: 29 Oct 2015 12:39

Instrument :
BNA_G
ClientSampleId :
SBLK89

Tgt Ion: 70 Resp: 4402
Ion Ratio Lower Upper
70 100
42 207.8 36.6 55.0#
101 0.0 5.8 8.8#
130 0.0 14.6 22.0#

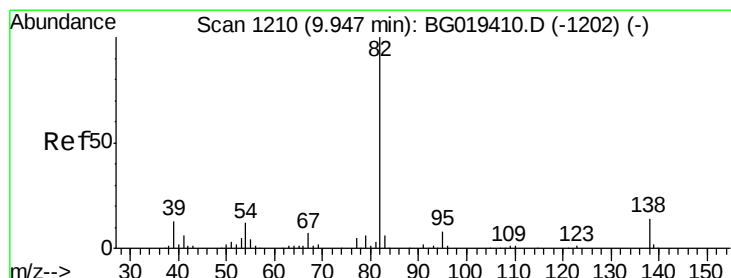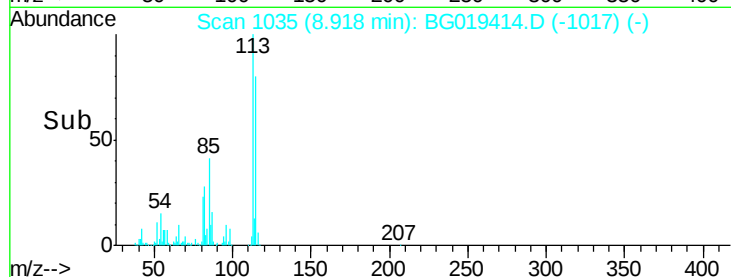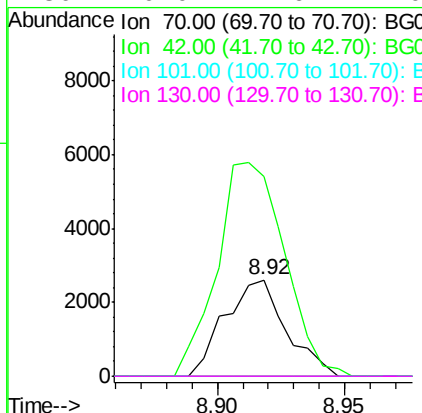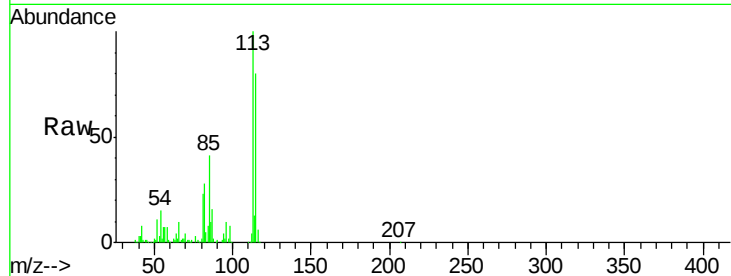

#21
Isophorone
Concen: 1.03 ng/ul
RT: 10.11 min Scan# 1238
Delta R.T. 0.16 min
Lab File: BG019414.D
Acq: 29 Oct 2015 12:39

Tgt Ion: 82 Resp: 8231
Ion Ratio Lower Upper
82 100
95 15.9 6.7 10.1#
138 0.0 10.8 16.2#

