

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102816\
 Data File : BG024540.D
 Acq On : 28 Oct 2016 15:48
 Operator : UM/SJ
 Sample : PB94361BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB94361BL

Quant Time: Oct 28 23:43:01 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	103077	20.00	ng	0.00
21) Naphthalene-d8	11.10	136	393519	20.00	ng	0.00
38) Acenaphthene-d10	14.89	164	297469	20.00	ng	0.00
63) Phenanthrene-d10	17.63	188	685759	20.00	ng	0.00
75) Chrysene-d12	21.93	240	972368	20.00	ng	0.00
86) Perylene-d12	25.36	264	996352	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	754612	119.99	ng	0.00
7) Phenol-d6	7.40	99	1022402	118.51	ng	0.00
23) Nitrobenzene-d5	9.45	82	720176	83.32	ng	0.00
41) 2,4,6-Tribromophenol	16.37	330	487721	109.75	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	1481232	82.76	ng	0.00
78) Terphenyl-d14	20.21	244	2666424	81.94	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102816\
Data File : BG024540.D
Acq On : 28 Oct 2016 15:48
Operator : UM/SJ
Sample : PB94361BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB94361BL

Quant Time: Oct 28 23:43:01 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

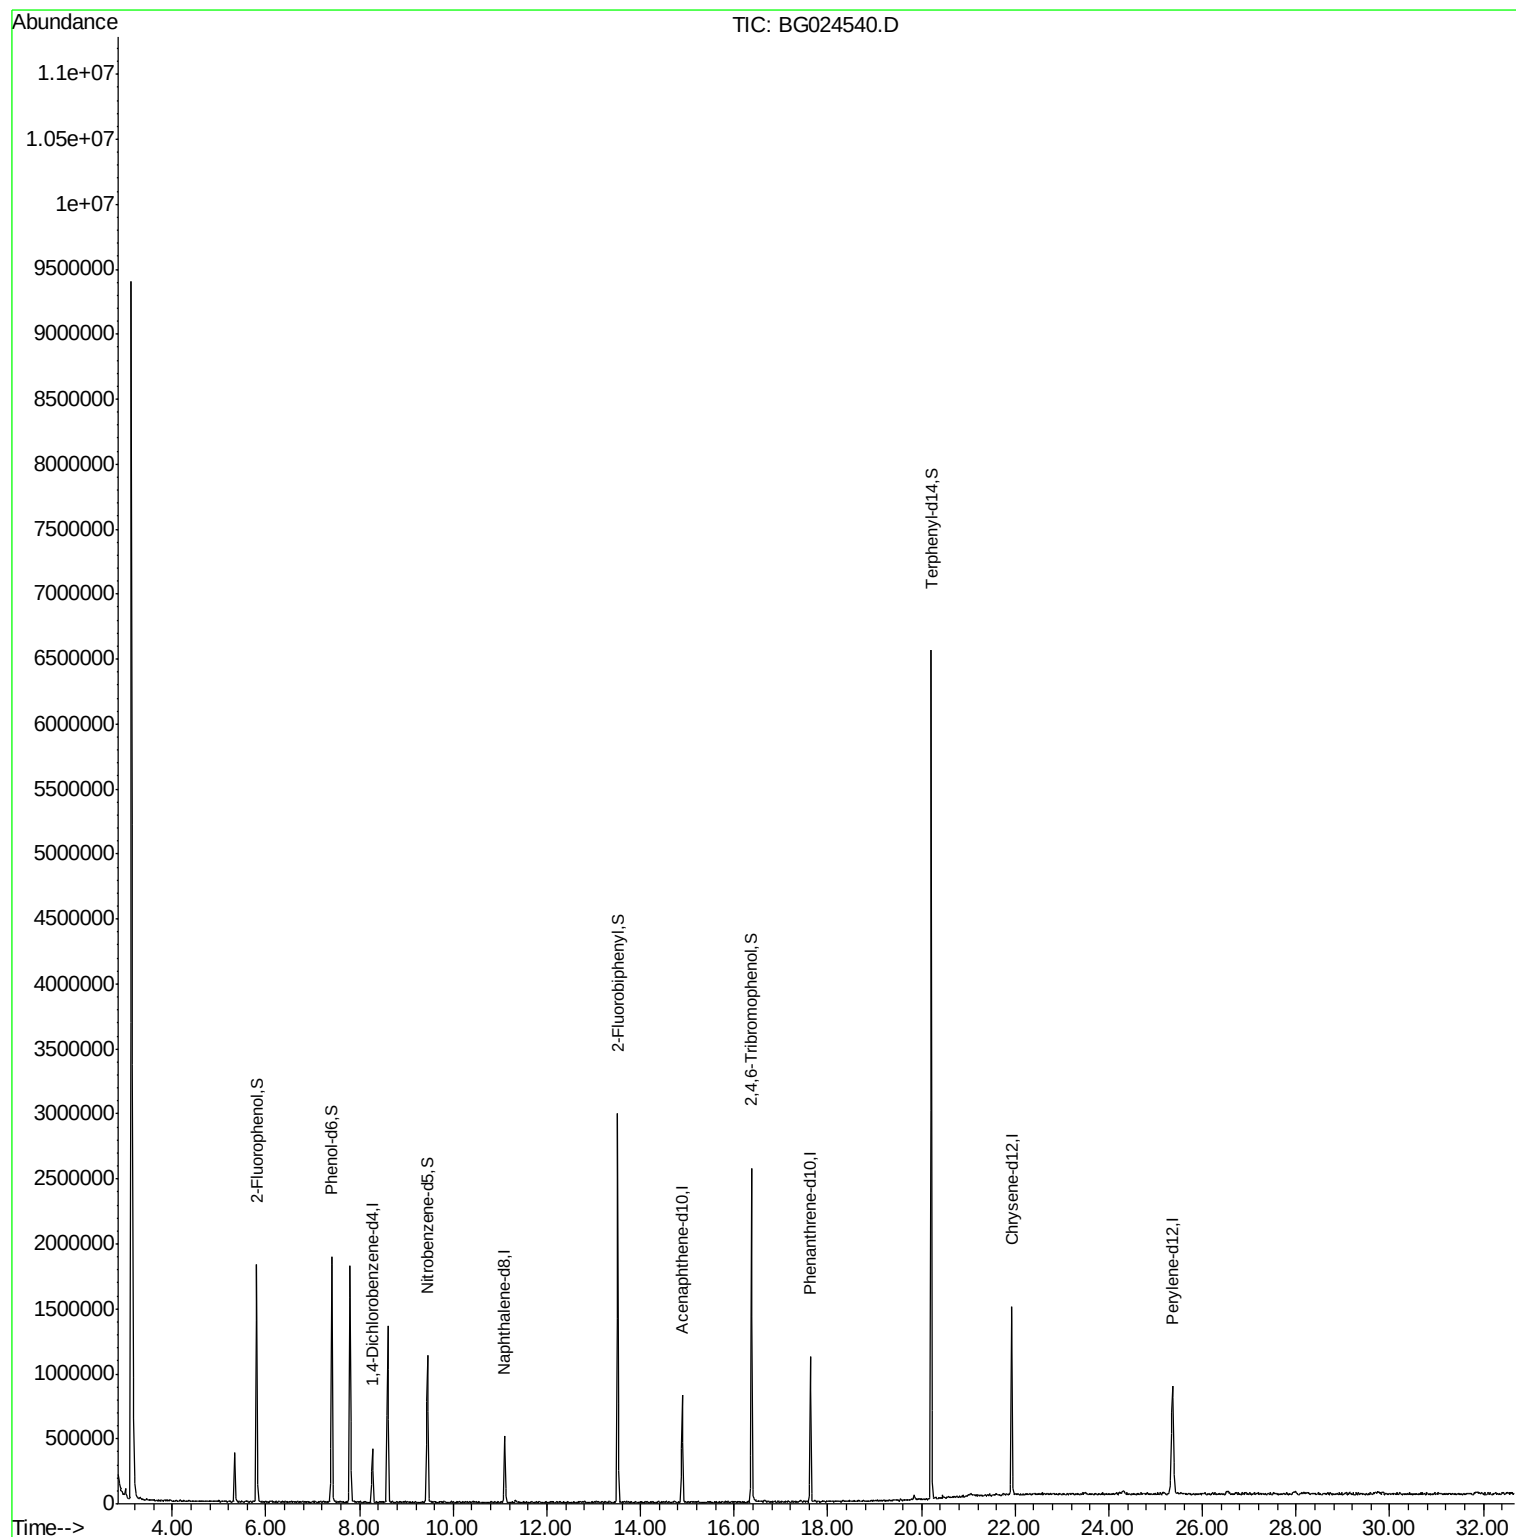

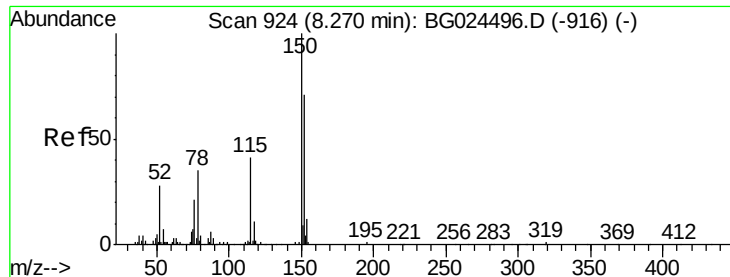

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.27 min Scan# 925

Delta R.T. 0.00 min

Lab File: BG024540.D

Acq: 28 Oct 2016 15:48

Instrument :

BNA_G

ClientSampleId :

PB94361BL


Tgt Ion:152 Resp: 103077

Ion Ratio Lower Upper

152 100

150 178.1 114.0 171.0#




115 64.8 48.1 72.1

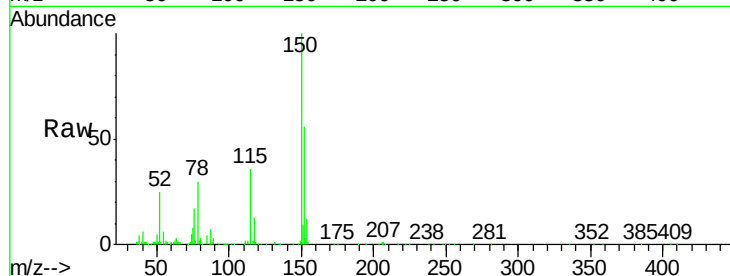

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

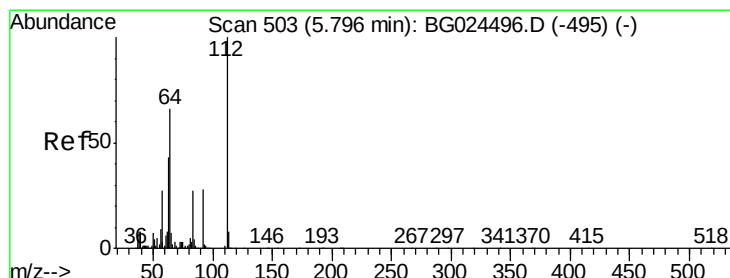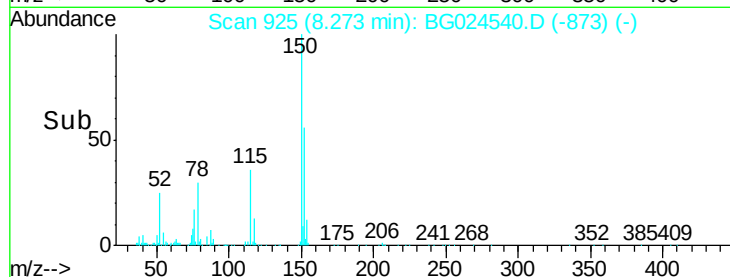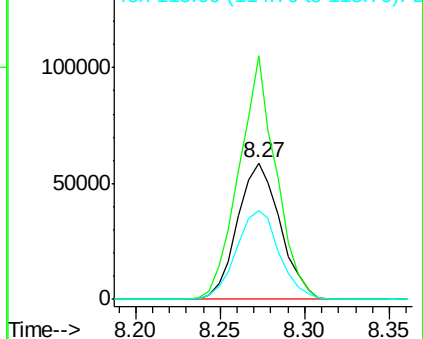

#5

2-Fluorophenol

Concen: 119.99 ng

RT: 5.80 min Scan# 505

Delta R.T. 0.01 min

Lab File: BG024540.D

Acq: 28 Oct 2016 15:48


Tgt Ion:112 Resp: 754612

Ion Ratio Lower Upper

112 100

64 70.1 61.8 92.6



63 40.0 37.2 55.8

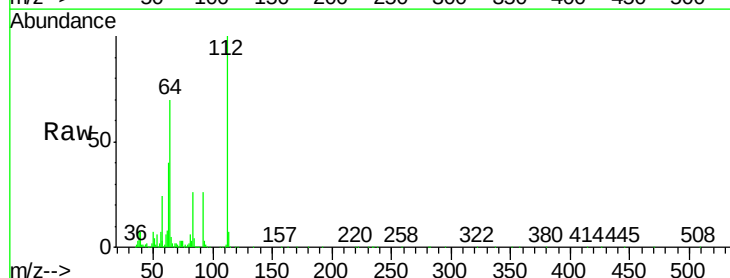


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

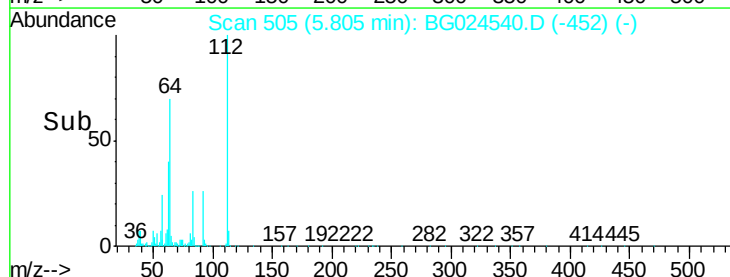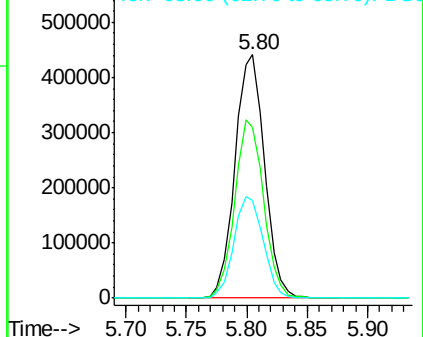

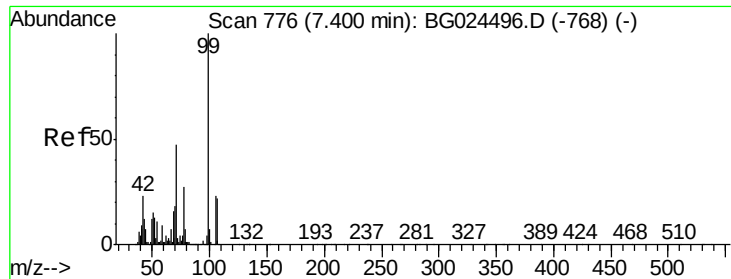

#7

Phenol-d6

Concen: 118.51 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024540.D

Acq: 28 Oct 2016 15:48

Instrument :

BNA_G

ClientSampleId :

PB94361BL


Tgt Ion: 99 Resp: 1022402

Ion Ratio Lower Upper




99 100

42 21.6 20.5 30.7

71 46.8 37.6 56.4

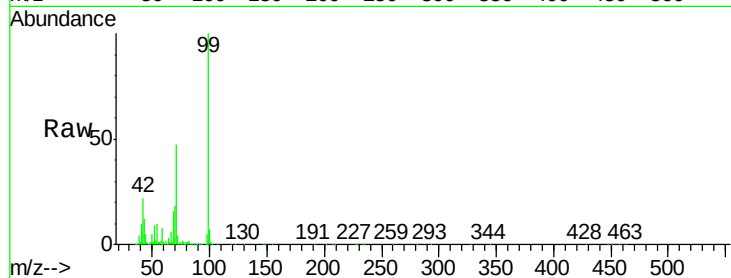

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

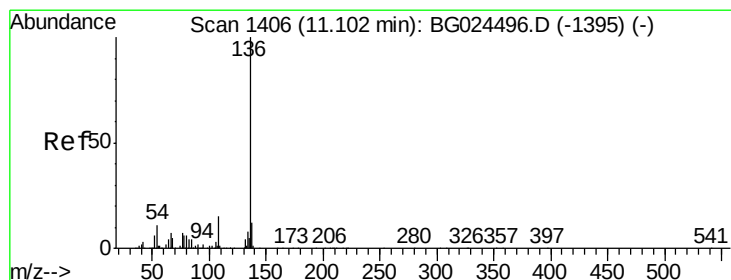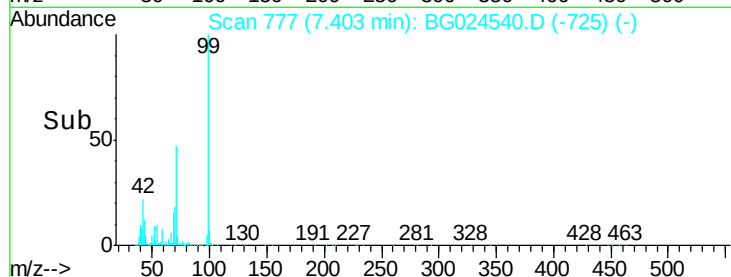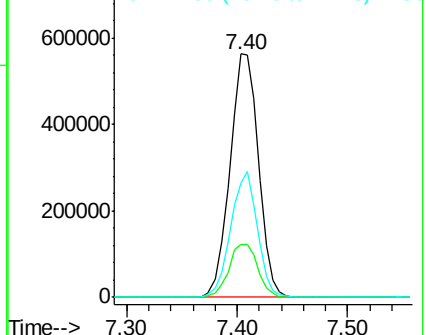

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.10 min Scan# 1406

Delta R.T. -0.00 min

Lab File: BG024540.D

Acq: 28 Oct 2016 15:48

Tgt Ion: 136 Resp: 393519


Ion Ratio Lower Upper

136 100



137 10.3 8.9 13.3


54 10.0 9.3 13.9

68 6.9 5.1 7.7

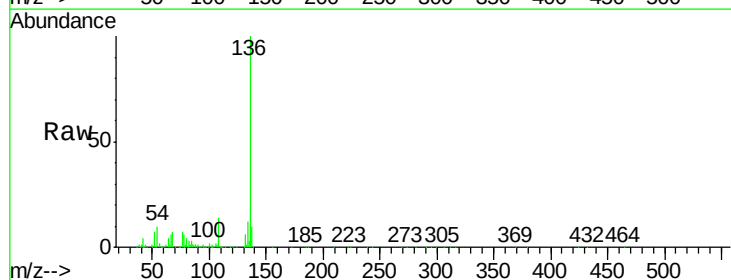

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



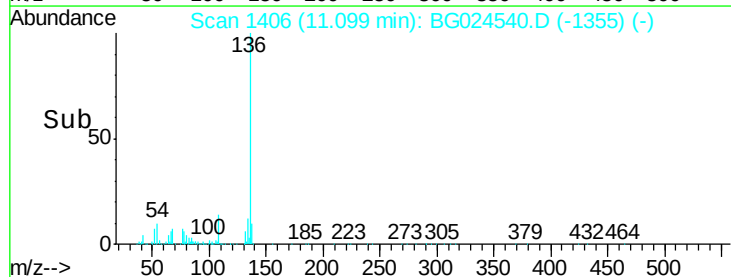
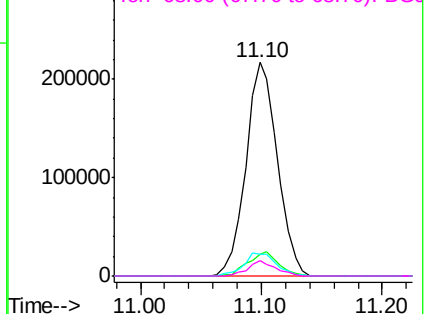


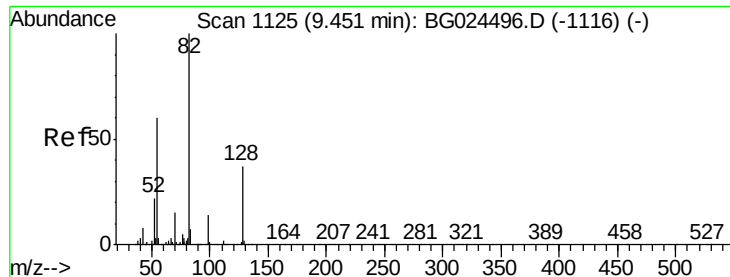

#23
 Nitrobenzene-d5
 Concen: 83.32 ng
 RT: 9.45 min Scan# 1125
 Delta R.T. -0.00 min
 Lab File: BG024540.D
 Acq: 28 Oct 2016 15:48




Instrument :
 BNA_G
 ClientSampleId :
 PB94361BL


Tgt Ion	Ratio	Lower	Upper
82	100		
128	34.4	26.4	39.6
54	56.2	49.4	74.2

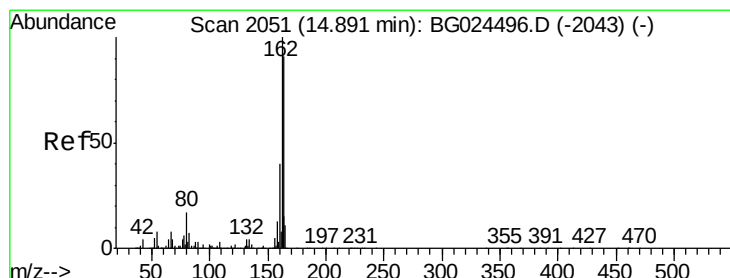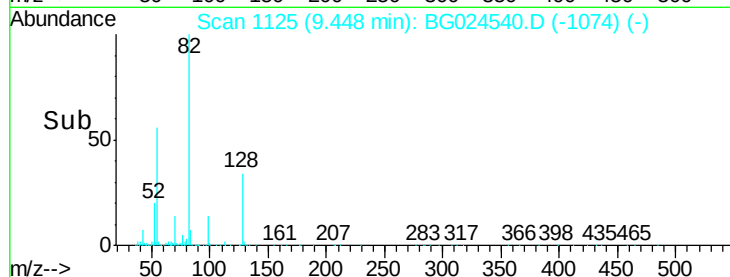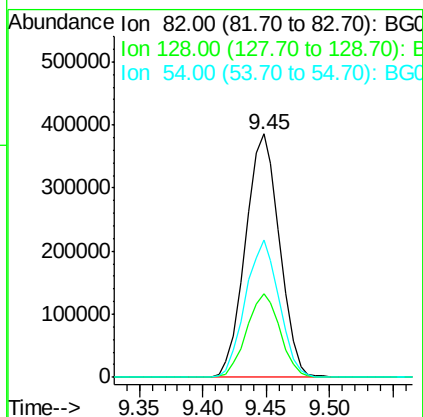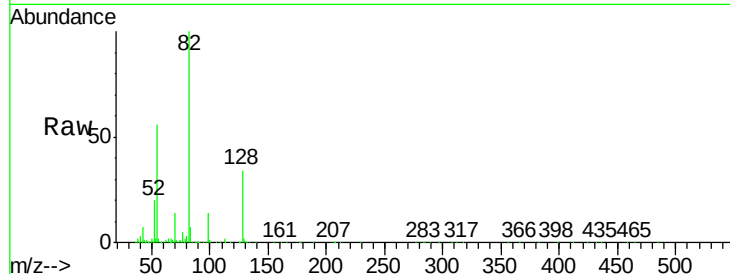

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.89 min Scan# 2051
 Delta R.T. -0.00 min
 Lab File: BG024540.D
 Acq: 28 Oct 2016 15:48

Tgt Ion	Ratio	Lower	Upper
164	100		
162	108.4	85.1	127.7
160	41.4	34.7	52.1


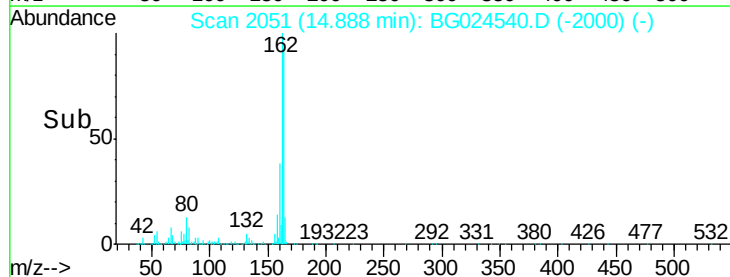
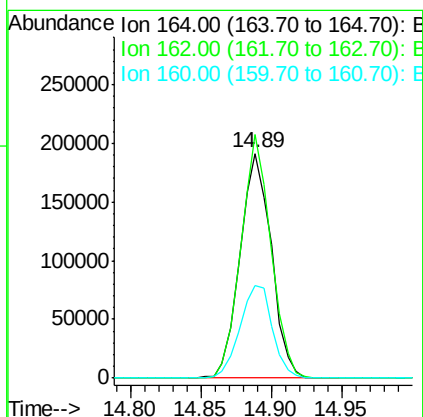
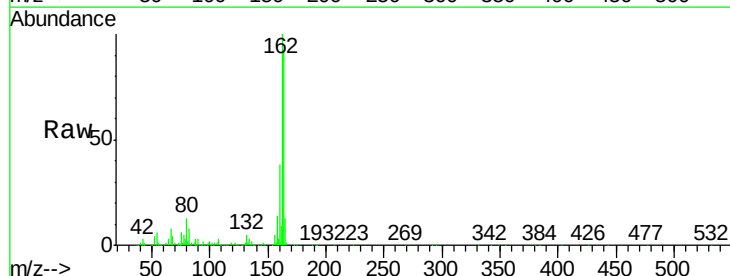


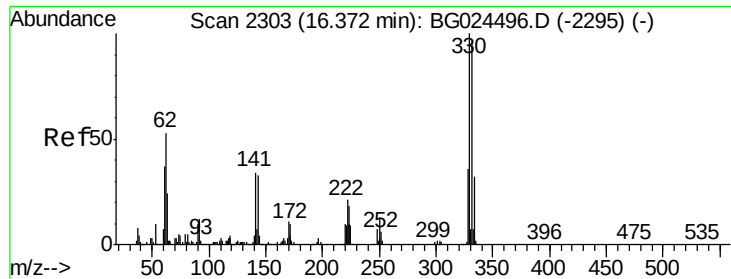

#41
 2,4,6-Tribromophenol
 Concen: 109.75 ng
 RT: 16.37 min Scan# 2303
 Delta R.T. -0.00 min
 Lab File: BG024540.D
 Acq: 28 Oct 2016 15:48




Instrument :
 BNA_G
 ClientSampleId :
 PB94361BL


Tgt Ion:330 Resp: 487721
 Ion Ratio Lower Upper
 330 100
 332 95.2 77.3 115.9
 141 33.8 32.1 48.1

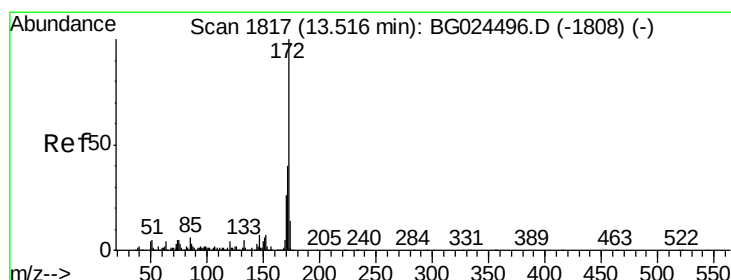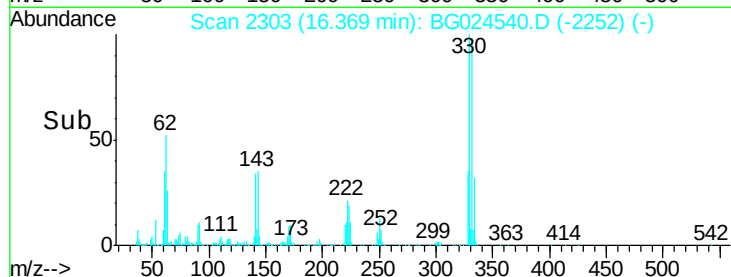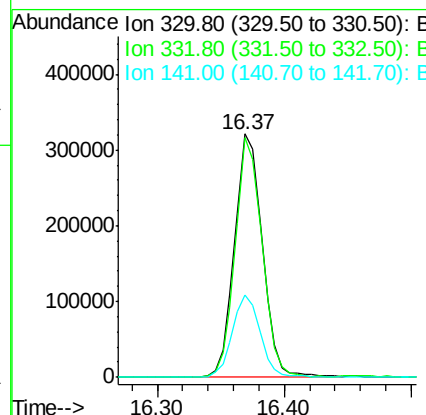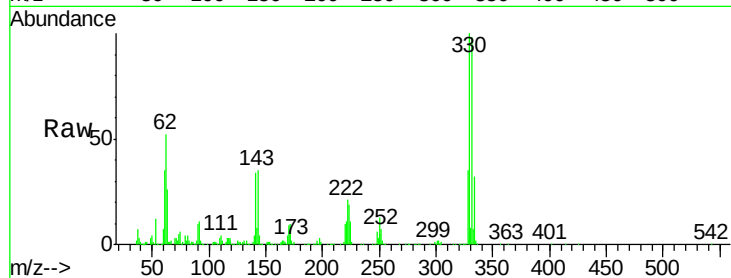

#44
 2-Fluorobiphenyl
 Concen: 82.76 ng
 RT: 13.51 min Scan# 1817
 Delta R.T. -0.00 min
 Lab File: BG024540.D
 Acq: 28 Oct 2016 15:48

Tgt Ion:172 Resp: 1481232
 Ion Ratio Lower Upper
 172 100
 171 37.8 32.2 48.2
 170 25.7 21.8 32.6

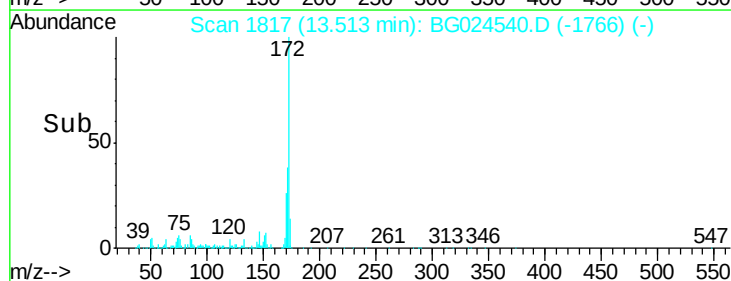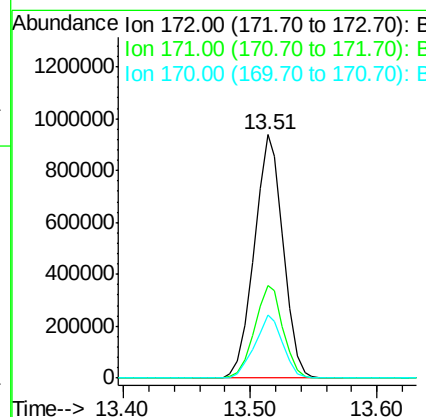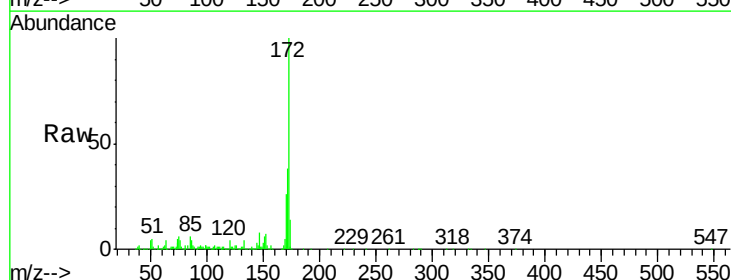


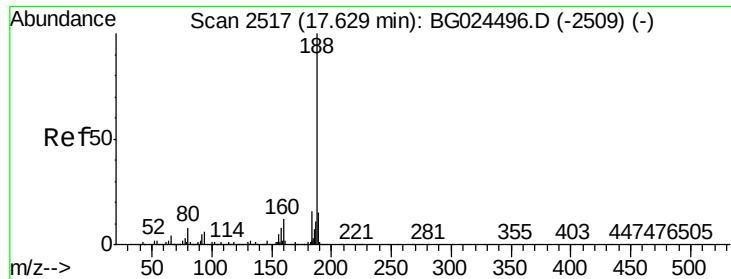




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.63 min Scan# 2518
Delta R.T. 0.00 min
Lab File: BG024540.D
Acq: 28 Oct 2016 15:48

Instrument :
BNA_G
ClientSampleId :
PB94361BL

Tgt Ion:188 Resp: 685759
Ion Ratio Lower Upper
188 100
94 6.9 5.8 8.8
80 7.4 7.5 11.3#

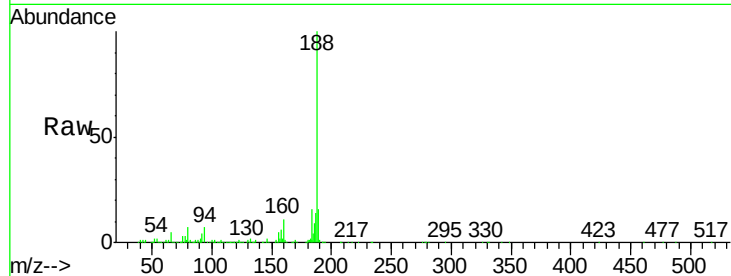


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

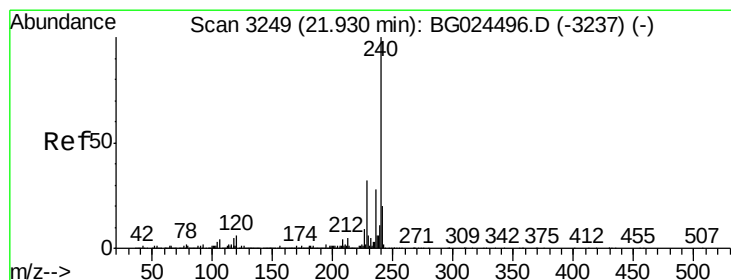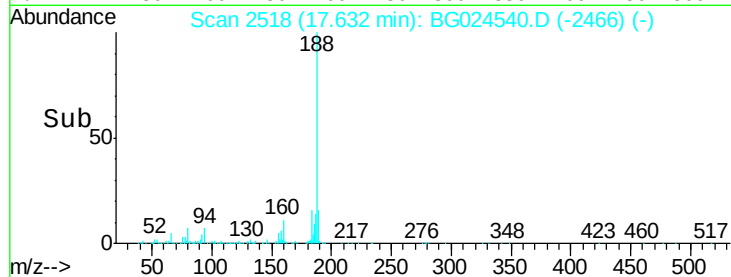
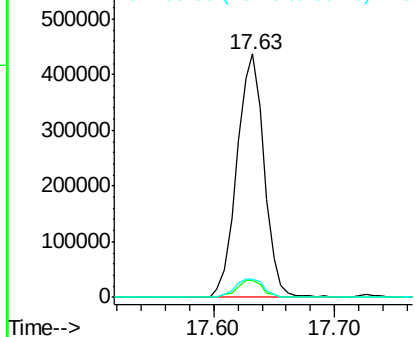



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.93 min Scan# 3249
Delta R.T. -0.00 min
Lab File: BG024540.D
Acq: 28 Oct 2016 15:48

Tgt Ion:240 Resp: 972368
Ion Ratio Lower Upper
240 100
120 6.2 5.7 8.5
236 28.3 22.2 33.4

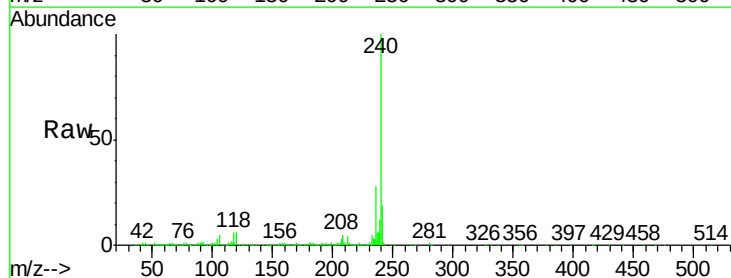

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

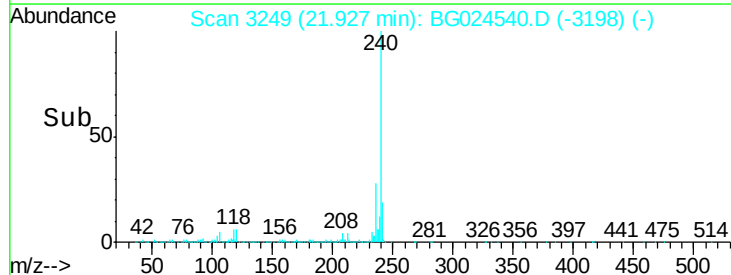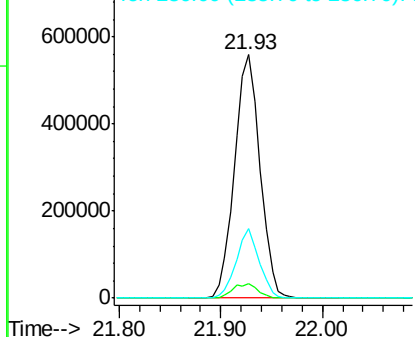

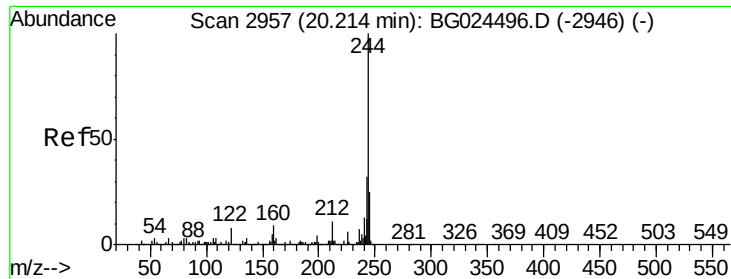

#78

Terphenyl-d14

Concen: 81.94 ng

RT: 20.21 min Scan# 2957

Delta R.T. -0.00 min

Lab File: BG024540.D

Acq: 28 Oct 2016 15:48

Instrument :

BNA_G

ClientSampleId :

PB94361BL


Tgt Ion:244 Resp: 2666424

Ion Ratio Lower Upper

244 100

212 10.4 10.0 15.0




122 9.0 8.6 12.8

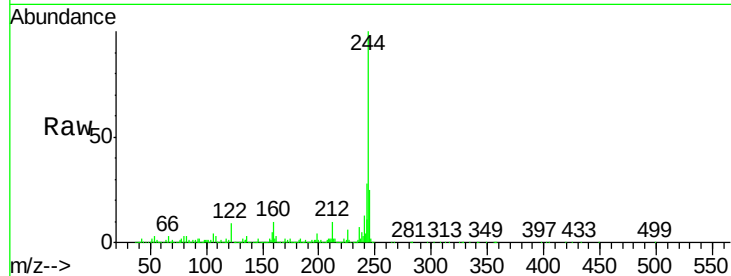

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

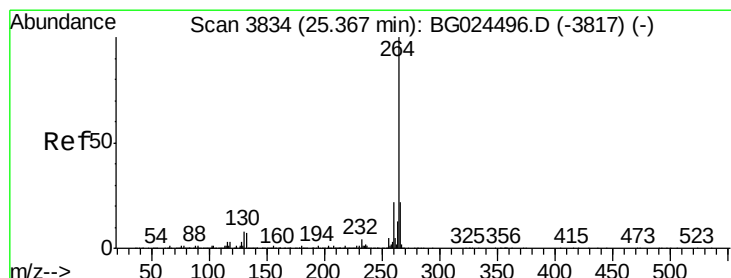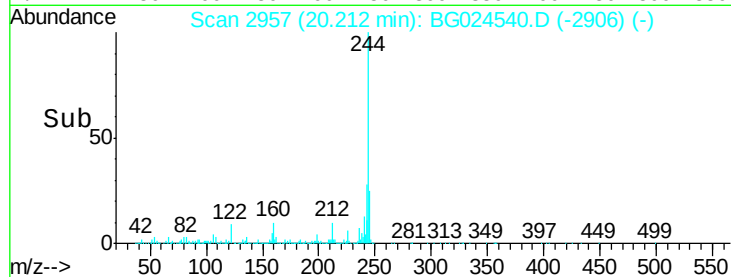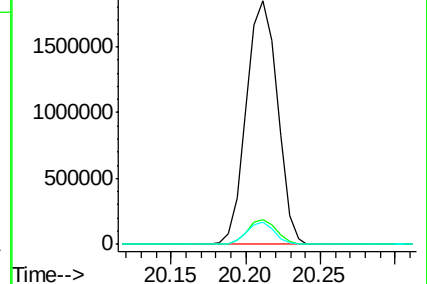

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.36 min Scan# 3833

Delta R.T. -0.01 min

Lab File: BG024540.D

Acq: 28 Oct 2016 15:48


Tgt Ion:264 Resp: 996352

Ion Ratio Lower Upper

264 100

260 24.3 21.8 32.8

265 21.2 18.2 27.4

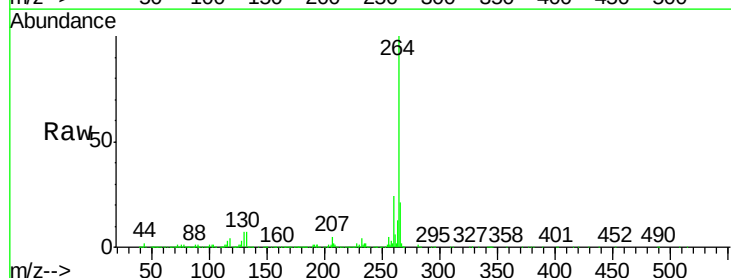

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

