


Data Path : Z:\HPCHEM1\BNA_G\Data\BG102816\
Data File : BG024535.D
Acq On : 28 Oct 2016 11:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 26 11:14:13 2016

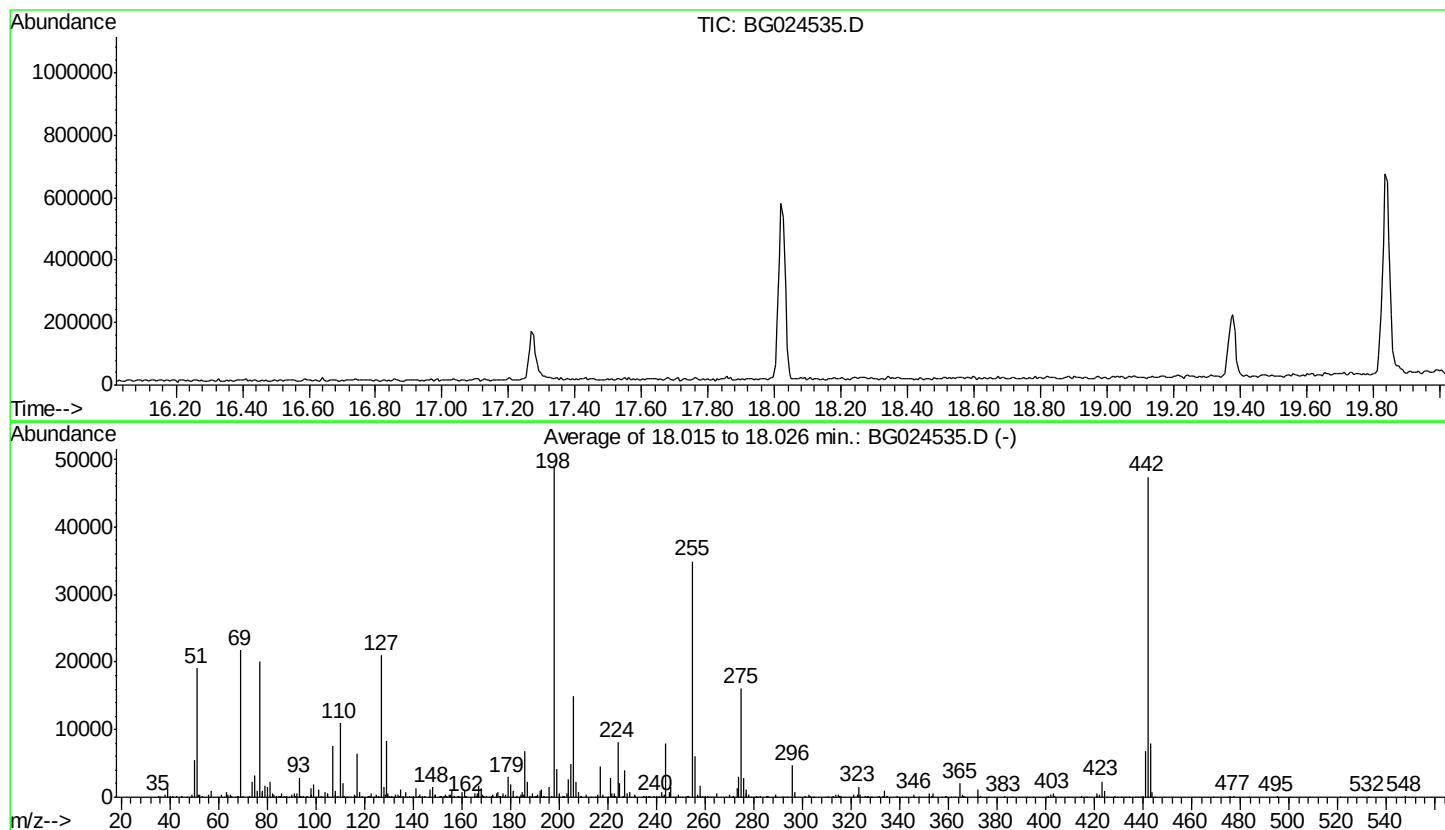

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	19058	PASS
68	69	0.00	2	0.8	178	PASS
69	198	0.00	100	44.3	21738	PASS
70	69	0.00	2	0.9	198	PASS
127	198	10	80	42.8	21018	PASS
197	198	0.00	2	0.4	188	PASS
198	198	100	100	100.0	49088	PASS
199	198	5	9	8.4	4139	PASS
275	198	10	60	32.7	16028	PASS
365	198	1	100	4.1	2024	PASS
441	442	0.01	24	14.4	6828	PASS
442	198	50	100	96.6	47429	PASS
443	442	15	24	16.8	7954	PASS