


Data Path : Z:\HPCHEM1\BNA_G\Data\BG102816\
 Data File : BG024538.D
 Acq On : 28 Oct 2016 14:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

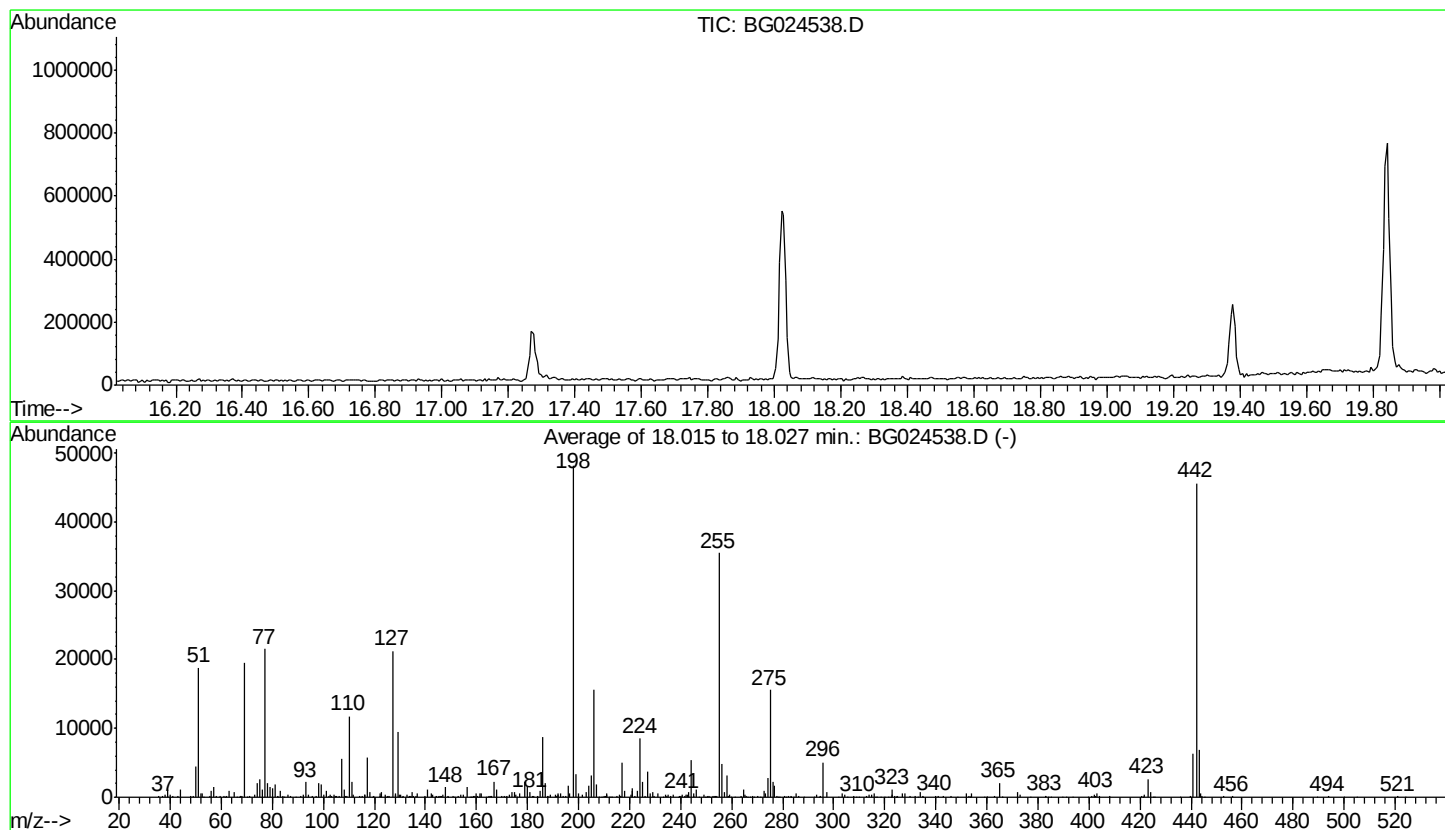

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	18863	PASS
68	69	0.00	2	1.2	237	PASS
69	198	0.00	100	40.6	19552	PASS
70	69	0.00	2	0.4	75	PASS
127	198	10	80	44.0	21189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48133	PASS
199	198	5	9	6.9	3325	PASS
275	198	10	60	32.3	15546	PASS
365	198	1	100	4.3	2060	PASS
441	442	0.01	24	14.0	6388	PASS
442	198	50	100	94.7	45589	PASS
443	442	15	24	15.1	6867	PASS