

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102817\
 Data File : BG030571.D
 Acq On : 29 Oct 2017 21:23
 Operator : SJ/JU
 Sample : I6094-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 30 08:04:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 17:32:15 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	71364	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	306923	20.00	ng	0.00
38) Acenaphthene-d10	14.78	164	204513	20.00	ng	-0.01
63) Phenanthrene-d10	17.52	188	508448	20.00	ng	0.00
75) Chrysene-d12	21.80	240	541306	20.00	ng	0.00
86) Perylene-d12	25.11	264	532495	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	713365	166.99	ng	0.00
7) Phenol-d6	7.32	99	853868	142.40	ng	0.00
23) Nitrobenzene-d5	9.33	82	596600	123.52	ng	0.00
41) 2,4,6-Tribromophenol	16.27	330	419471	158.86	ng	0.00
44) 2-Fluorobiphenyl	13.41	172	1570836	112.65	ng	0.00
78) Terphenyl-d14	20.11	244	2469946	103.80	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.49	79	9898	2.342	ng	Qvalue # 43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102817\
Data File : BG030571.D
Acq On : 29 Oct 2017 21:23
Operator : SJ/JU
Sample : I6094-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 30 08:04:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

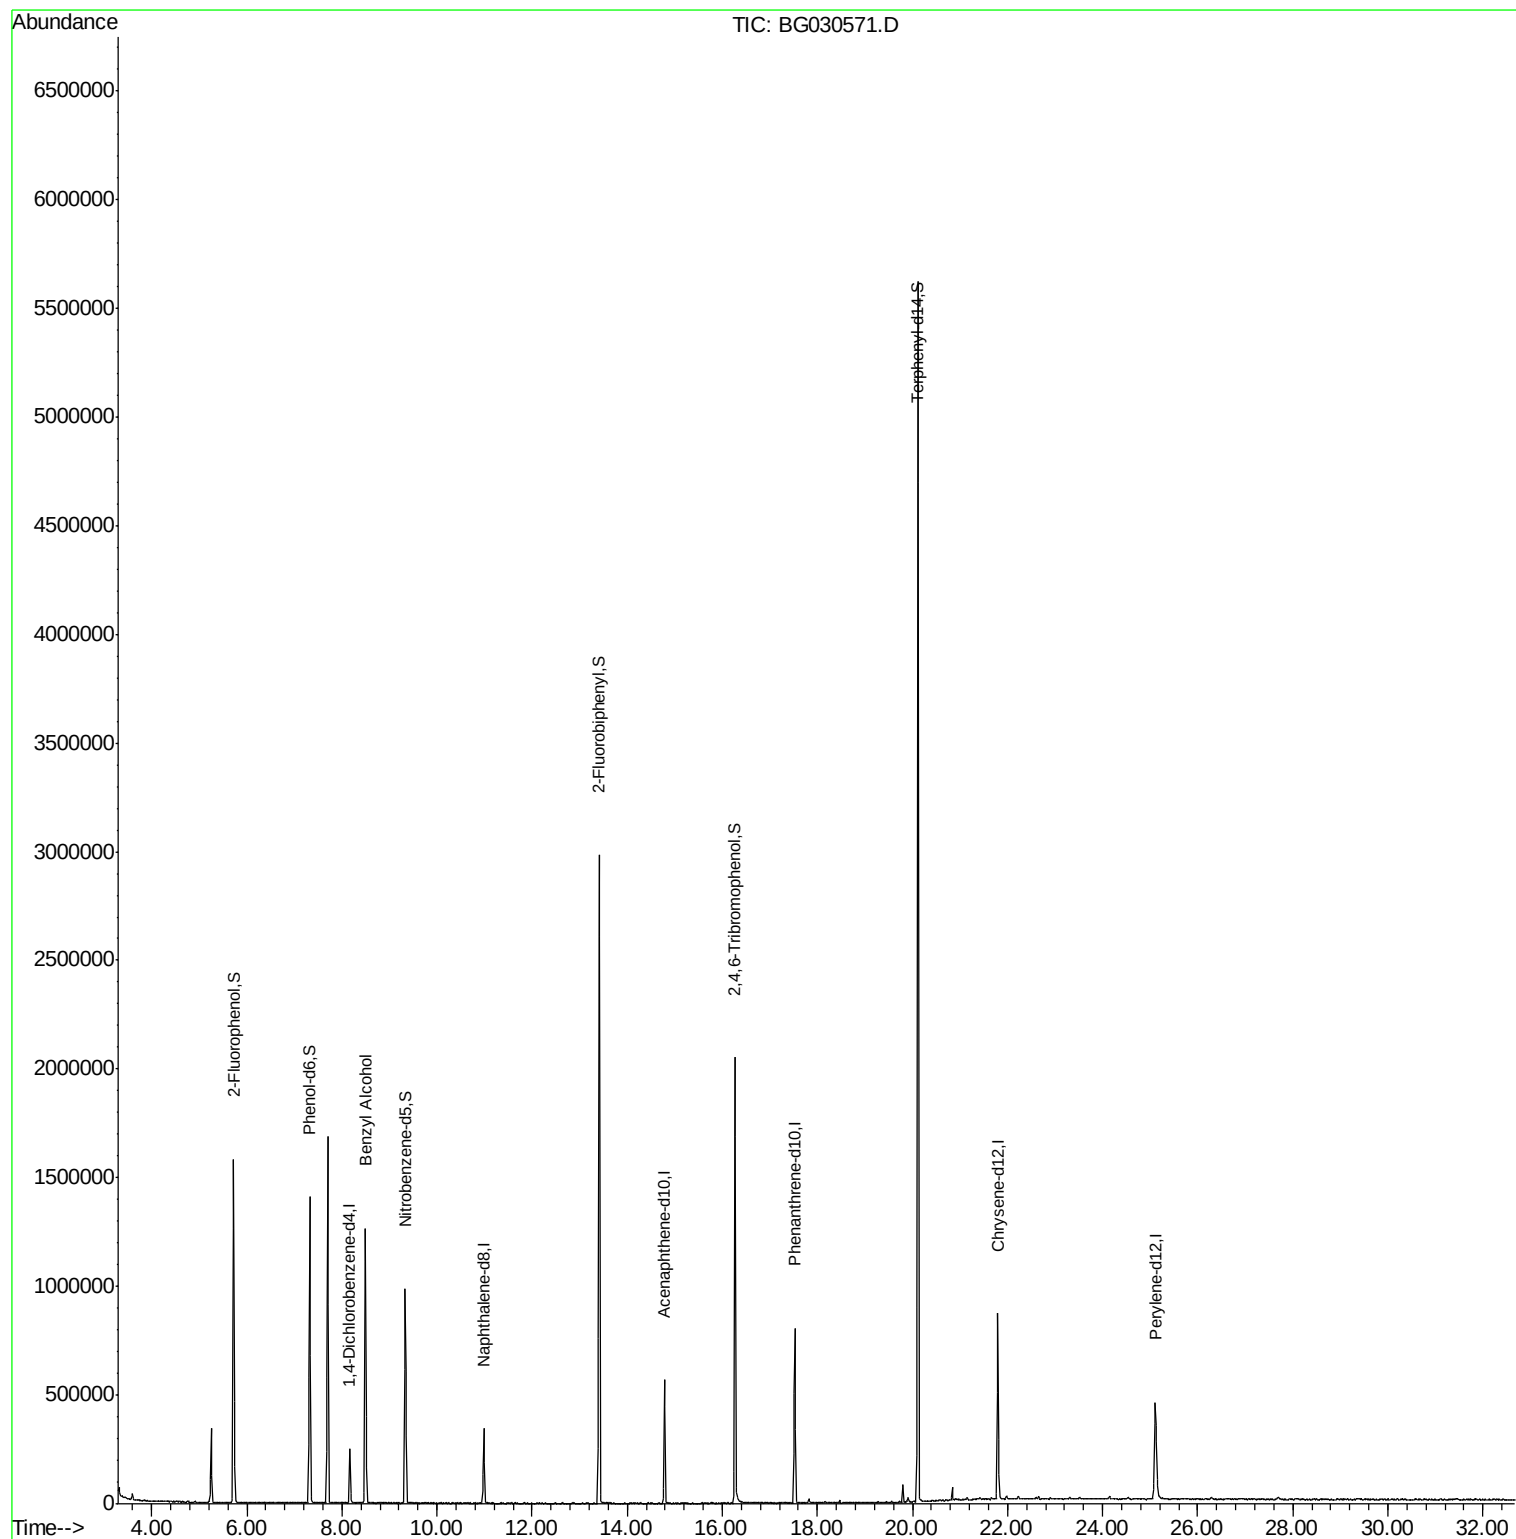




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 830
Delta R.T. -0.01 min
Lab File: BG030571.D
Acq: 29 Oct 2017 21:23

Instrument :
BNA_G
ClientSampled :

Tot Ion:152 Resp: 71364
Ion Ratio Lower Upper
152 100
150 157.8 126.6 189.8
115 58.3 53.0 79.4

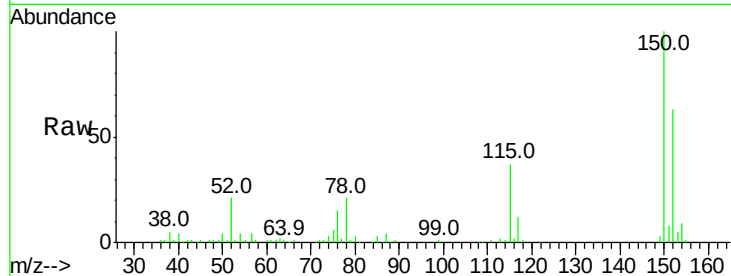


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

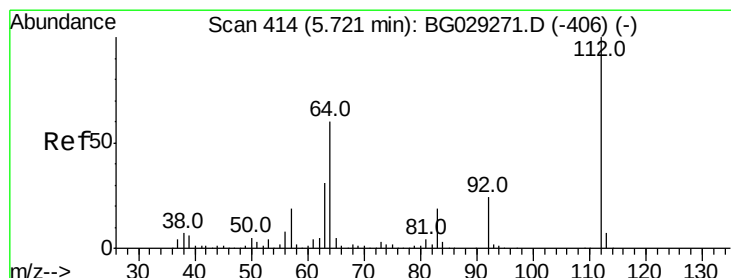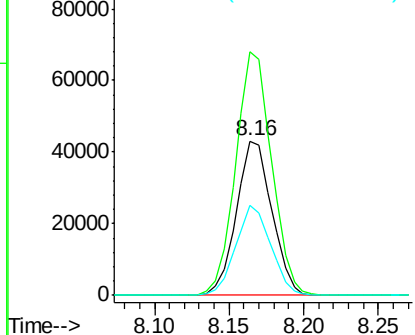



#5


2-Fluorophenol
Concen: 166.991 ng
RT: 5.72 min Scan# 414
Delta R.T. -0.00 min
Lab File: BG030571.D
Acq: 29 Oct 2017 21:23

Tgt Ion:112 Resp: 713365
Ion Ratio Lower Upper
112 100
64 59.8 56.3 84.5
63 31.9 30.1 45.1

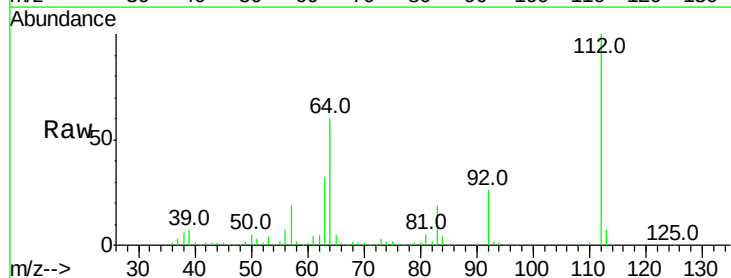

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

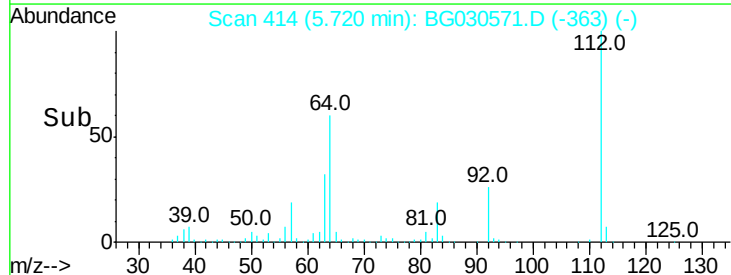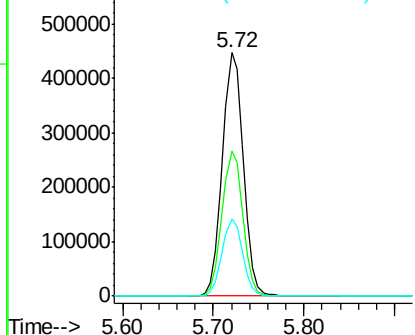

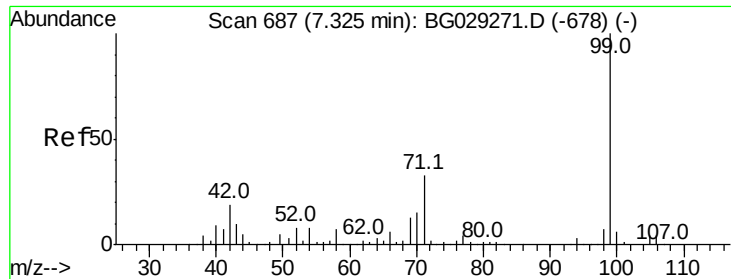

#7

Phenol-d6

Concen: 142.400 ng

RT: 7.32 min Scan# 687

Delta R.T. -0.00 min

Lab File: BG030571.D

Acq: 29 Oct 2017 21:23

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 853868

Ion Ratio Lower Upper




99 100

42 19.0 14.1 21.1

71 34.0 26.1 39.1

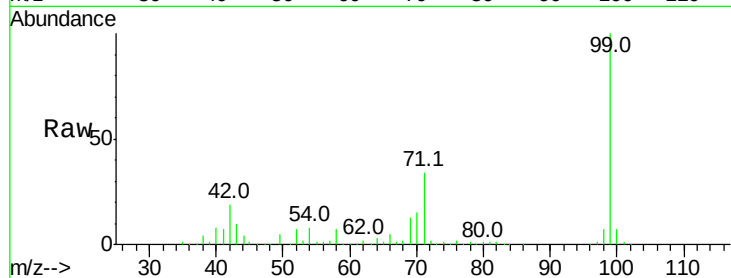

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

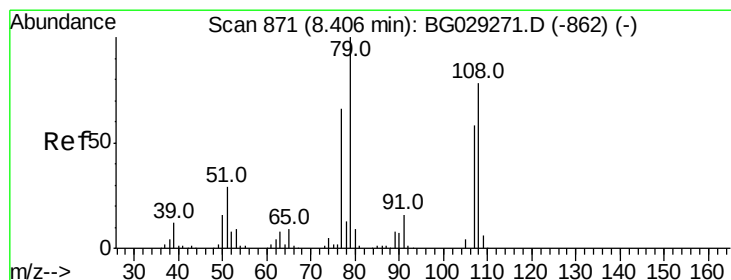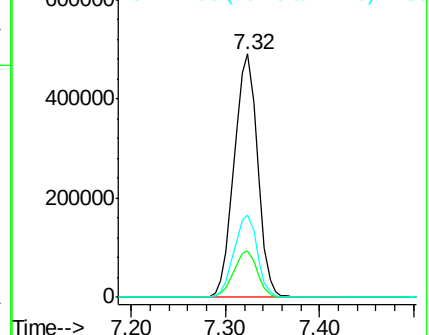

#15

Benzyl Alcohol

Concen: 2.342 ng

RT: 8.49 min Scan# 886

Delta R.T. 0.09 min

Lab File: BG030571.D

Acq: 29 Oct 2017 21:23


Tgt Ion: 79 Resp: 9898

Ion Ratio Lower Upper



79 100


108 40.3 57.2 85.8#

77 118.3 46.1 69.1#

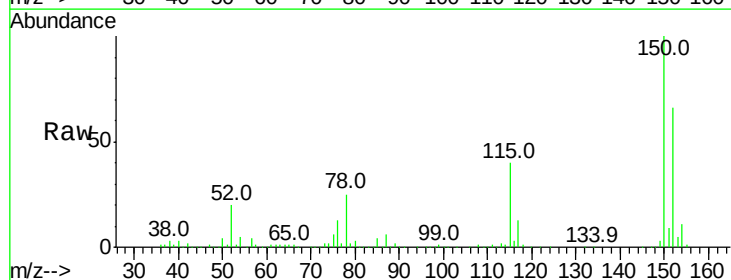

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

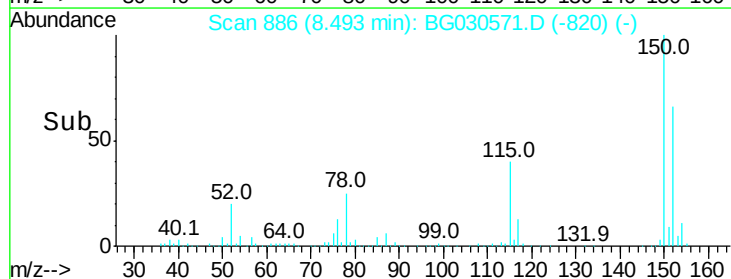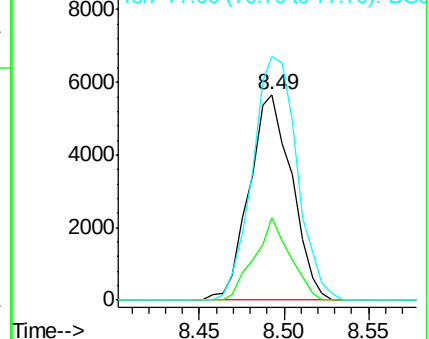







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.98 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BG030571.D
Acq: 29 Oct 2017 21:23

Instrument :
BNA_G
ClientSampled :

Tot Ion:136	Resp:	306923
Ion Ratio	Lower	Upper
136	100	
137	11.3	9.2 13.8
54	8.2	10.3 15.5#
68	6.4	4.5 6.7

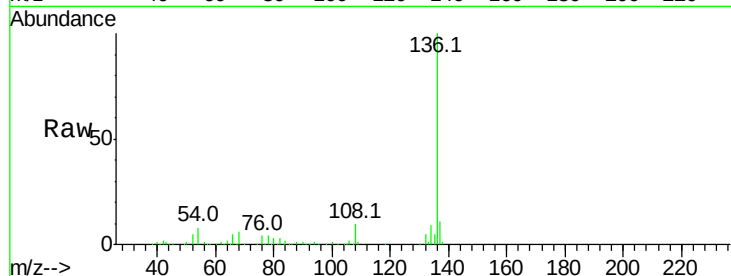


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

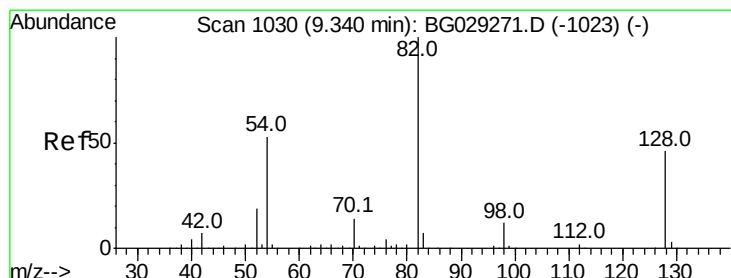
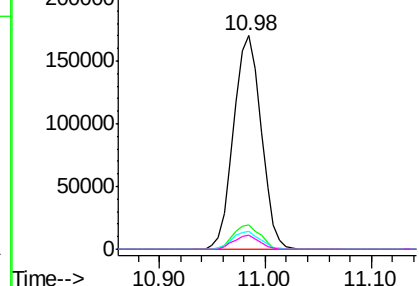



#23
Nitrobenzene-d5
Concen: 123.524 ng
RT: 9.33 min Scan# 1029
Delta R.T. -0.01 min
Lab File: BG030571.D
Acq: 29 Oct 2017 21:23

Tgt Ion: 82	Resp:	596600
Ion Ratio	Lower	Upper
82	100	
128	46.7	29.7 44.5#
54	52.6	43.1 64.7

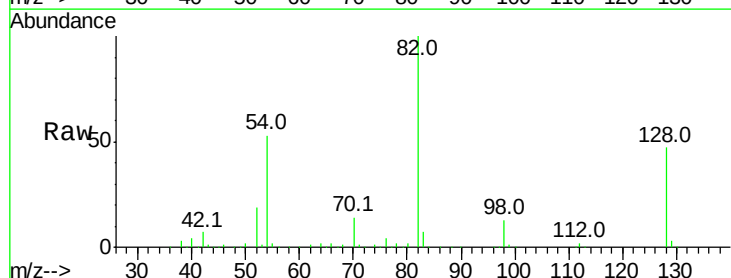

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

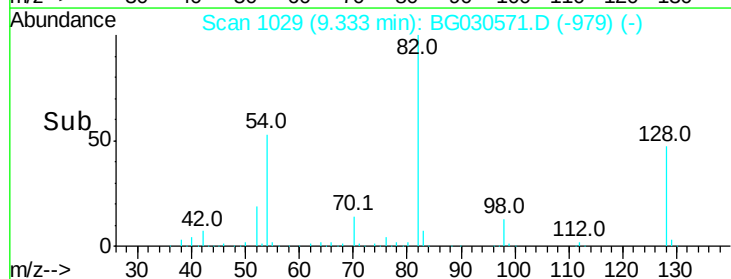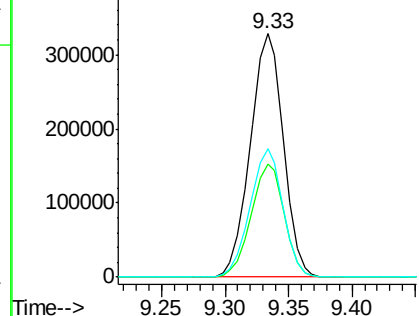







#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.78 min Scan# 1956
Delta R.T. -0.01 min
Lab File: BG030571.D
Acq: 29 Oct 2017 21:23

Instrument :
BNA_G
ClientSampleId :

Tot Ion:164 Resp: 204513
Ion Ratio Lower Upper
164 100
162 98.5 78.8 118.2
160 43.6 35.4 53.0

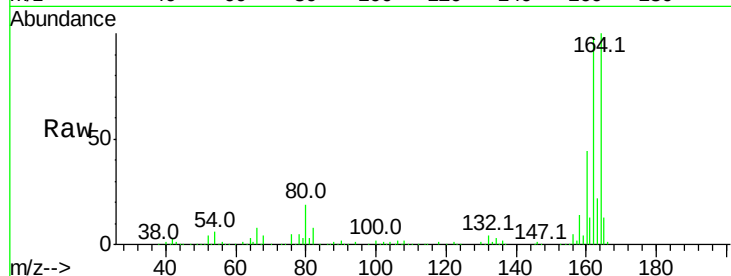


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

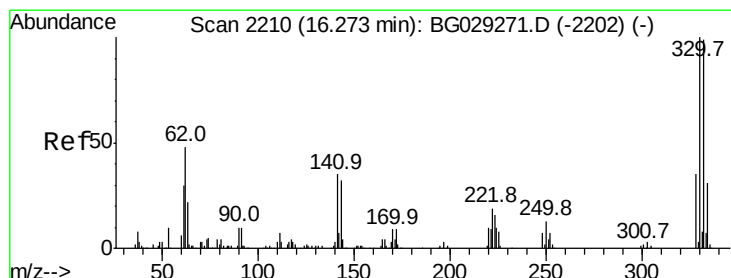
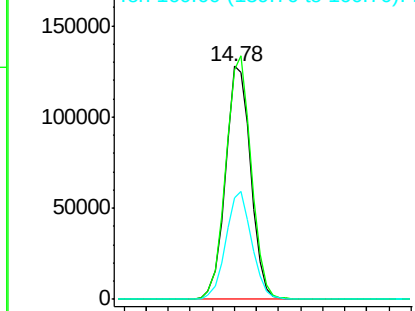



#41
2,4,6-Tribromophenol
Concen: 158.862 ng
RT: 16.27 min Scan# 2209
Delta R.T. -0.01 min
Lab File: BG030571.D
Acq: 29 Oct 2017 21:23

Tgt Ion:330 Resp: 419471
Ion Ratio Lower Upper
330 100
332 95.4 77.0 115.6
141 32.5 25.2 37.8

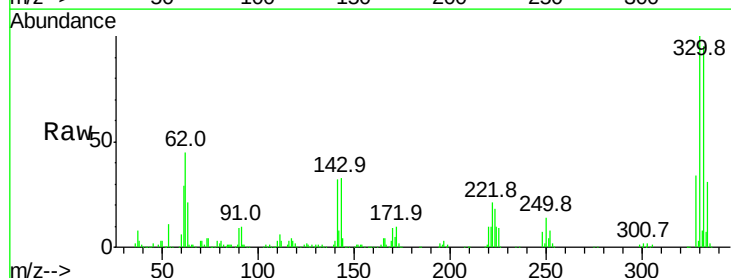

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

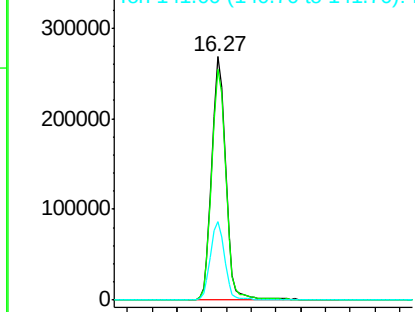




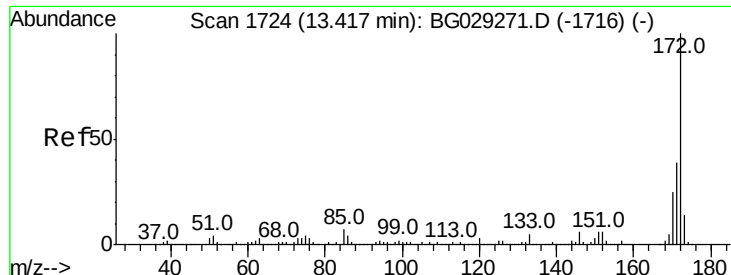


#44
 2-Fluorobiphenyl
 Concen: 112.652 ng
 RT: 13.41 min Scan# 1723
 Delta R.T. -0.01 min
 Lab File: BG030571.D
 Acq: 29 Oct 2017 21:23

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:172 Resp: 1570836




Ion	Ratio	Lower	Upper
172	100		
171	39.5	30.0	45.0
170	25.9	19.5	29.3

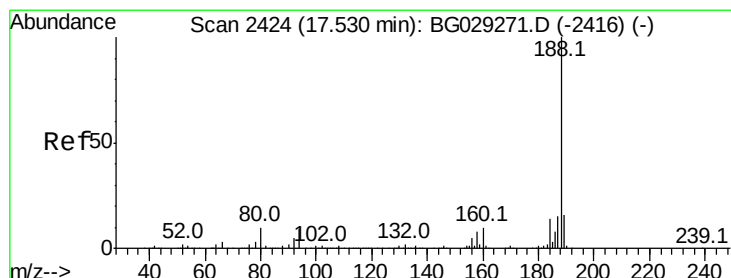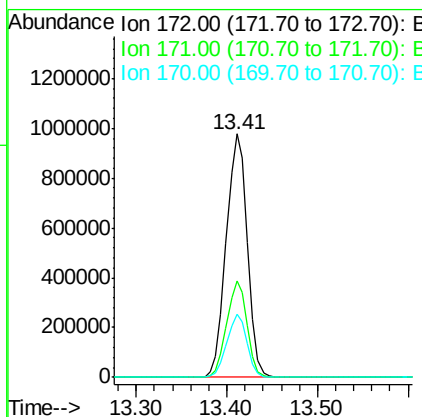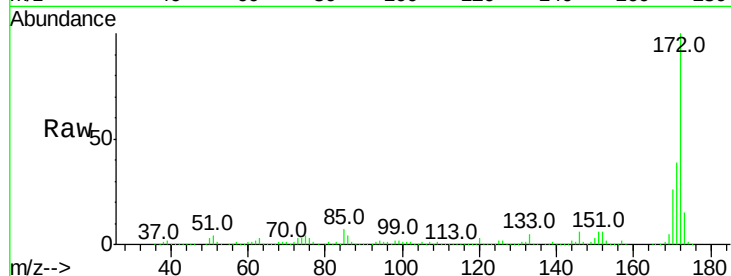


#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.52 min Scan# 2423
 Delta R.T. -0.01 min
 Lab File: BG030571.D
 Acq: 29 Oct 2017 21:23

Tgt Ion:188 Resp: 508448

Ion	Ratio	Lower	Upper
188	100		
94	8.9	6.9	10.3
80	9.3	7.7	11.5

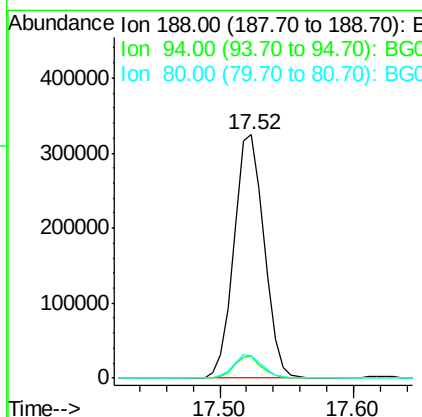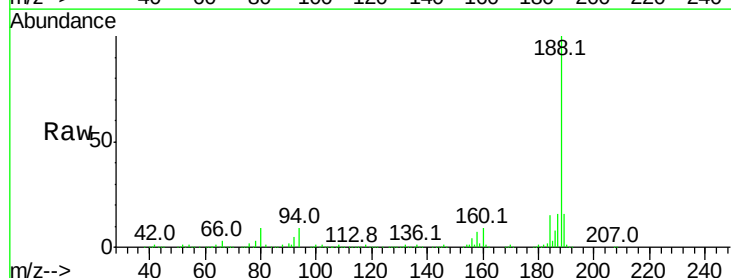

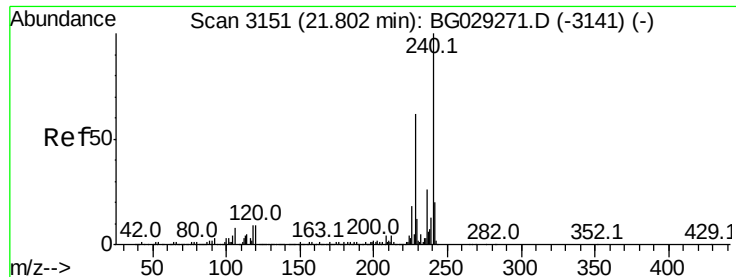

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.80 min Scan# 3150

Delta R.T. -0.01 min

Lab File: BG030571.D

Acq: 29 Oct 2017 21:23

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 541306

Ion Ratio Lower Upper

240 100

120 8.9 6.8 10.2




236 26.6 20.9 31.3

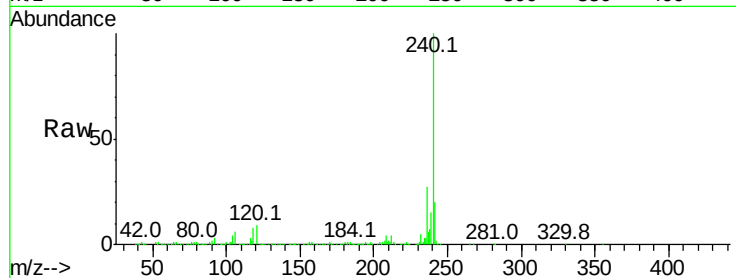

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

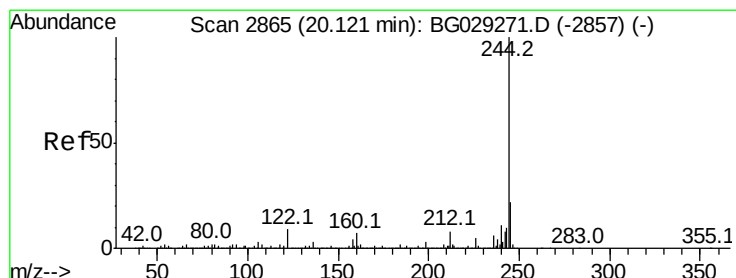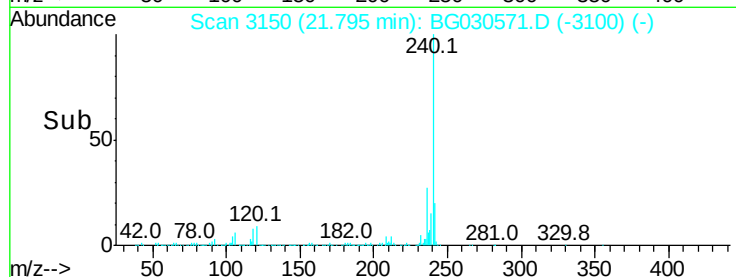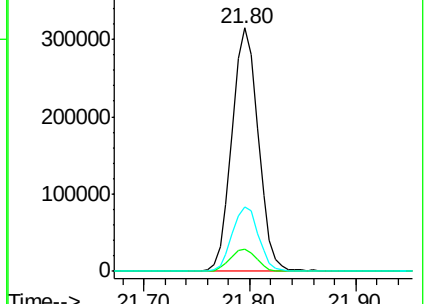

#78

Terphenyl-d14

Concen: 103.804 ng

RT: 20.11 min Scan# 2864

Delta R.T. -0.01 min

Lab File: BG030571.D

Acq: 29 Oct 2017 21:23


Tgt Ion:244 Resp: 2469946

Ion Ratio Lower Upper

244 100

212 9.4 5.8 8.8#



122 11.1 7.0 10.4#

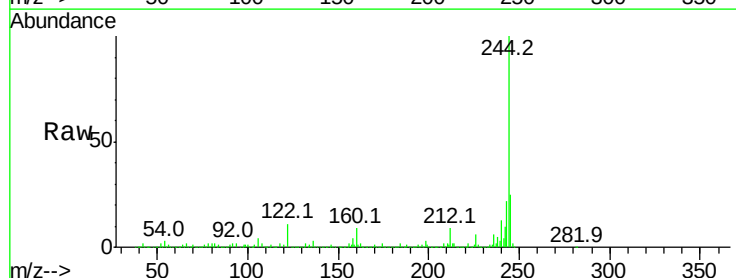


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

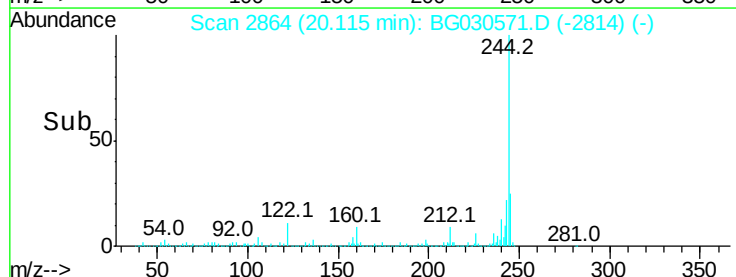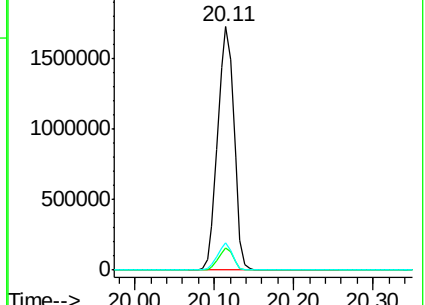


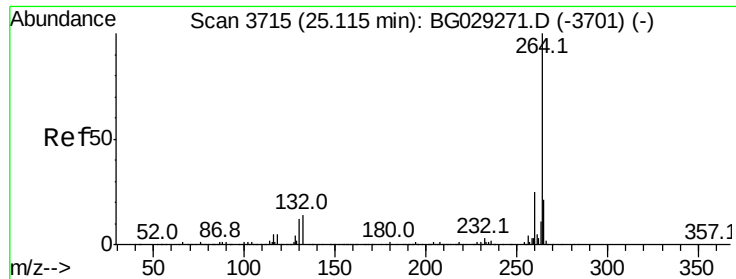

#86
Pervlene-d12
Concen: 20.000 ng
RT: 25.11 min Scan# 3714
Delta R.T. -0.01 min
Lab File: BG030571.D
Acq: 29 Oct 2017 21:23

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	17.4	26.0
265	21.8	17.7	26.5

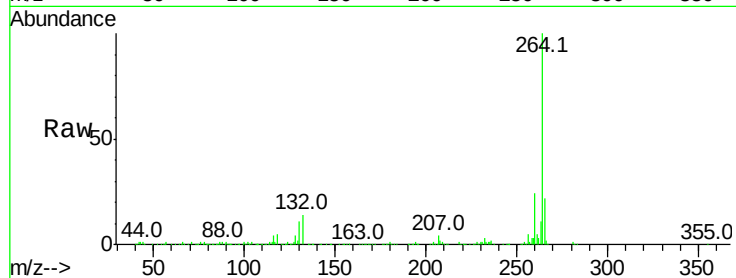

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

