


Data Path : Z:\HPCHEM1\BNA G\Data\BG102817\
 Data File : BG030540.D
 Acq On : 29 Oct 2017 00:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 16 17:32:15 2017

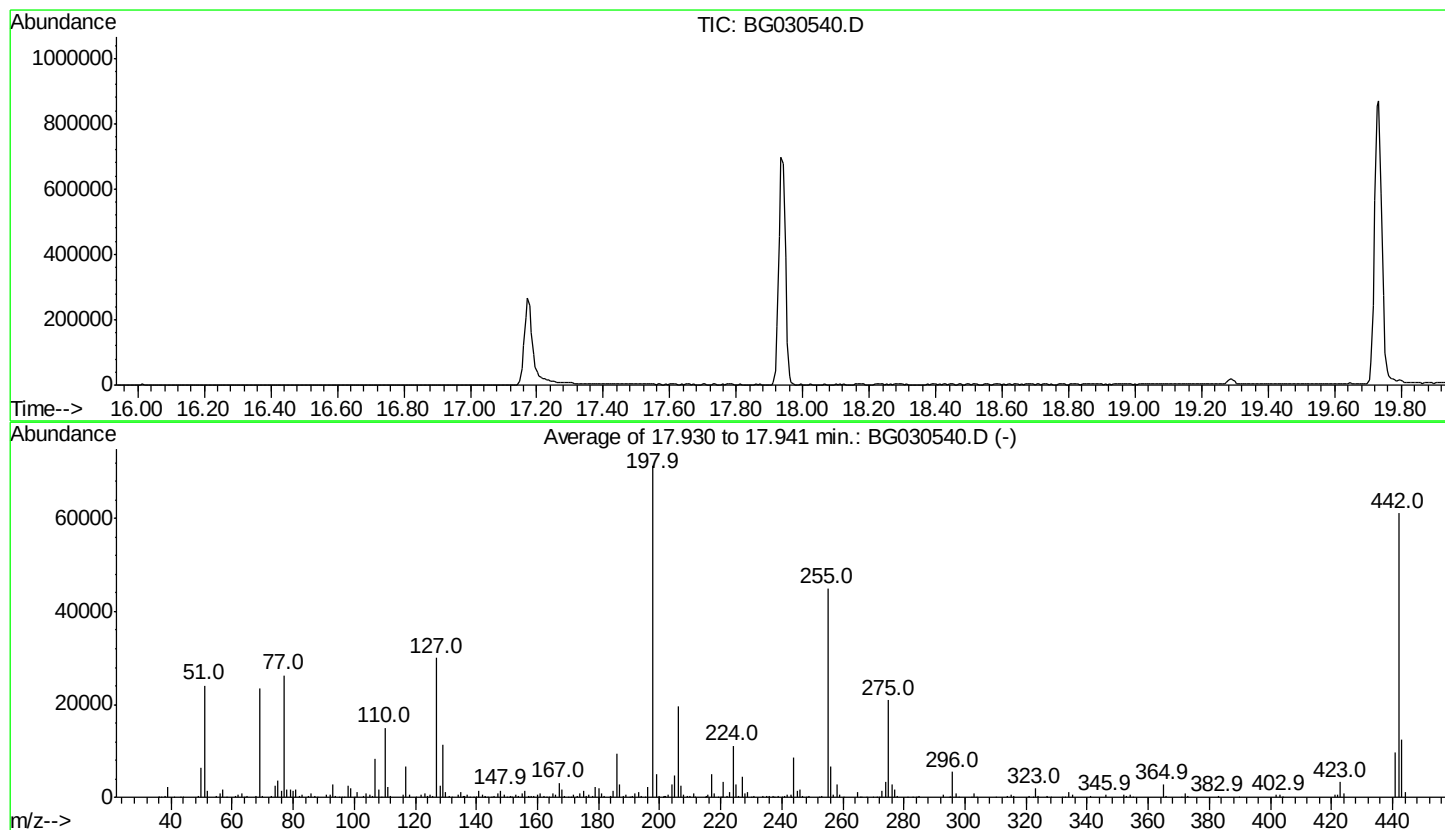

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	24050	PASS
68	69	0.00	2	0.7	173	PASS
69	198	0.00	100	32.9	23472	PASS
70	69	0.00	2	0.9	202	PASS
127	198	10	80	42.1	30053	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71440	PASS
199	198	5	9	7.0	4984	PASS
275	198	10	60	29.3	20910	PASS
365	198	1	100	3.8	2745	PASS
441	442	0.01	24	15.9	9705	PASS
442	198	50	100	85.7	61192	PASS
443	442	15	24	20.4	12481	PASS