


Data Path : Z:\HPCHEM1\BNA G\Data\BG102817\  
 Data File : BG030559.D  
 Acq On : 29 Oct 2017 13:21  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG101617.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Oct 16 17:32:15 2017

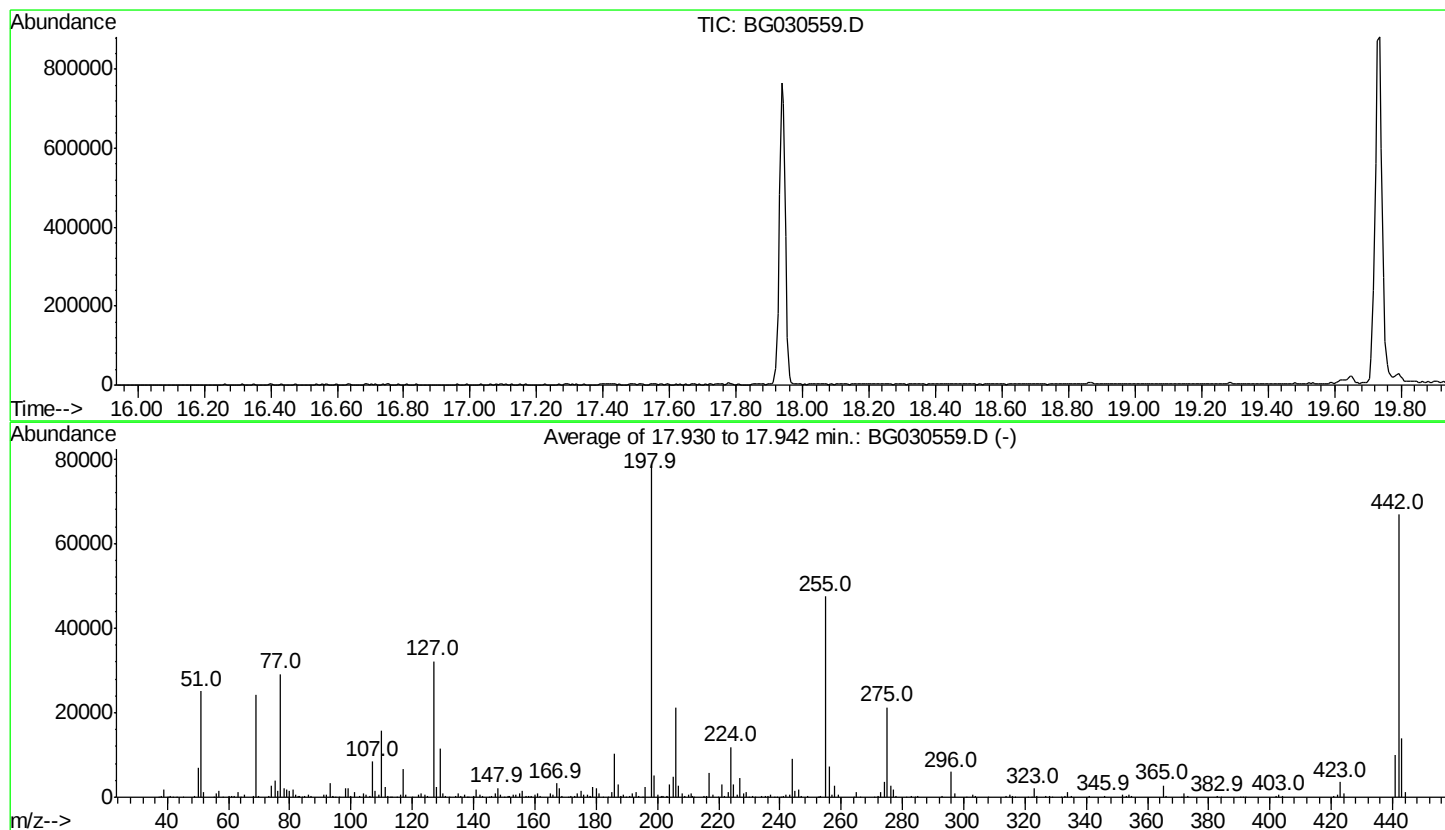

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 31.9      | 25026   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 323     | PASS             |
| 69          | 198          | 0.00         | 100          | 30.7      | 24114   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.8       | 198     | PASS             |
| 127         | 198          | 10           | 80           | 41.1      | 32216   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 78437   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 5264    | PASS             |
| 275         | 198          | 10           | 60           | 27.2      | 21328   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 2847    | PASS             |
| 441         | 442          | 0.01         | 24           | 14.9      | 9983    | PASS             |
| 442         | 198          | 50           | 100          | 85.3      | 66912   | PASS             |
| 443         | 442          | 15           | 24           | 20.7      | 13823   | PASS             |