

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102819\
 Data File : BG043357.D
 Acq On : 28 Oct 2019 19:35
 Operator : JU
 Sample : PB124310BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB124310BL

Quant Time: Oct 29 13:35:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 16:37:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	37120	20.00	ng	0.00
21) Naphthalene-d8	10.83	136	123601	20.00	ng	0.00
39) Acenaphthene-d10	14.65	164	101378	20.00	ng	0.00
64) Phenanthrene-d10	17.40	188	248129	20.00	ng	0.00
76) Chrysene-d12	21.66	240	274358	20.00	ng	0.00
87) Perylene-d12	24.86	264	318045	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	195581	96.55	ng	0.00
7) Phenol-d6	7.22	99	182785	62.72	ng	0.01
23) Nitrobenzene-d5	9.18	82	234056	97.63	ng	0.00
42) 2,4,6-Tribromophenol	16.14	330	266852	138.32	ng	0.00
45) 2-Fluorobiphenyl	13.27	172	665730	90.74	ng	0.00
79) Terphenyl-d14	20.01	244	1464469	100.14	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102819\
Data File : BG043357.D
Acq On : 28 Oct 2019 19:35
Operator : JU
Sample : PB124310BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124310BL

Quant Time: Oct 29 13:35:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

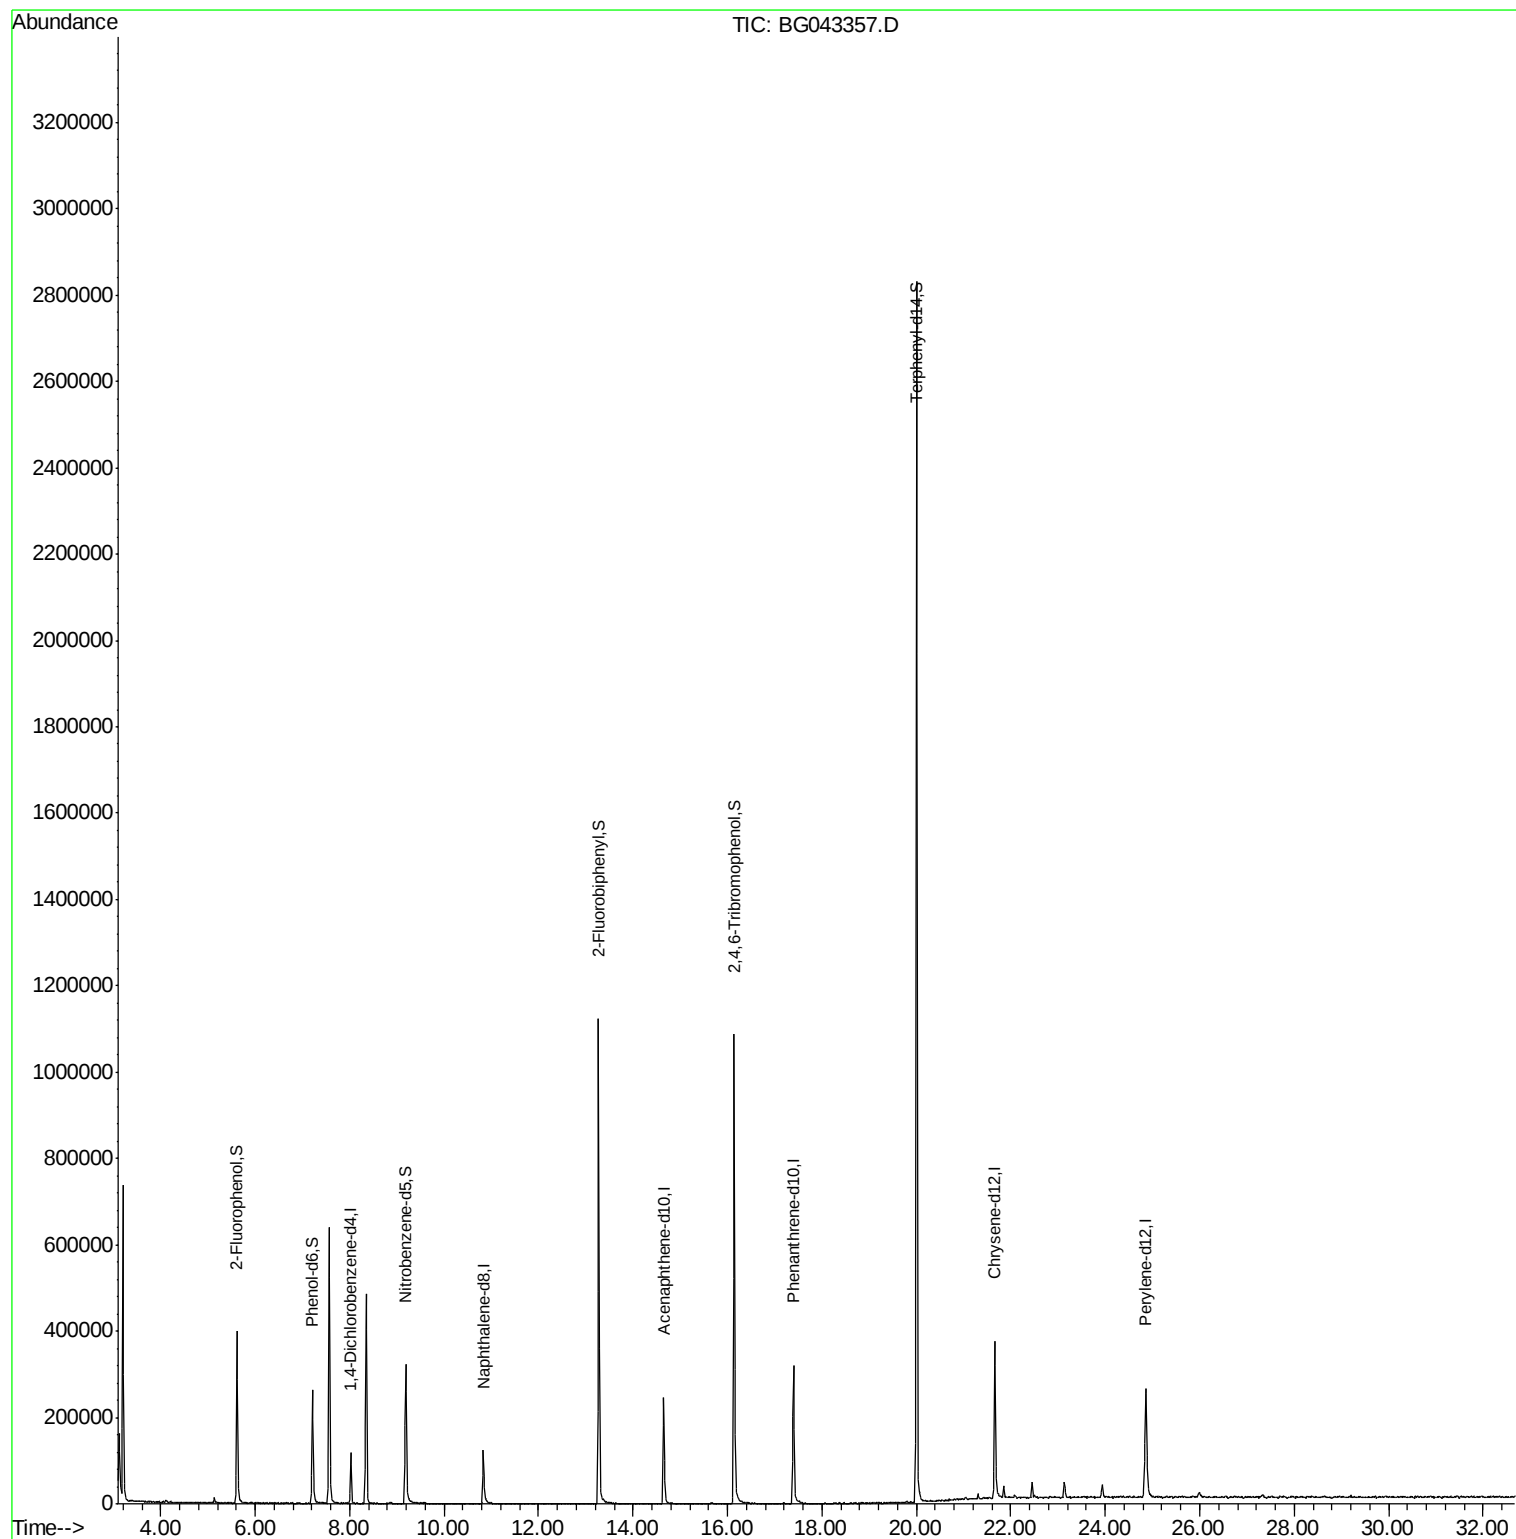




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.03 min Scan# 840
Delta R.T. 0.00 min
Lab File: BG043357.D
Acq: 28 Oct 2019 19:35

Instrument :
BNA_G
ClientSampleId :
PB124310BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.2	113.6	170.4
115	59.8	45.9	68.9



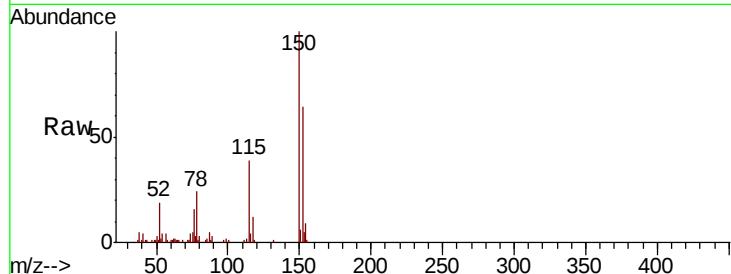


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

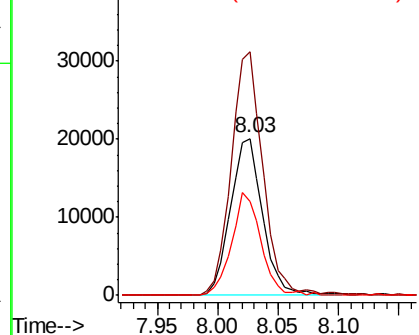

#5

2-Fluorophenol
Concen: 96.550 ng
RT: 5.61 min Scan# 428
Delta R.T. 0.01 min
Lab File: BG043357.D
Acq: 28 Oct 2019 19:35

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.9	50.2	75.2
63	32.2	26.7	40.1






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

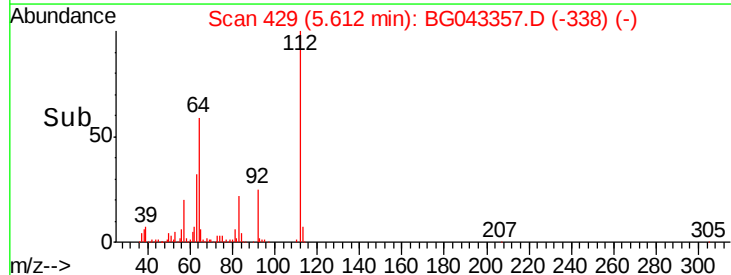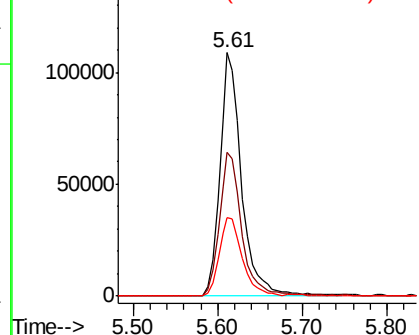



#7

Phenol-d6

Concen: 62.715 ng

RT: 7.22 min Scan# 702

Delta R.T. 0.01 min

Lab File: BG043357.D

Acq: 28 Oct 2019 19:35

Instrument :

BNA_G

ClientSampleId :

PB124310BL


Tot Ion: 99 Resp: 182785

Ion Ratio Lower Upper




99 100

42 17.9 14.9 22.3

71 39.4 32.2 48.2

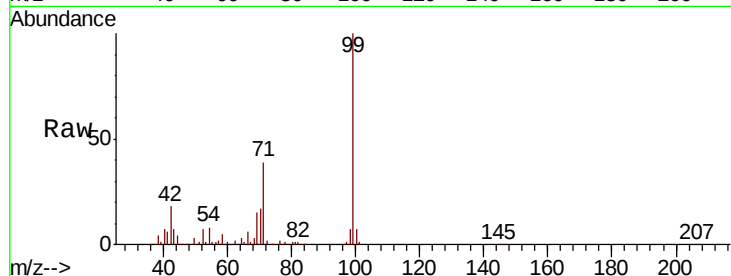

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

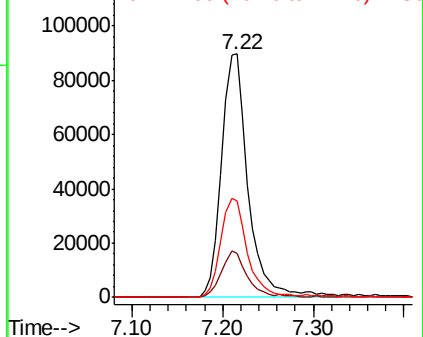

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1317

Delta R.T. 0.00 min

Lab File: BG043357.D

Acq: 28 Oct 2019 19:35

Tgt Ion: 136 Resp: 123601


Ion Ratio Lower Upper

136 100



137 13.0 8.2 12.2#


54 8.0 5.4 8.2

68 3.1 3.3 4.9#



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




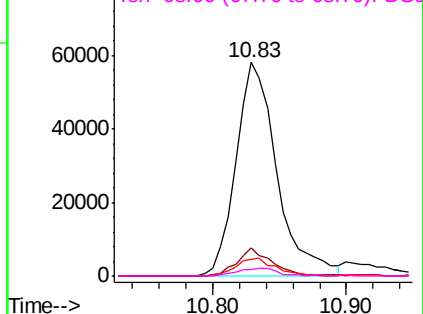




#23
Nitrobenzene-d5
Concen: 97.626 ng
RT: 9.18 min Scan# 1037
Delta R.T. -0.00 min
Lab File: BG043357.D
Acq: 28 Oct 2019 19:35




Instrument :
BNA_G
ClientSampled :
PB124310BL


Tot Ion	82	Resp	234056
Ion Ratio	Lower	Upper	
82	100		
128	40.8	35.3	52.9
54	49.4	42.3	63.5

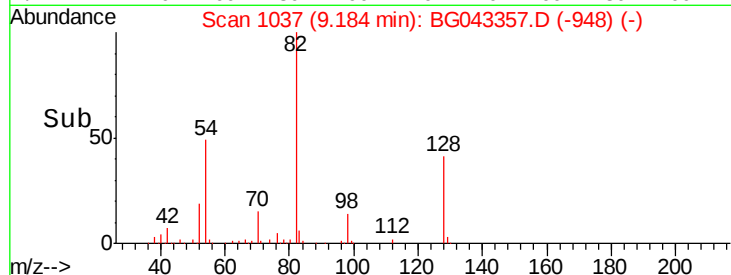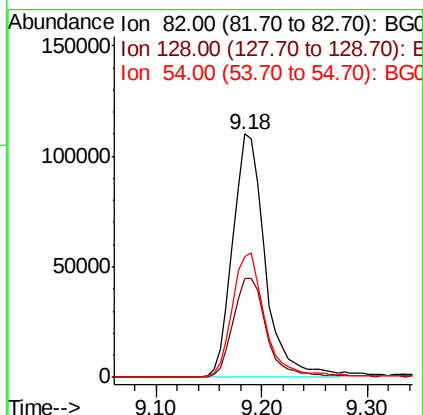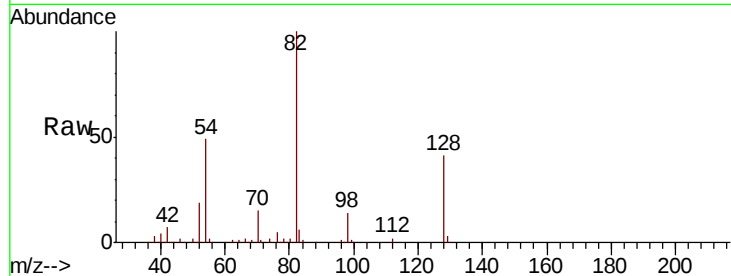

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.65 min Scan# 1967
Delta R.T. -0.00 min
Lab File: BG043357.D
Acq: 28 Oct 2019 19:35

Tgt Ion	164	Resp	101378
Ion Ratio	Lower	Upper	
164	100		
162	106.8	87.0	130.4
160	46.5	35.5	53.3

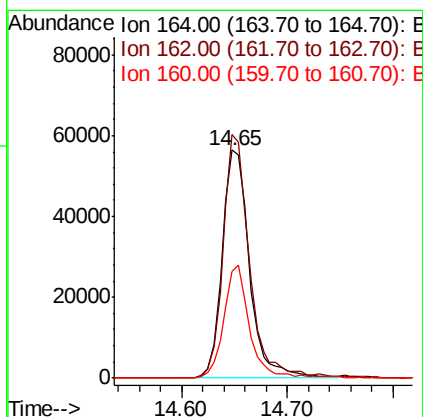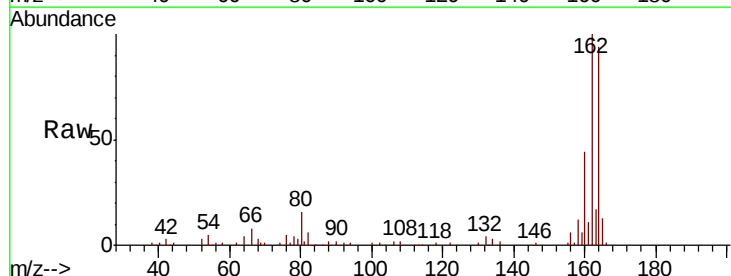


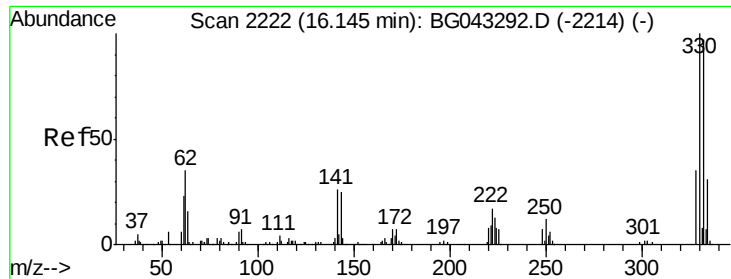

#42
 2,4,6-Tribromophenol
 Concen: 138.321 ng
 RT: 16.14 min Scan# 2221
 Delta R.T. -0.00 min
 Lab File: BG043357.D
 Acq: 28 Oct 2019 19:35

Instrument :
 BNA_G
 ClientSampleId :
 PB124310BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	76.4	114.6
141	28.5	21.4	32.0






Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

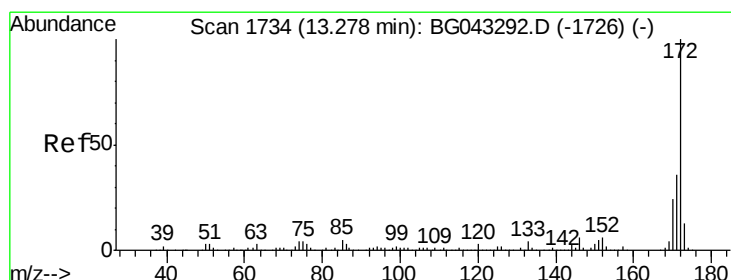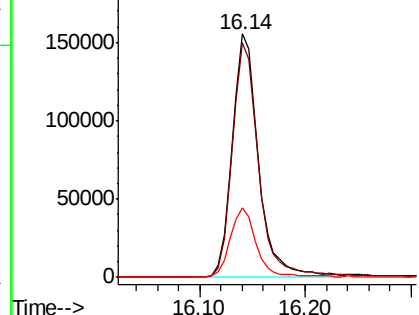

#45
 2-Fluorobiphenyl
 Concen: 90.740 ng
 RT: 13.27 min Scan# 1733
 Delta R.T. -0.00 min
 Lab File: BG043357.D
 Acq: 28 Oct 2019 19:35

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.5	42.7
170	23.4	18.8	28.2


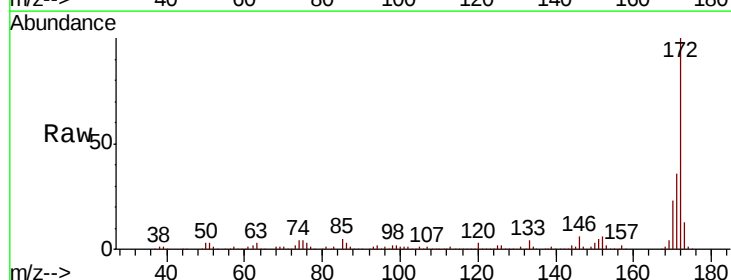



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

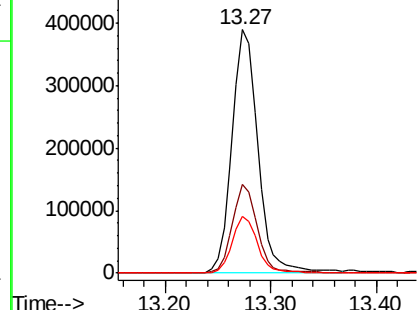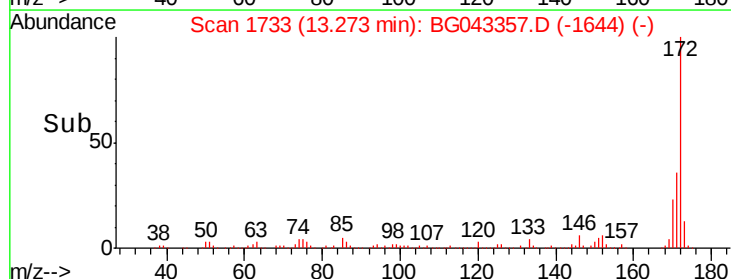



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2435

Delta R.T. -0.00 min

Lab File: BG043357.D

Acq: 28 Oct 2019 19:35

Instrument :

BNA_G

ClientSampleId :

PB124310BL


Tot Ion:188 Resp: 248129

Ion Ratio Lower Upper

188 100

94 5.4 4.2 6.2




80 6.8 5.2 7.8

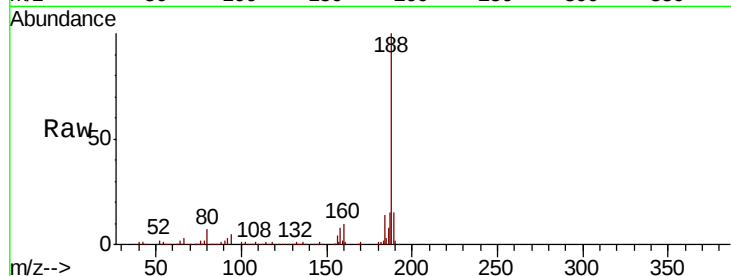

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

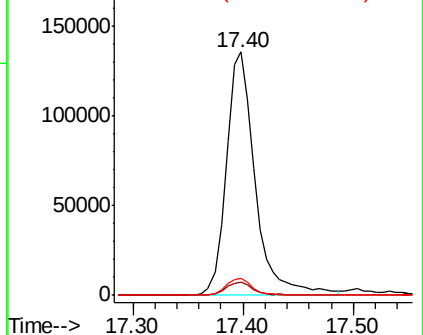

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.66 min Scan# 3161

Delta R.T. -0.00 min

Lab File: BG043357.D

Acq: 28 Oct 2019 19:35


Tgt Ion:240 Resp: 274358

Ion Ratio Lower Upper

240 100

120 5.1 4.6 7.0



236 27.2 20.2 30.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

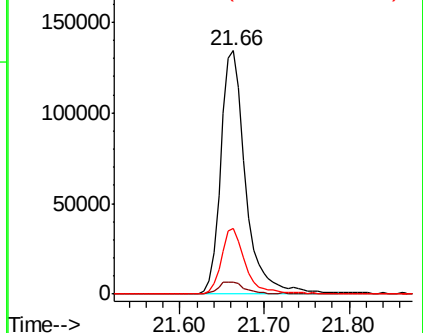

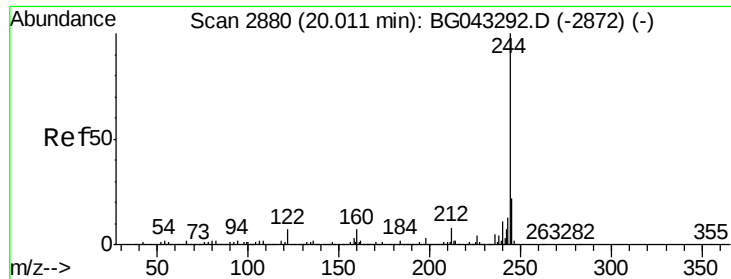

#79

Terphenyl-d14

Concen: 100.140 ng

RT: 20.01 min Scan# 2879

Delta R.T. -0.00 min

Lab File: BG043357.D

Acq: 28 Oct 2019 19:35

Instrument :

BNA_G

ClientSampled :

PB124310BL


Tot Ion:244 Resp: 1464469

Ion Ratio Lower Upper

244 100

212 7.5 6.4 9.6




122 6.6 5.3 7.9



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

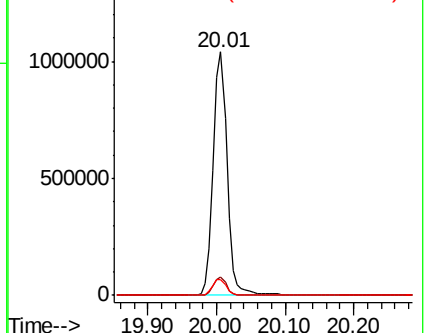

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.86 min Scan# 3705

Delta R.T. -0.01 min

Lab File: BG043357.D

Acq: 28 Oct 2019 19:35


Tgt Ion:264 Resp: 318045

Ion Ratio Lower Upper

264 100

260 24.4 17.9 26.9

265 24.2 17.4 26.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

