
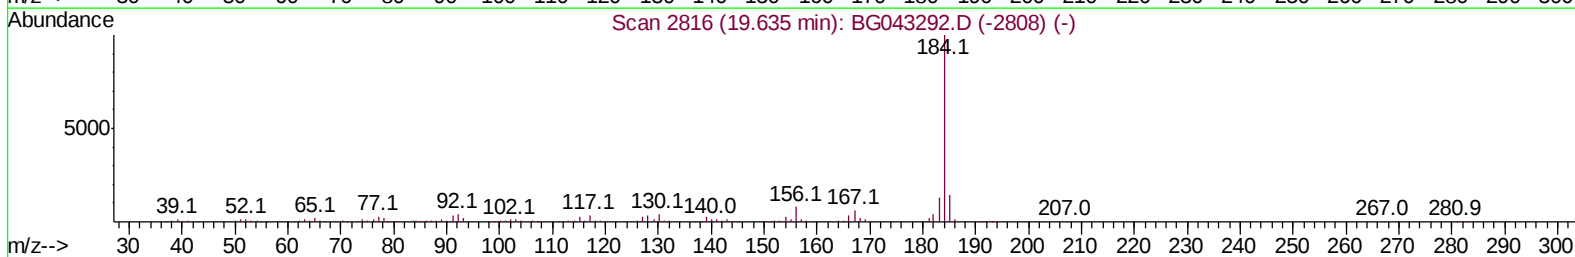
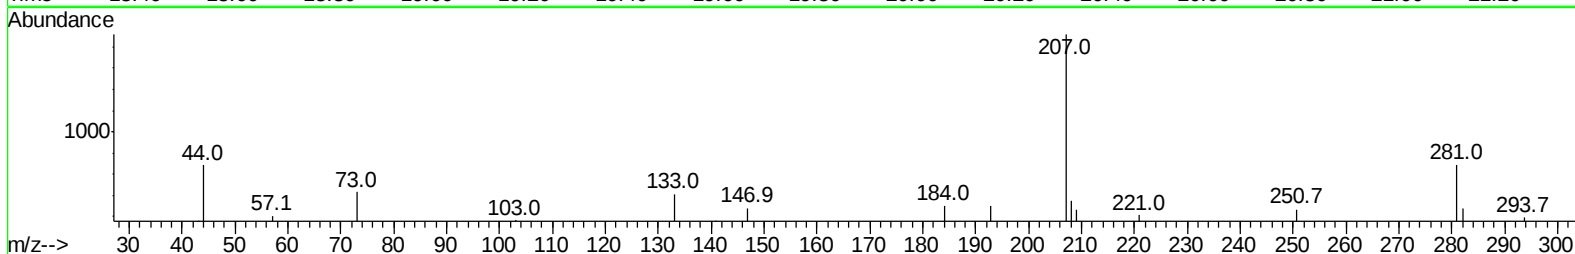


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102819\
Data File : BG043349.D
Acq On : 28 Oct 2019 14:27
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 15:26:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

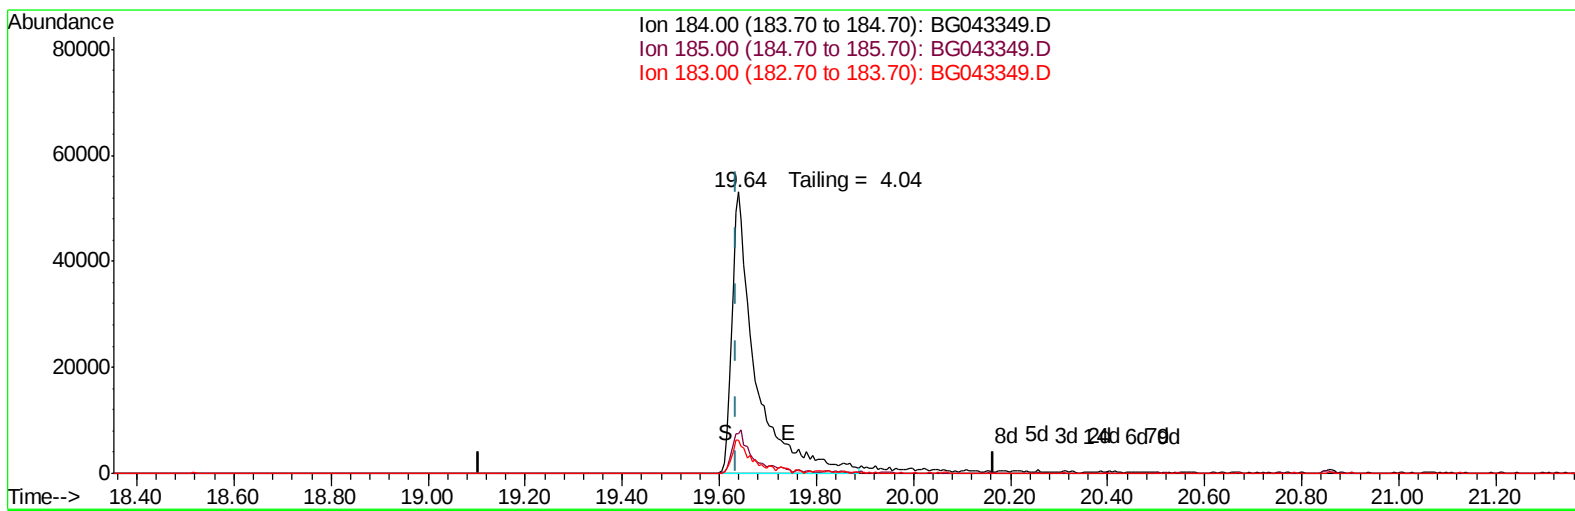

TIC: BG043349.D

(77) Benzidine




20.362min (+0.727) 349.60ng

response 394

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102819\
Data File : BG043349.D
Acq On : 28 Oct 2019 14:27
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 15:26:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

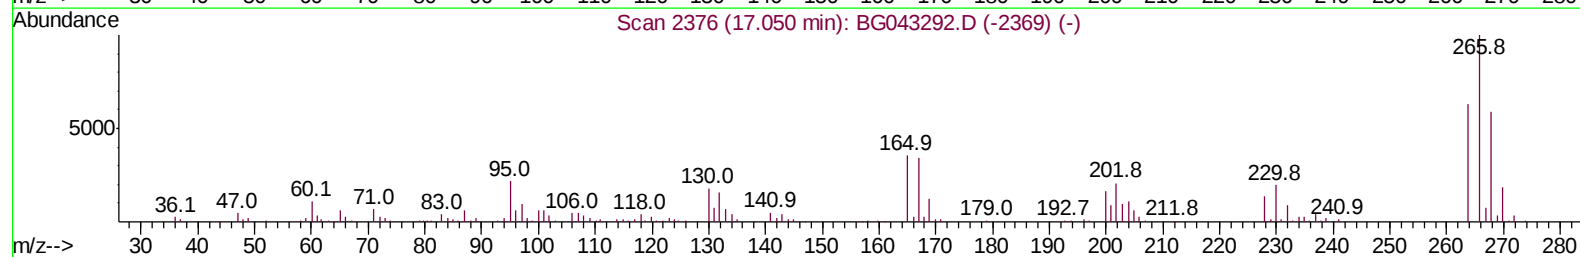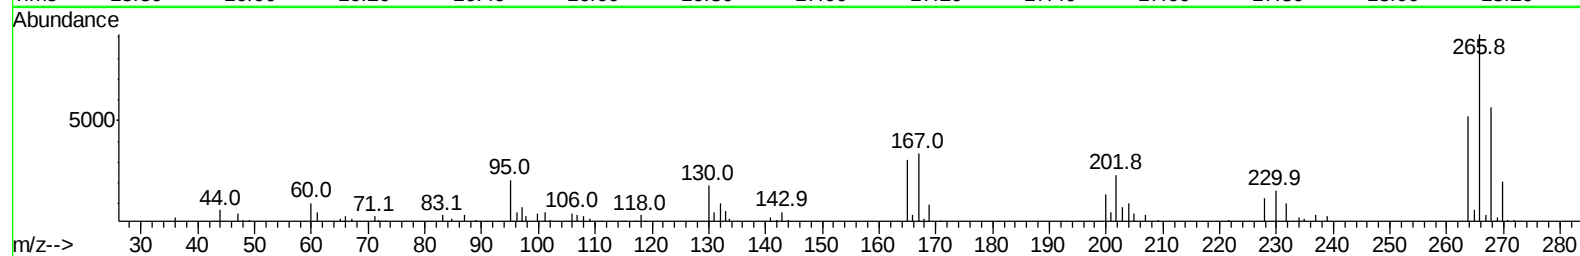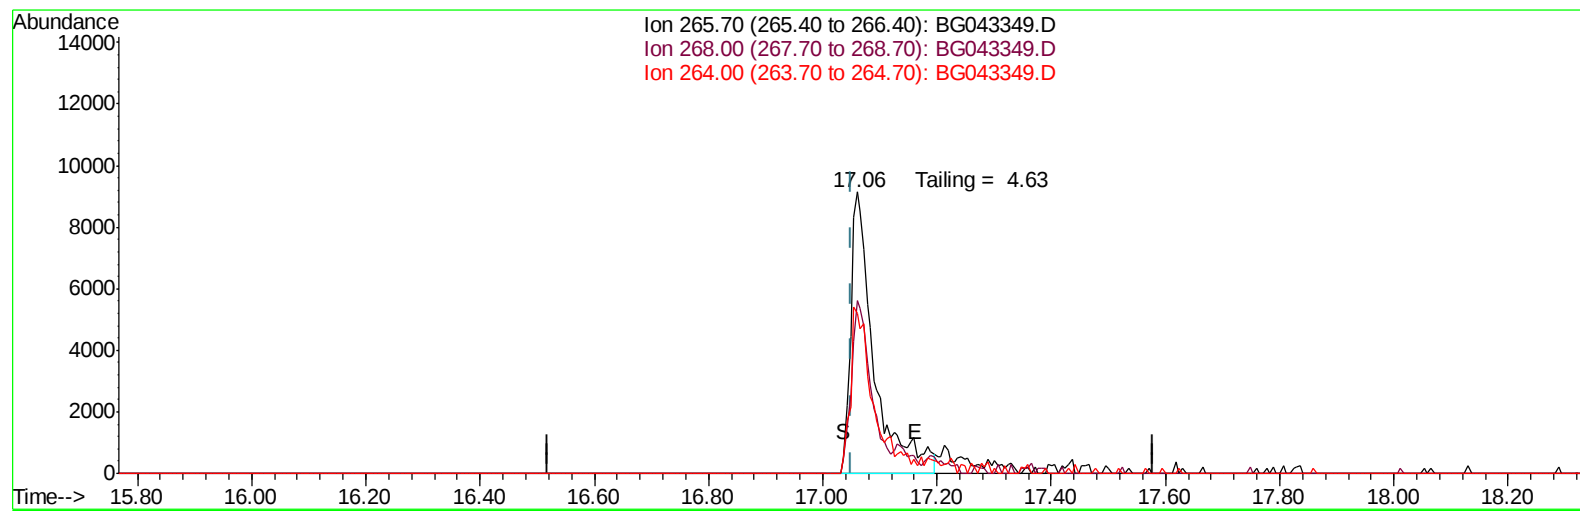

TIC: BG043349.D

(70) Pentachlorophenol (C)

17.060min (+0.010) 16400.40ng

response 24012

Ion	Exp%	Act%
265.70	100	100
268.00	58.90	61.56
264.00	63.00	56.83
0.00	0.00	0.00