

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102819\
 Data File : BG043355.D
 Acq On : 28 Oct 2019 18:18
 Operator : JU
 Sample : PB124295BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB124295BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.617	423	430	443	rBV	291073	541735	12.70%	4.434%
2	7.215	694	702	714	rBV	280075	568678	13.34%	4.654%
3	7.568	755	762	773	rBV	327244	597866	14.02%	4.893%
4	8.026	832	840	850	rBV	118917	223956	5.25%	1.833%
5	8.349	885	895	904	rBV	273218	493021	11.56%	4.035%
6	9.183	1030	1037	1048	rBV	148330	334058	7.83%	2.734%
7	10.828	1309	1317	1339	rBV	123331	280318	6.57%	2.294%
8	13.273	1726	1733	1748	rBV	517888	945142	22.16%	7.735%
9	14.653	1960	1968	1974	rBV	259613	446747	10.48%	3.656%
10	16.140	2214	2221	2243	rBV	571531	1069686	25.08%	8.754%
11	17.397	2427	2435	2446	rBV2	328232	605473	14.20%	4.955%
12	20.006	2872	2879	2895	rBV	3136450	4264520	100.00%	34.901%
13	21.663	3153	3161	3178	rBV2	398849	805444	18.89%	6.592%
14	22.450	3289	3295	3300	rBV3	37525	63064	1.48%	0.516%
15	23.138	3407	3412	3418	rBV3	35240	63215	1.48%	0.517%
16	23.931	3541	3547	3557	rVB4	26867	64775	1.52%	0.530%
17	24.859	3695	3705	3718	rBV2	271645	851257	19.96%	6.967%


Sum of corrected areas: 12218955

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102819\
Data File : BG043355.D
Acq On : 28 Oct 2019 18:18
Operator : JU
Sample : PB124295BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124295BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

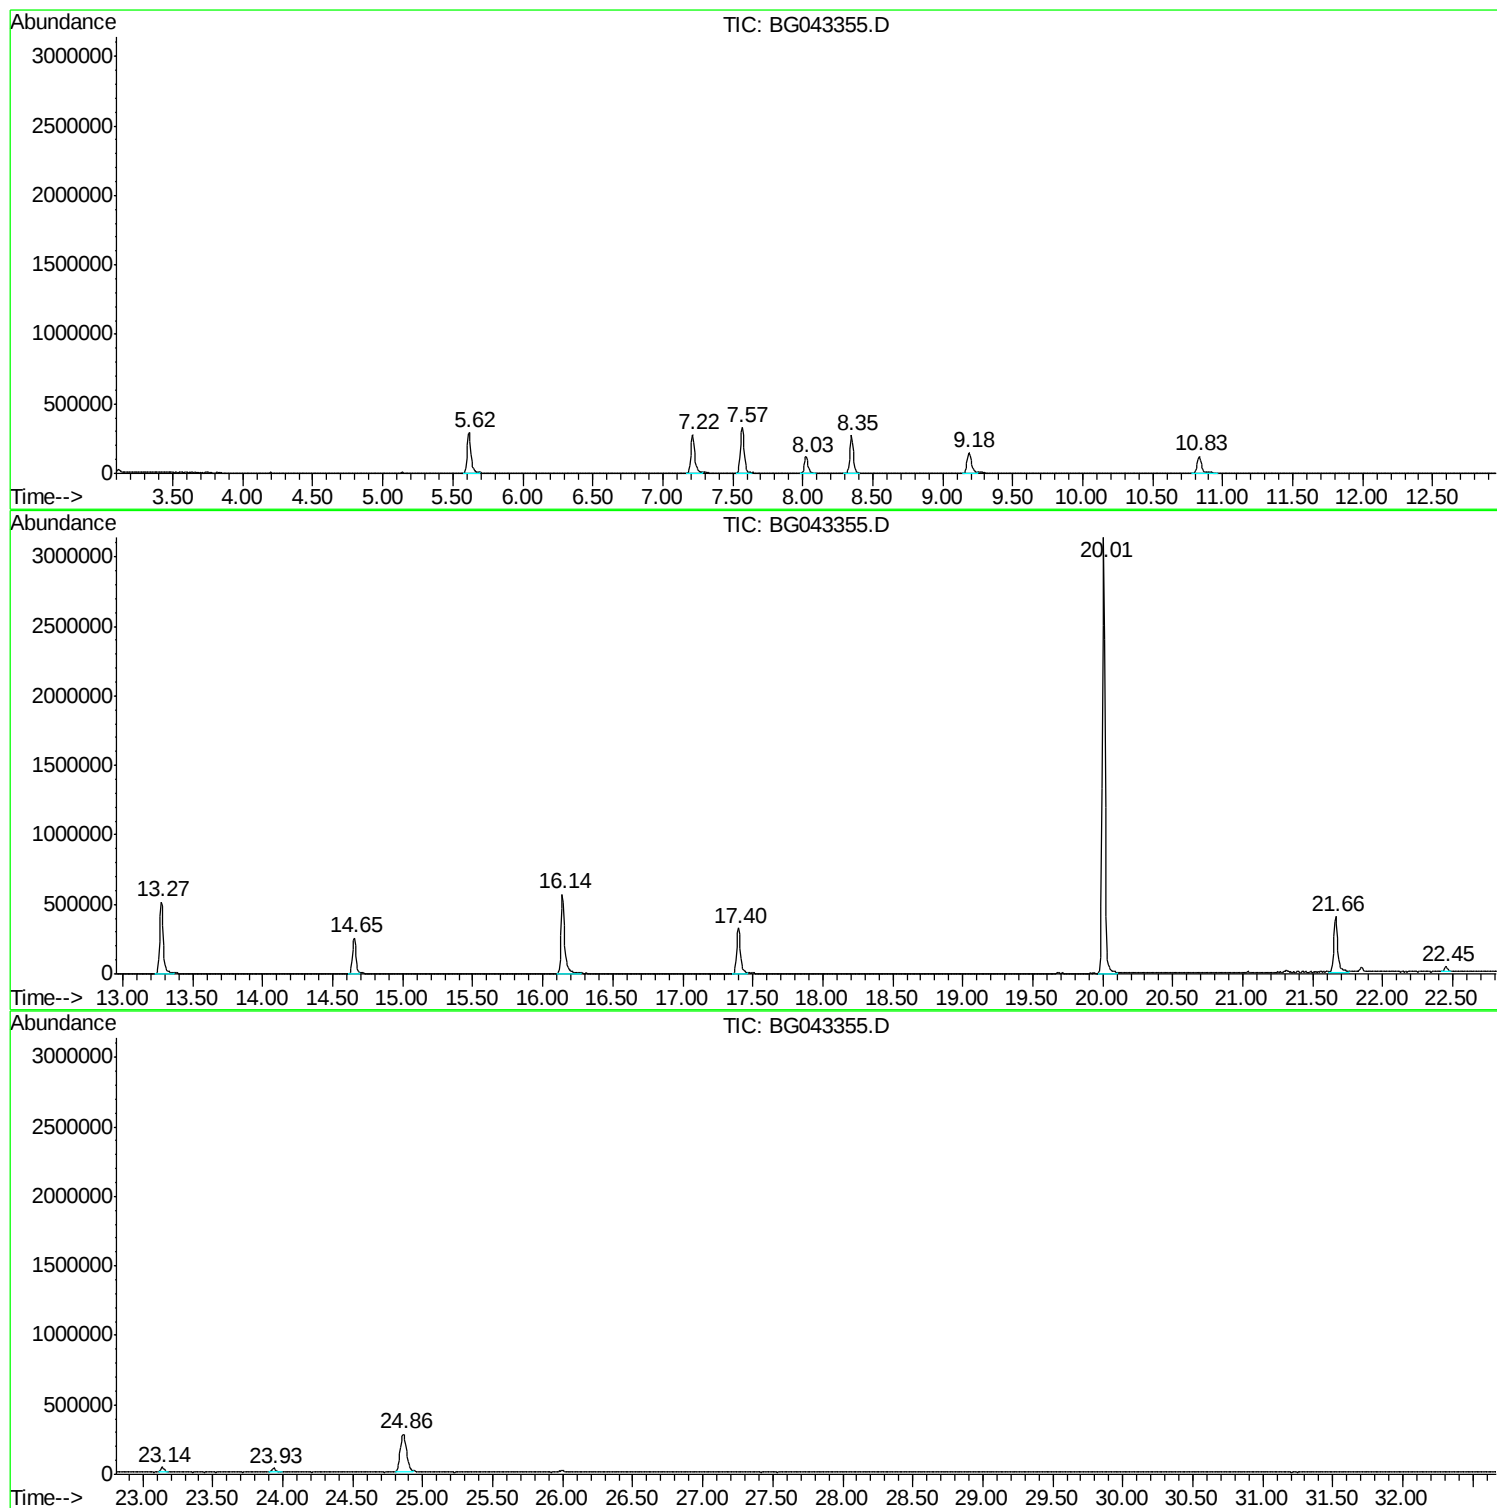

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102819\
Data File : BG043355.D
Acq On : 28 Oct 2019 18:18
Operator : JU
Sample : PB124295BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124295BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.57 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.57	53.39 ng	597866	1,4-Dichlorobenzene-d4	8.03

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	47
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
4		5-Aminoindole	132	C8H8N2	005192-03-0	22
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	12

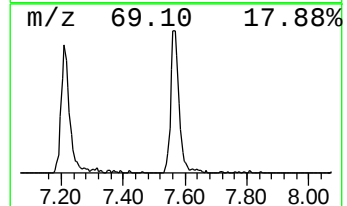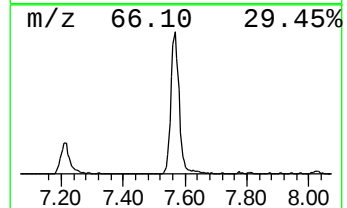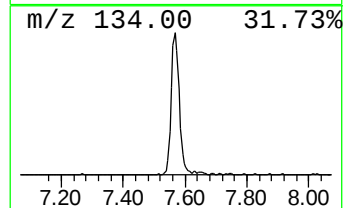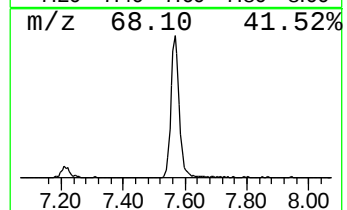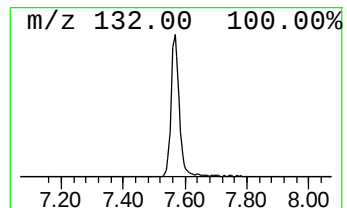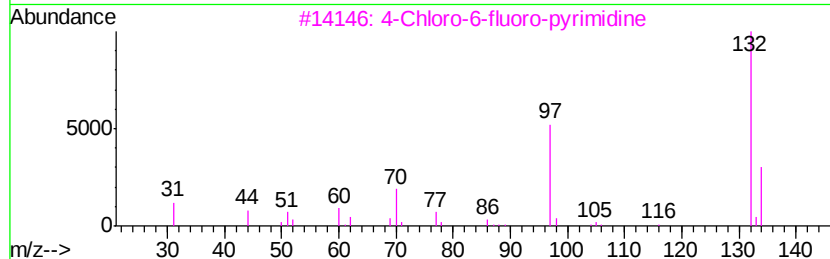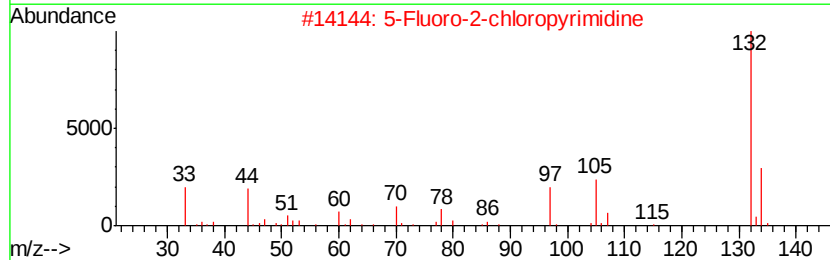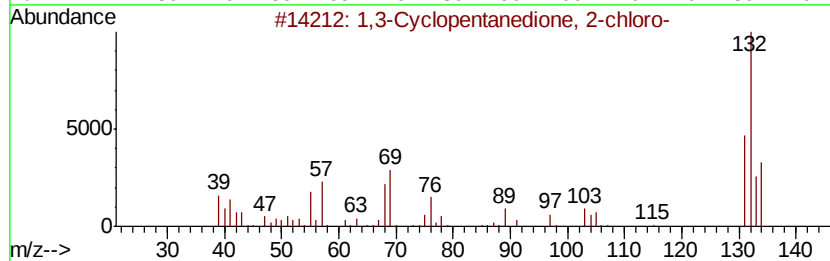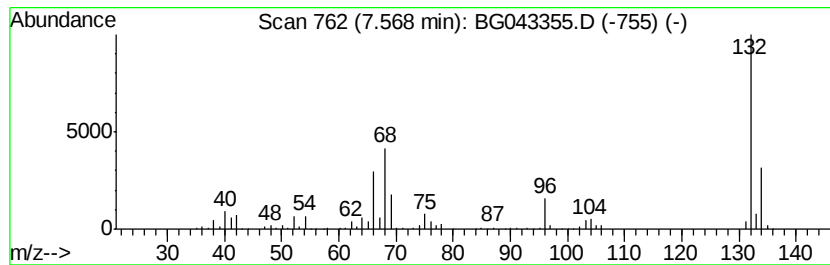

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102819\
Data File : BG043355.D
Acq On : 28 Oct 2019 18:18
Operator : JU
Sample : PB124295BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124295BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.57	7.57	53.4	ng	597866	1	8.03	223956	20.0