
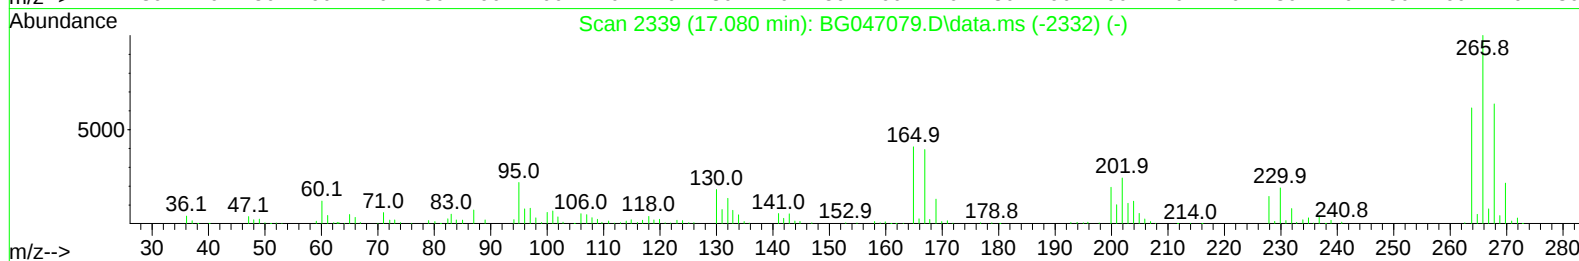
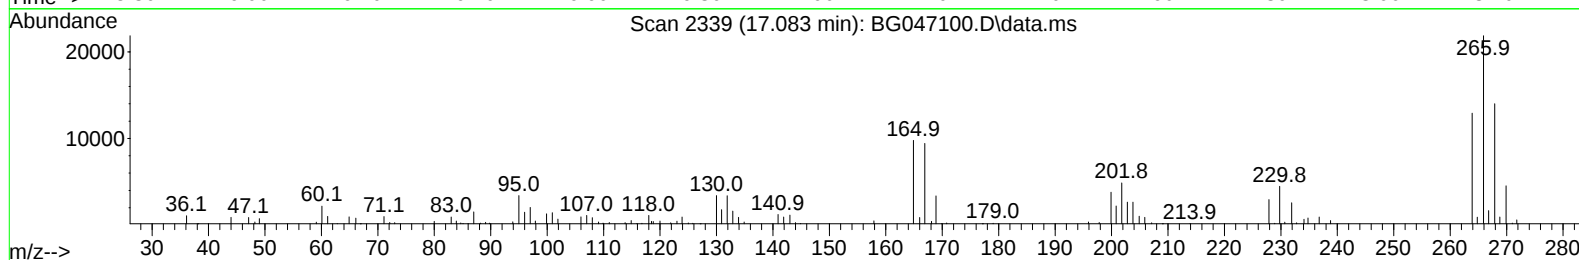


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102820\
Data File : BG047100.D
Acq On : 28 Oct 2020 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 06:38:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:55:38 2020
Response via : Initial Calibration

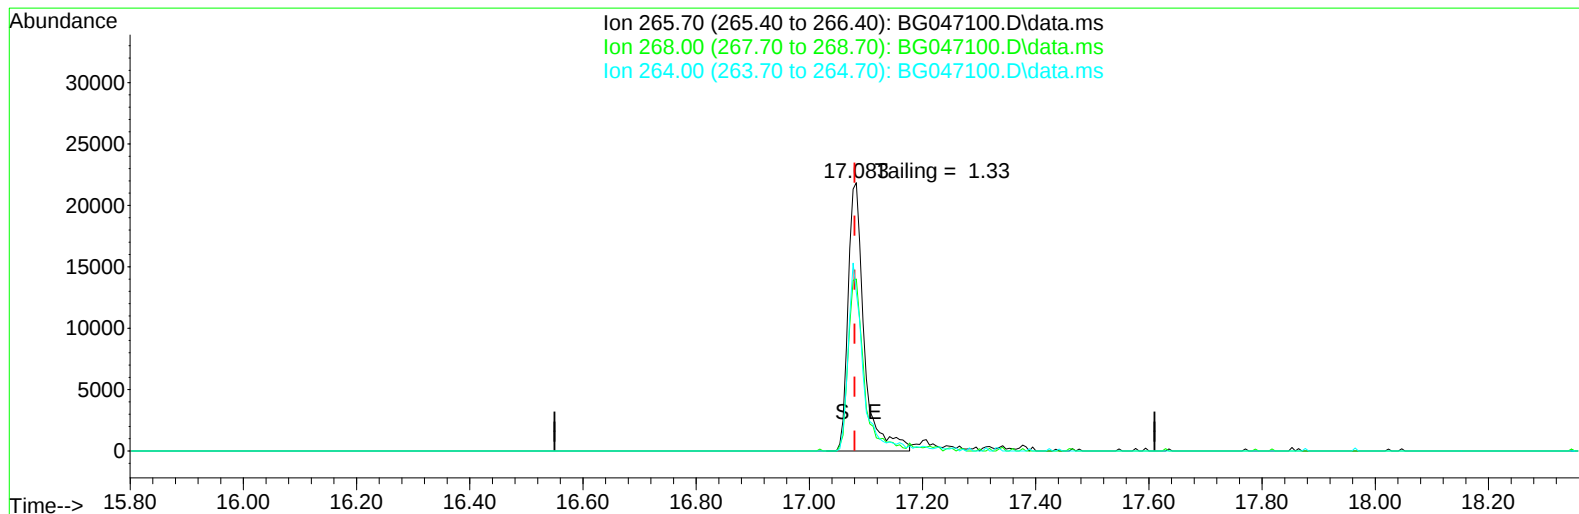

TIC: BG047100.D\data.ms

(70) Pentachlorophenol (C)




17.083min (+ 0.003) 25277.01 ng

response 40889

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.08
264.00	61.60	59.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102820\
Data File : BG047100.D
Acq On : 28 Oct 2020 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 06:38:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:55:38 2020
Response via : Initial Calibration

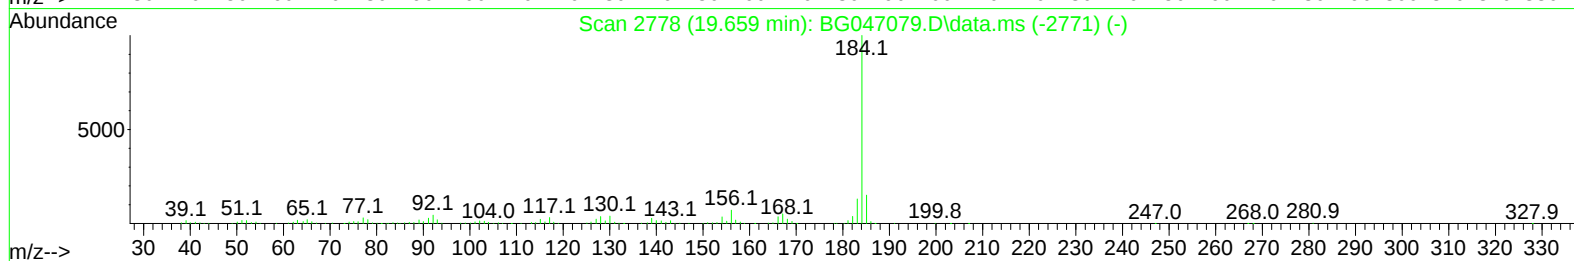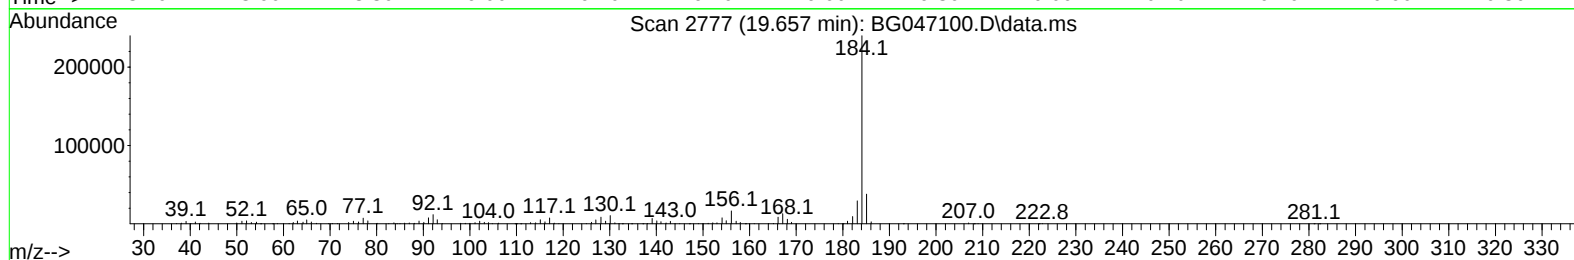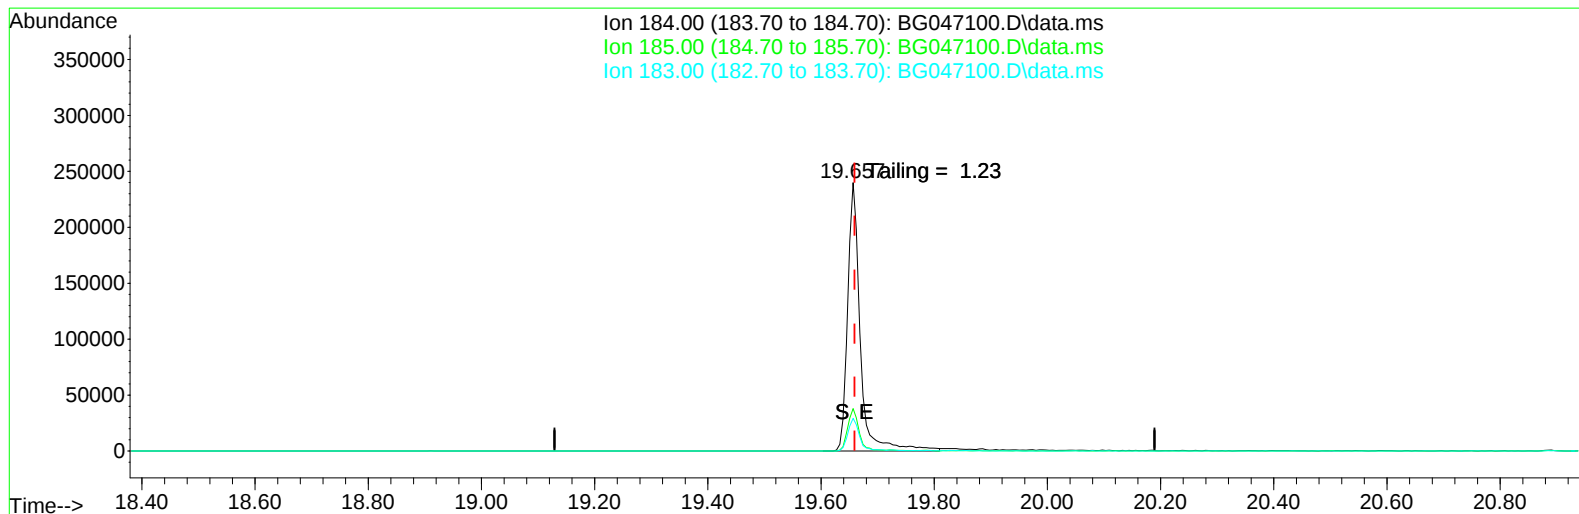

TIC: BG047100.D\data.ms

(77) Benzidine

19.657min (-0.002) 0.00 ng

response 377805

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.80
183.00	13.20	12.19
0.00	0.00	0.00