

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102820\  
 Data File : BG047103.D  
 Acq On : 28 Oct 2020 11:16  
 Operator : CG/JU  
 Sample : PB132419BL  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB132419BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG102720.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG047103.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.617       | 381           | 388         | 397          | rBV      | 1066625        | 1653345       | 31.79%          | 8.819%        |
| 2         | 7.210       | 651           | 659         | 671          | rBV      | 1011366        | 1707829       | 32.84%          | 9.110%        |
| 3         | 8.056       | 796           | 803         | 813          | rBV      | 194485         | 329437        | 6.34%           | 1.757%        |
| 4         | 9.219       | 992           | 1001        | 1012         | rBV      | 665810         | 1180944       | 22.71%          | 6.299%        |
| 5         | 10.870      | 1274          | 1282        | 1291         | rBV      | 224831         | 426686        | 8.21%           | 2.276%        |
| 6         | 13.308      | 1690          | 1697        | 1710         | rBV      | 1797964        | 2710662       | 52.13%          | 14.459%       |
| 7         | 14.689      | 1925          | 1932        | 1948         | rVB      | 365463         | 606286        | 11.66%          | 3.234%        |
| 8         | 16.170      | 2178          | 2184        | 2201         | rBV      | 1384599        | 2101760       | 40.42%          | 11.211%       |
| 9         | 17.433      | 2392          | 2399        | 2409         | rBV      | 520415         | 796043        | 15.31%          | 4.246%        |
| 10        | 20.036      | 2836          | 2842        | 2854         | rBV      | 3993820        | 5200026       | 100.00%         | 27.738%       |
| 11        | 21.699      | 3118          | 3125        | 3135         | rBV      | 620769         | 1010358       | 19.43%          | 5.389%        |
| 12        | 24.930      | 3663          | 3675        | 3687         | rBV2     | 356750         | 1023476       | 19.68%          | 5.459%        |




Sum of corrected areas: 18746852

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102820\  
Data File : BG047103.D  
Acq On : 28 Oct 2020 11:16  
Operator : CG/JU  
Sample : PB132419BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB132419BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG102720.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

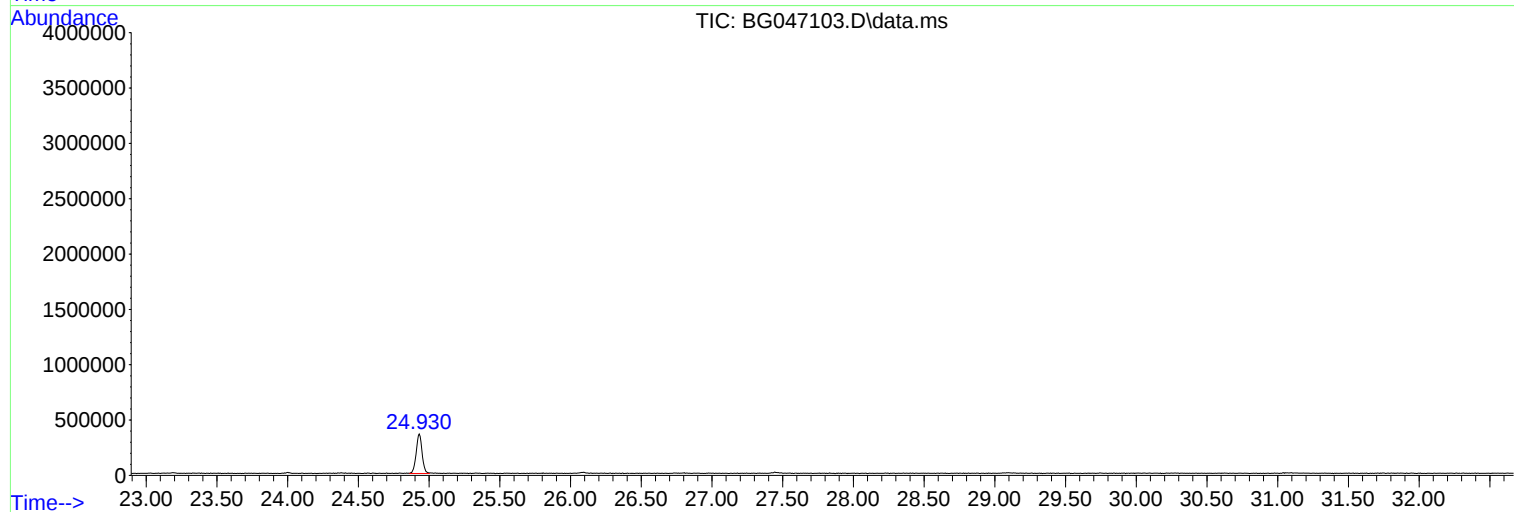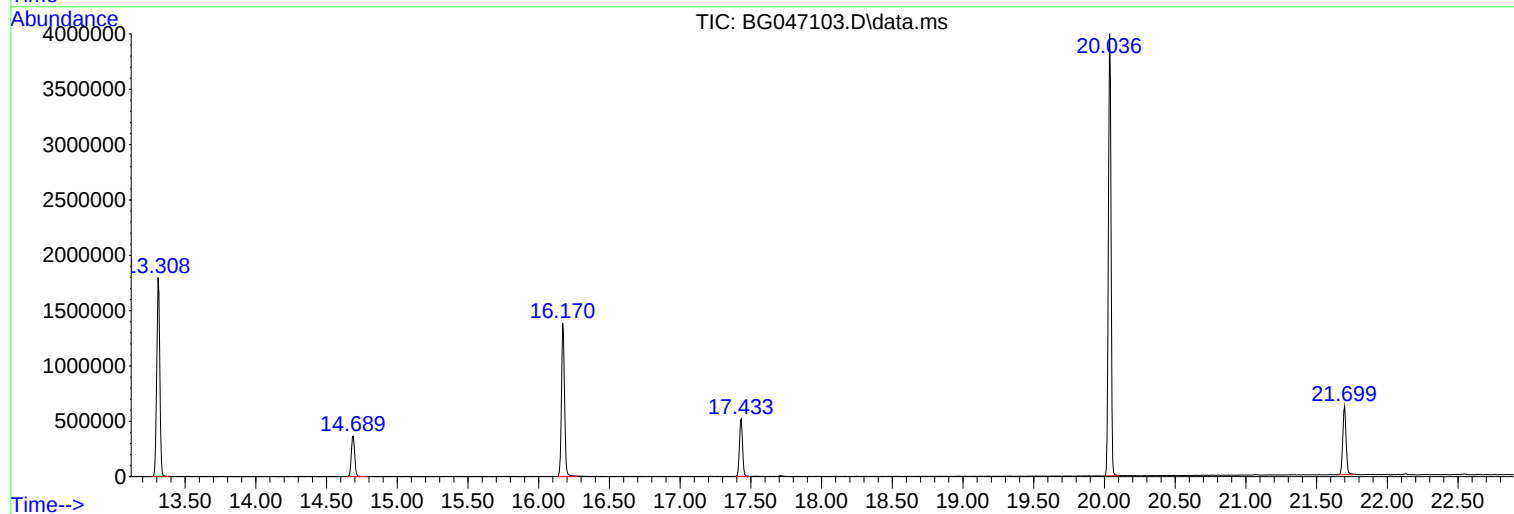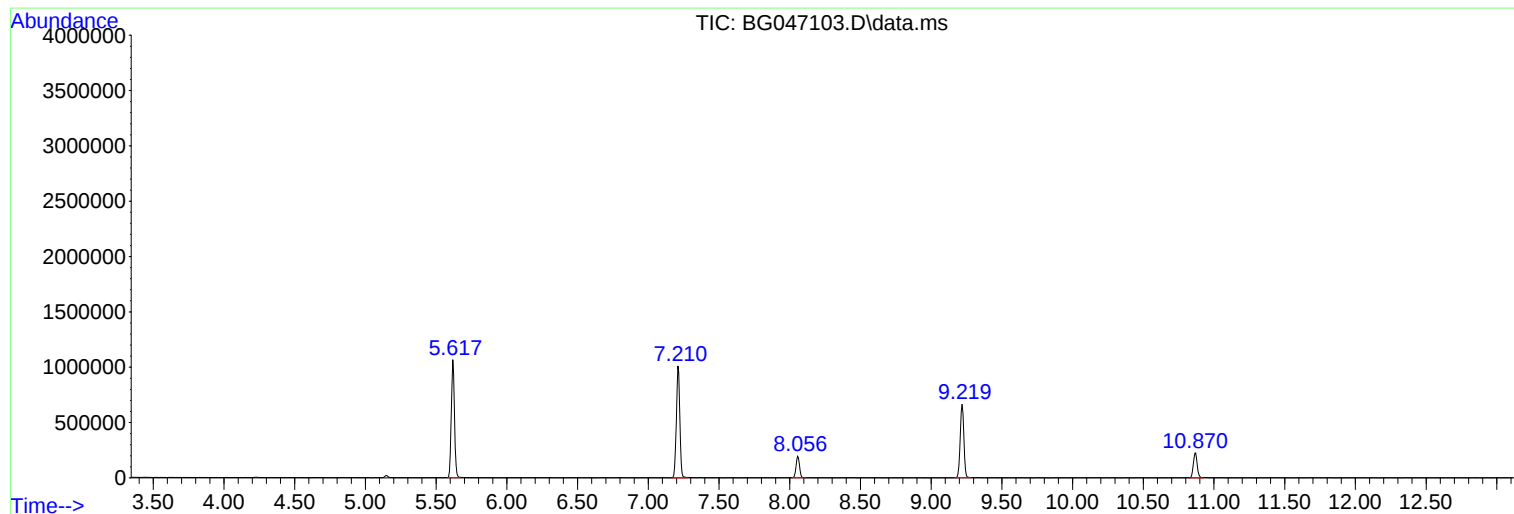

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102820\  
Data File : BG047103.D  
Acq On : 28 Oct 2020 11:16  
Operator : CG/JU  
Sample : PB132419BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB132419BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG102720.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102820\  
Data File : BG047103.D  
Acq On : 28 Oct 2020 11:16  
Operator : CG/JU  
Sample : PB132419BL  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB132419BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG102720.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----