
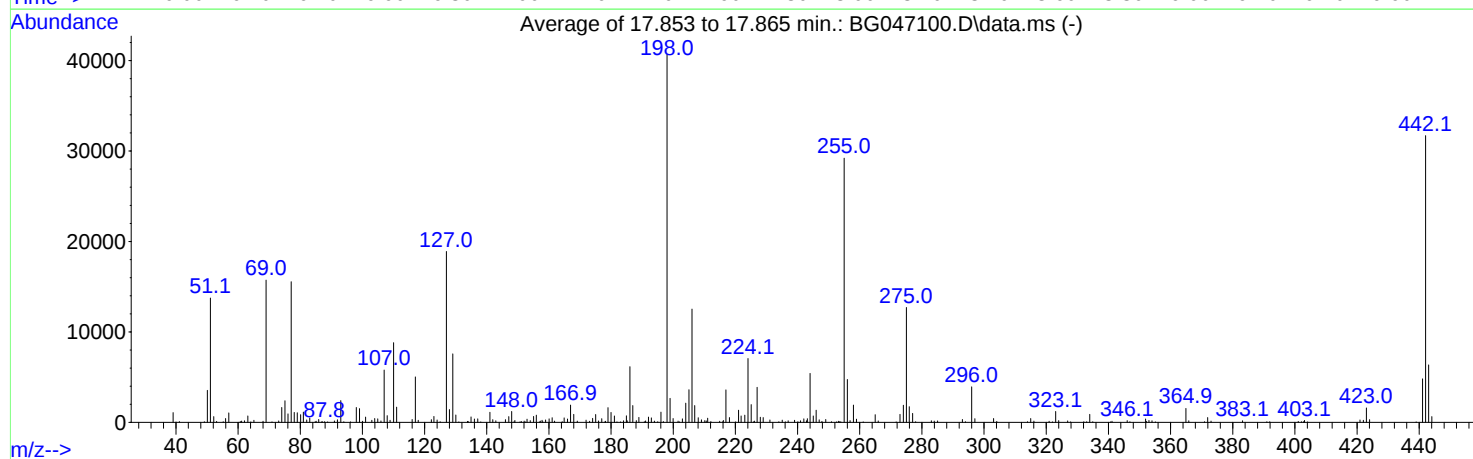


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102820\
 Data File : BG047100.D
 Acq On : 28 Oct 2020 9:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 27 02:55:38 2020

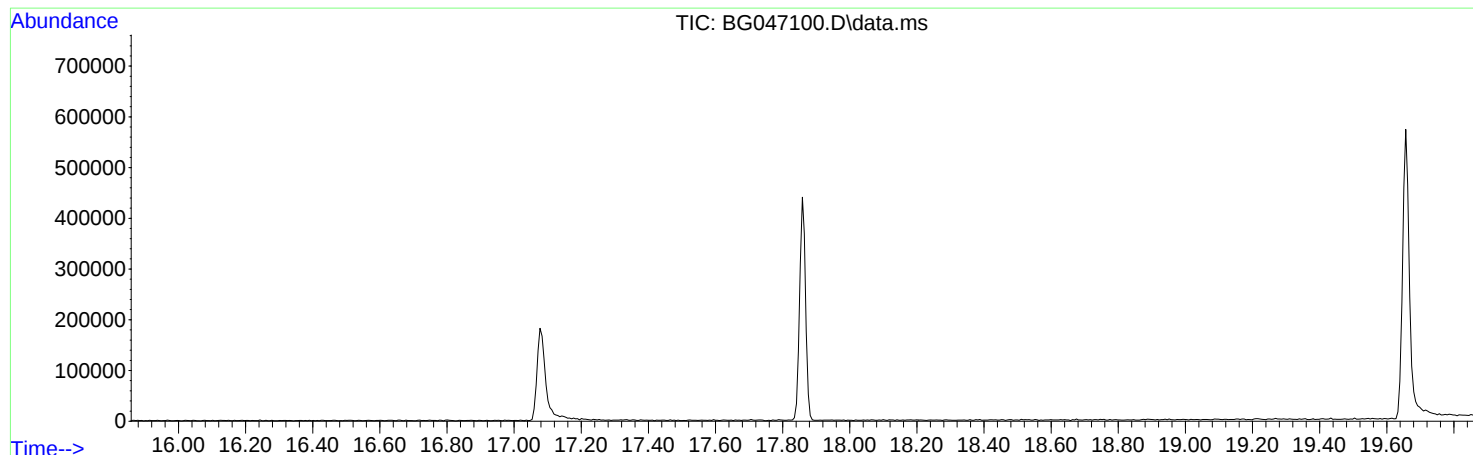

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	13755	PASS
68	69	0.00	2	0.8	122	PASS
69	198	0.00	100	38.7	15727	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	18904	PASS
197	198	0.00	2	0.2	97	PASS
198	198	100	100	100.0	40677	PASS
199	198	5	9	6.5	2646	PASS
275	198	10	60	31.2	12702	PASS
365	198	1	100	3.8	1540	PASS
441	198	0.01	100	11.8	4807	PASS
442	198	50	100	77.9	31699	PASS
443	442	15	24	20.1	6359	PASS