


Data Path : Z:\HPCHEM1\BNA G\DATA\BG103017\
Data File : BG030591.D
Acq On : 30 Oct 2017 23:09
Operator : SJ/JU
Sample : I5842-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 31 07:22:50 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 31 07:15:18 2017
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampled :
C0AA6

Manual Integrations
APPROVED

Sohil
10/31/2017 7:43:48 PM

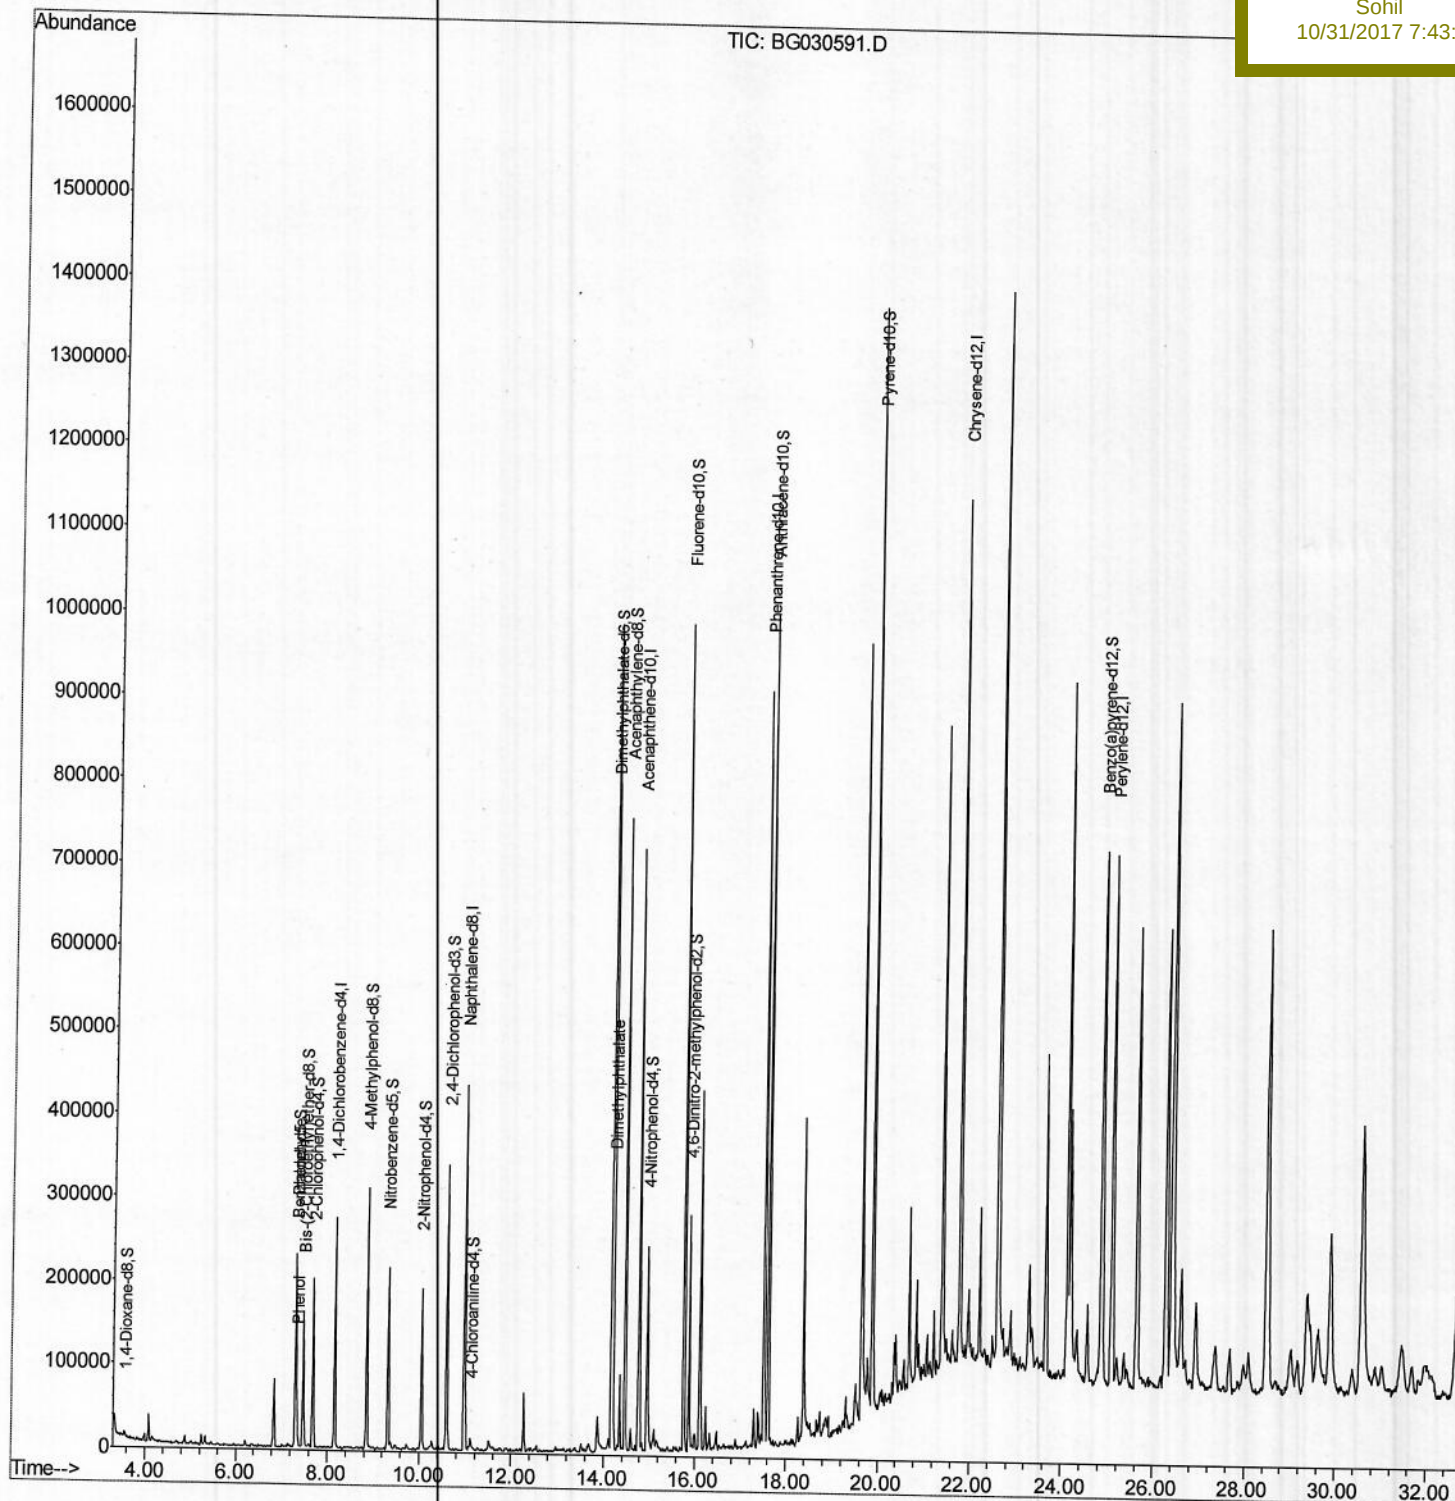

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA G\DATA\BG103017\
 Data File : BG030591.D
 Acq On : 30 Oct 2017 23:09
 Operator : SJ/JU
 Sample : I5842-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 31 07:18:05 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 07:15:18 2017
 Response via : Initial Calibration

Instrument :

BNA_G

ClientSampleId :




C0AA6

Manual Integrations

APPROVED

Sohil

10/31/2017 7:43:48 PM

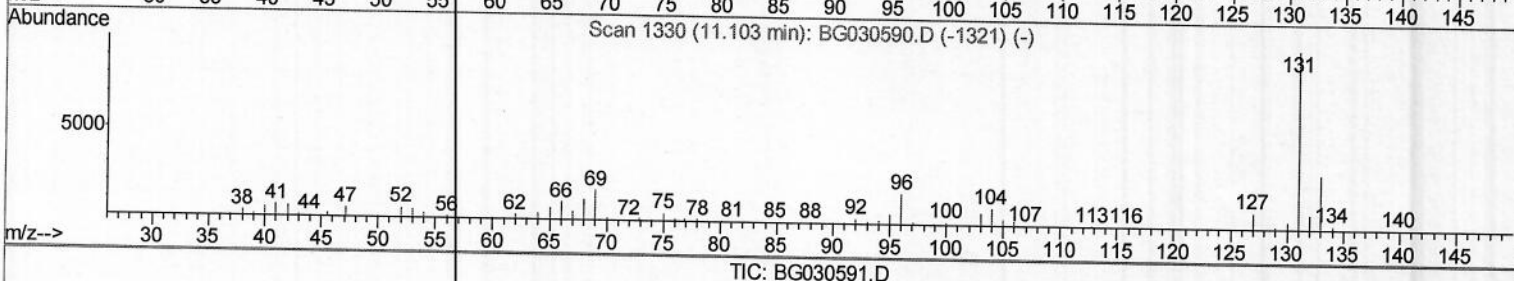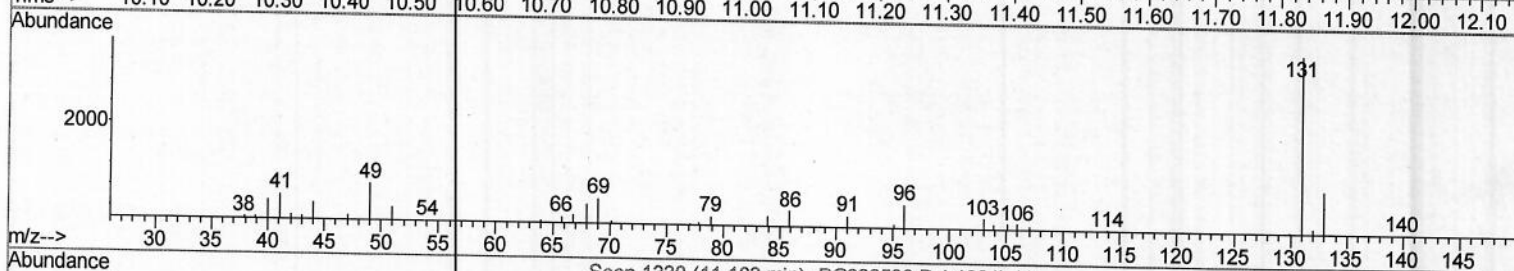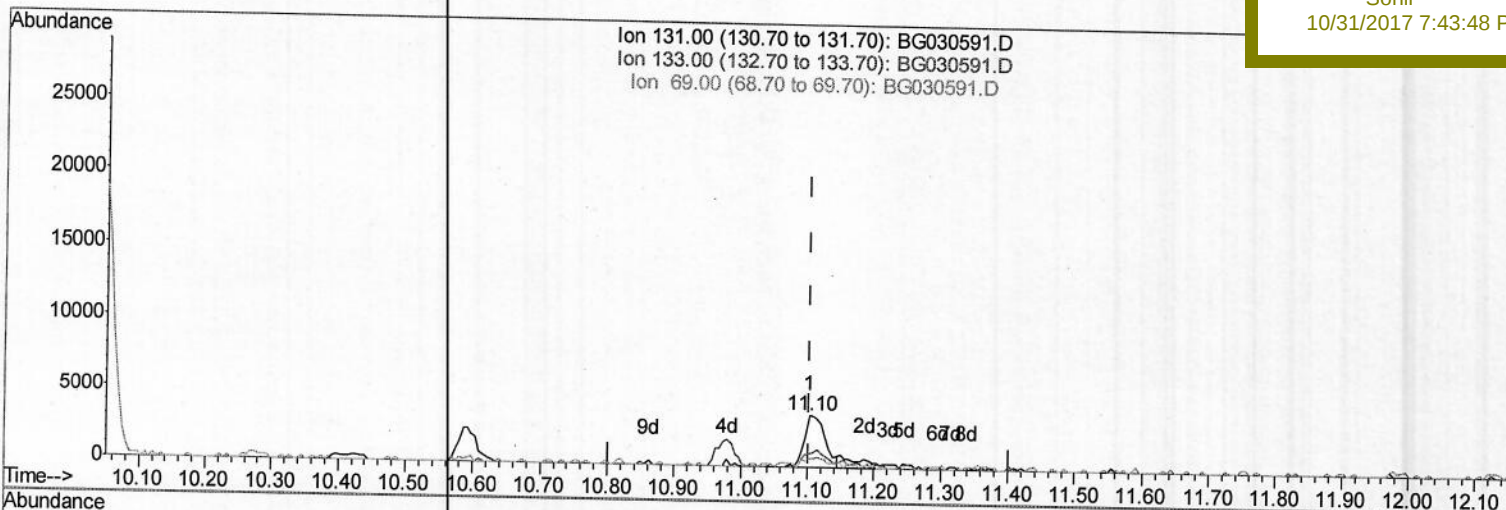

TIC: BG030591.D

(29) 4-Chloroaniline-d4 (S)

11.103min (-0.001) 1.00ng/ul

response 7679

Ion	Exp%	Act%
-----	------	------

131.00	100	100
--------	-----	-----

133.00	33.90	27.06#
--------	-------	--------

69.00	22.20	17.67#
-------	-------	--------

0.00	0.00	0.00
------	------	------

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG103017\
 Data File : BG030591.D
 Acq On : 30 Oct 2017 23:09
 Operator : SJ/JU
 Sample : I5842-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 31 07:18:05 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 07:15:18 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 Client Sampled :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 10/31/2017 7:43:48 PM

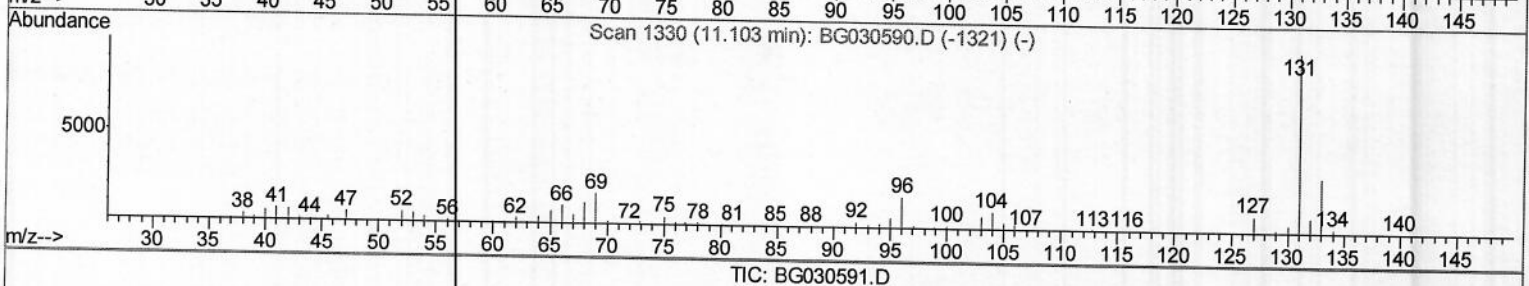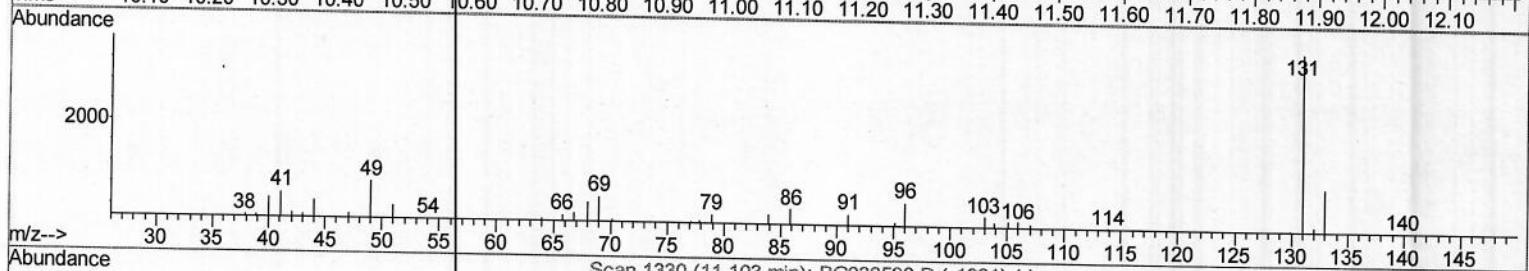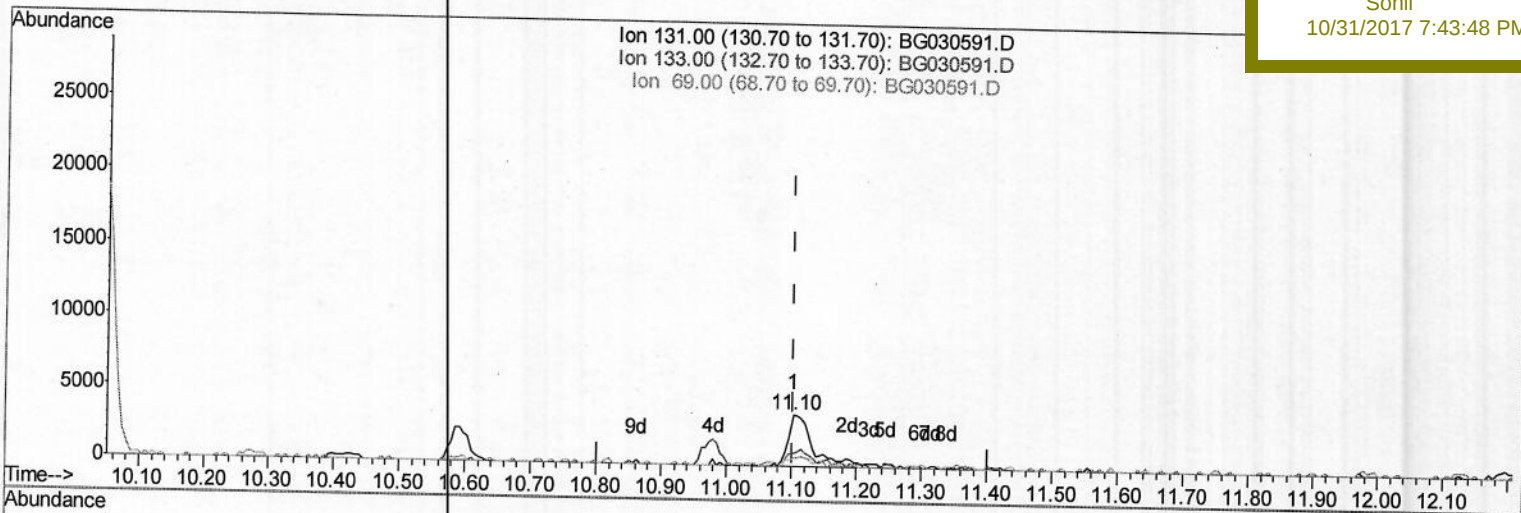

(29) 4-Chloroaniline-d4 (S)

11.103min (-0.001) 1.24ng/ul m > SJ11/11/17

response 9512

Ion	Exp%	Act%
131.00	100	100
133.00	33.90	27.06#
69.00	22.20	17.67#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG103017\
 Data File : BG030591.D
 Acq On : 30 Oct 2017 23:09
 Operator : SJ/JU
 Sample : I5842-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA6

Quant Time: Oct 31 07:22:50 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 31 07:15:18 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 10/31/2017 7:43:48 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	78914	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	394999	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.77	164	249513	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	559154	20.00	ng/ul	0.00
75) Chrysene-d12	21.79	240	602643	20.00	ng/ul	0.00
83) Perylene-d12	25.10	264	599544	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.55	96	3922	2.02	ng/uL	0.00
5) Phenol-d5	7.31	99	138162	18.24	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.48	67	75336	15.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	104757	19.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	129522	21.17	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	57620	20.32	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	70447	24.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	142310	21.49	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	9512m)	1.24	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	468980	21.99	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	578362	22.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.96	143	74814	19.00	ng/ul	0.00
57) Fluorene-d10	15.76	176	424286	24.29	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.87	200	73753	27.02	ng/ul	0.00
70) Anthracene-d10	17.61	188	592861	22.42	ng/ul	0.00
76) Pyrene-d10	19.89	212	733893	23.53	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	660934	23.28	ng/ul	0.00
Target Compounds						
4) Benzaldehyde	7.30	77	6187	1.32	ng/ul	96
6) Phenol	7.34	94	25955	3.31	ng/ul	93
44) Dimethylphthalate	14.22	163	41341	1.99	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed