


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG103019\
Data File : BG043400.D
Acq On : 30 Oct 2019 14:04
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 21 16:37:43 2019

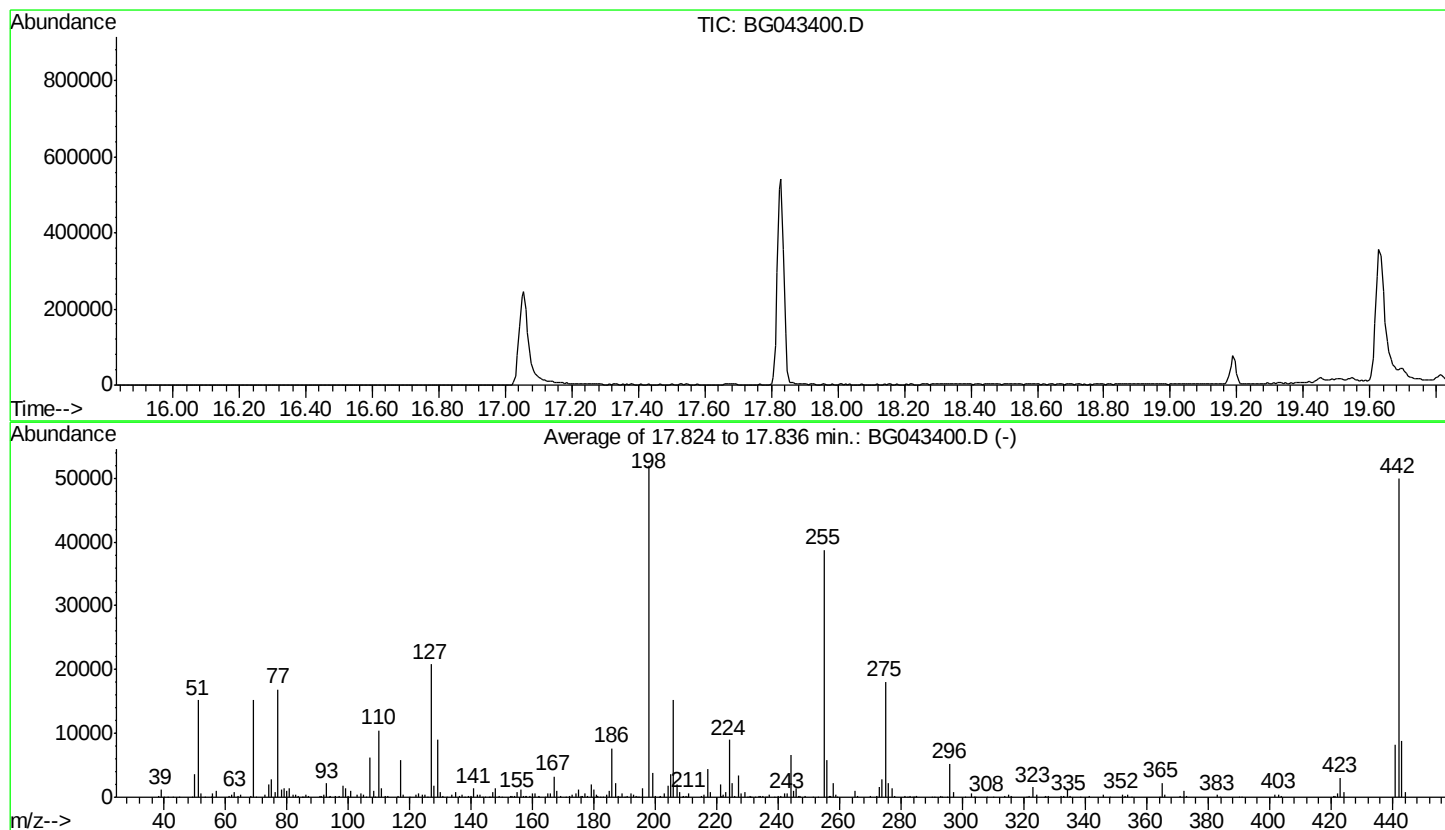

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	15211	PASS
68	69	0.00	2	0.9	132	PASS
69	198	0.00	100	29.5	15336	PASS
70	69	0.00	2	0.4	60	PASS
127	198	10	80	40.0	20799	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51954	PASS
199	198	5	9	7.2	3758	PASS
275	198	10	60	34.9	18139	PASS
365	198	1	100	4.3	2228	PASS
441	198	0.01	100	15.9	8253	PASS
442	198	50	100	96.1	49917	PASS
443	442	15	24	17.7	8841	PASS