


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG103019\
 Data File : BG043418.D
 Acq On : 31 Oct 2019 2:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 21 16:37:43 2019

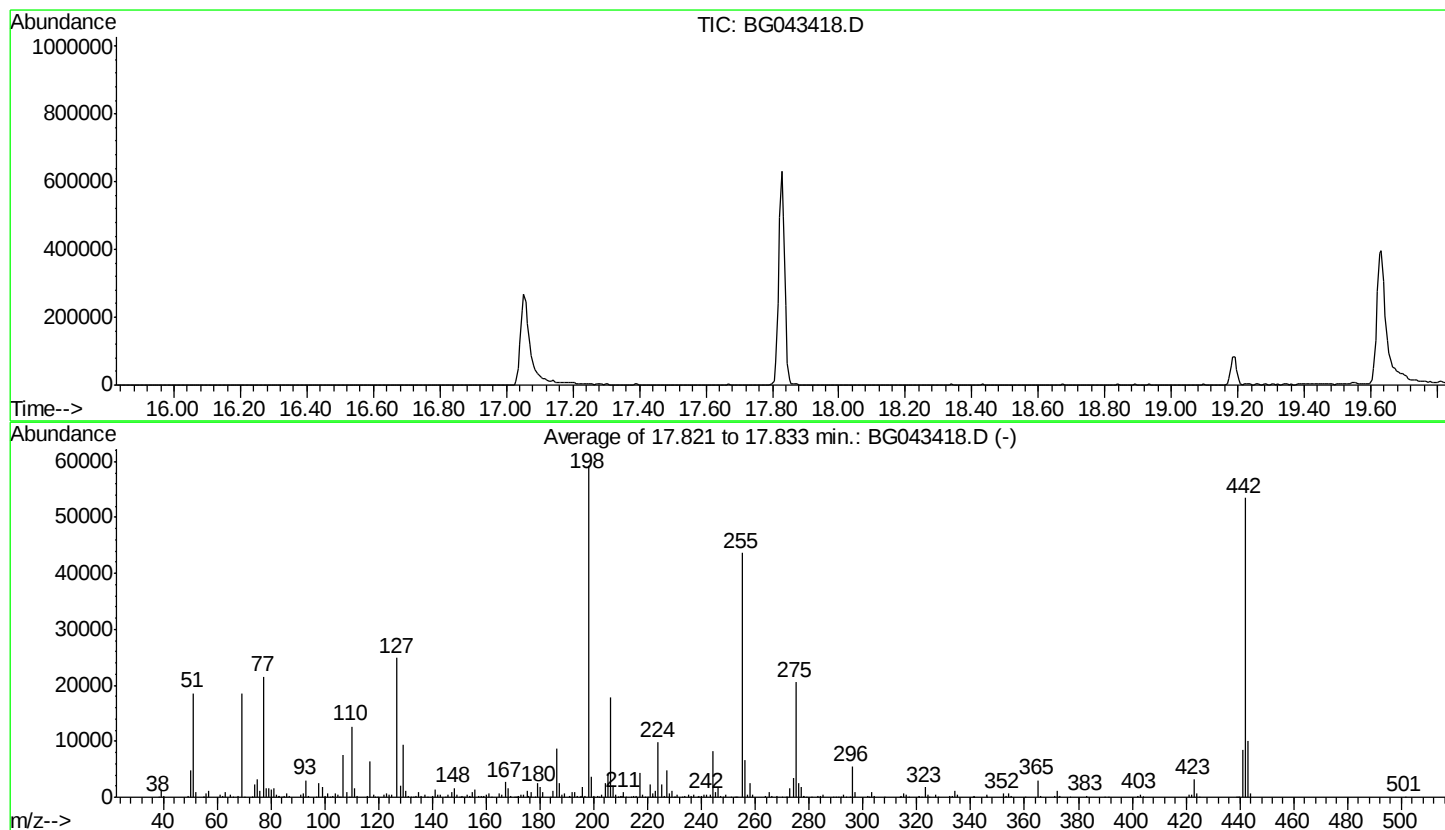

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	18609	PASS
68	69	0.00	2	0.8	152	PASS
69	198	0.00	100	31.5	18646	PASS
70	69	0.00	2	0.3	54	PASS
127	198	10	80	41.9	24837	PASS
197	198	0.00	2	0.4	214	PASS
198	198	100	100	100.0	59266	PASS
199	198	5	9	6.1	3627	PASS
275	198	10	60	34.6	20528	PASS
365	198	1	100	5.1	3040	PASS
441	198	0.01	100	14.3	8492	PASS
442	198	50	100	90.3	53514	PASS
443	442	15	24	19.0	10173	PASS