


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG103116\
 Data File : BG024556.D
 Acq On : 31 Oct 2016 14:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 01 11:50:40 2016

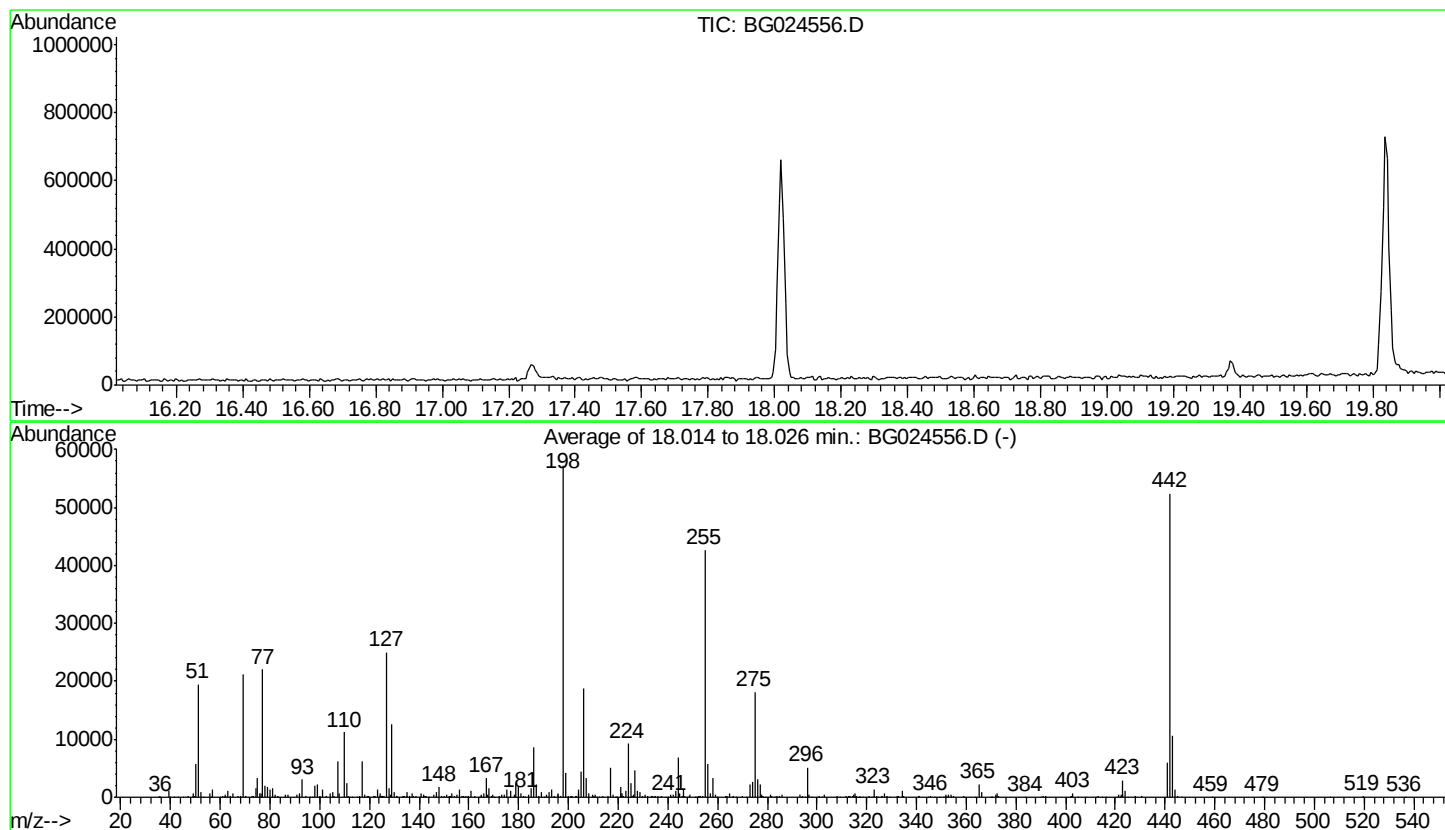

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	19495	PASS
68	69	0.00	2	1.3	269	PASS
69	198	0.00	100	37.2	21293	PASS
70	69	0.00	2	1.2	248	PASS
127	198	10	80	43.8	25053	PASS
197	198	0.00	2	0.5	262	PASS
198	198	100	100	100.0	57221	PASS
199	198	5	9	7.3	4187	PASS
275	198	10	60	31.8	18211	PASS
365	198	1	100	4.0	2313	PASS
441	442	0.01	24	11.5	6032	PASS
442	198	50	100	91.6	52434	PASS
443	442	15	24	20.4	10689	PASS