


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG103116\
 Data File : BG024574.D
 Acq On : 1 Nov 2016 3:08
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 01 11:50:40 2016

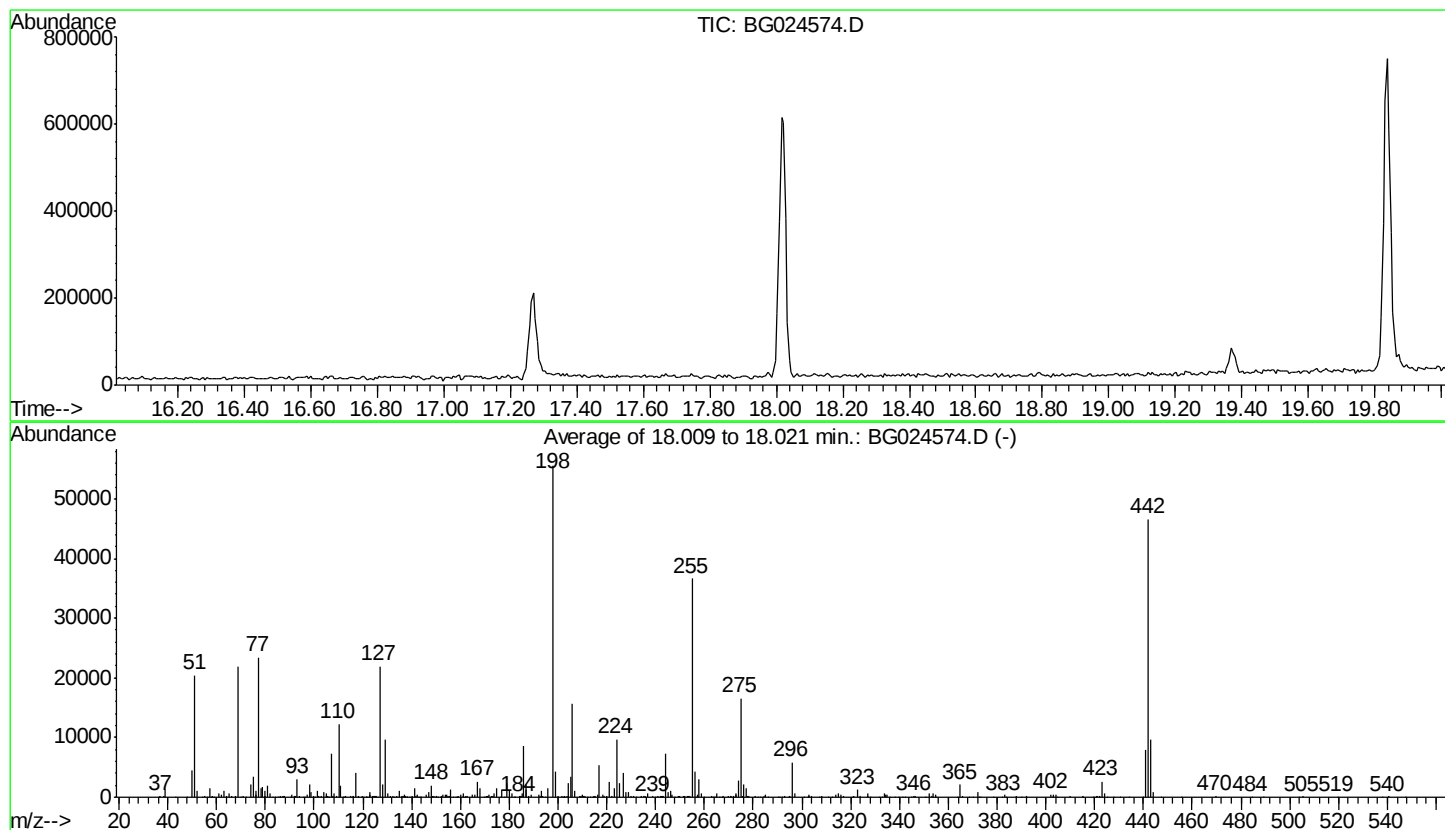

AutoFind: Scans 2582, 2583, 2584; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	20435	PASS
68	69	0.00	2	1.4	304	PASS
69	198	0.00	100	39.5	21946	PASS
70	69	0.00	2	0.5	108	PASS
127	198	10	80	39.5	21925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55552	PASS
199	198	5	9	7.7	4303	PASS
275	198	10	60	29.8	16546	PASS
365	198	1	100	3.9	2141	PASS
441	442	0.01	24	17.2	8013	PASS
442	198	50	100	84.0	46640	PASS
443	442	15	24	20.7	9649	PASS