
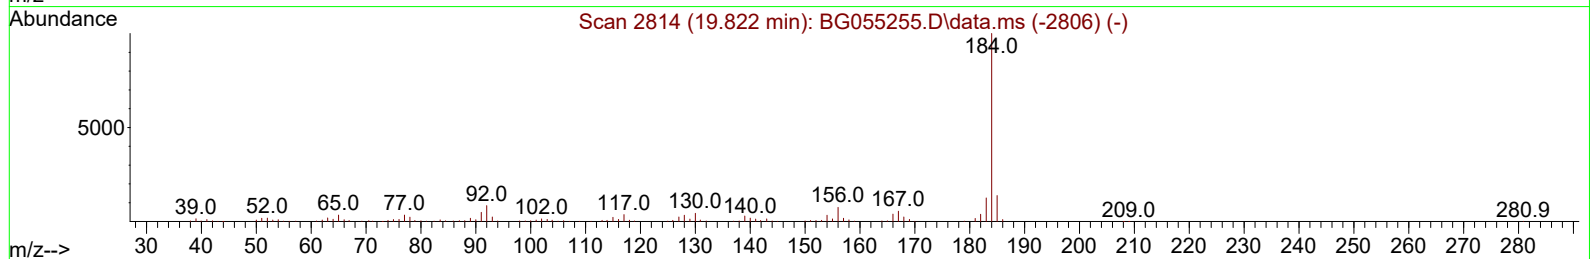
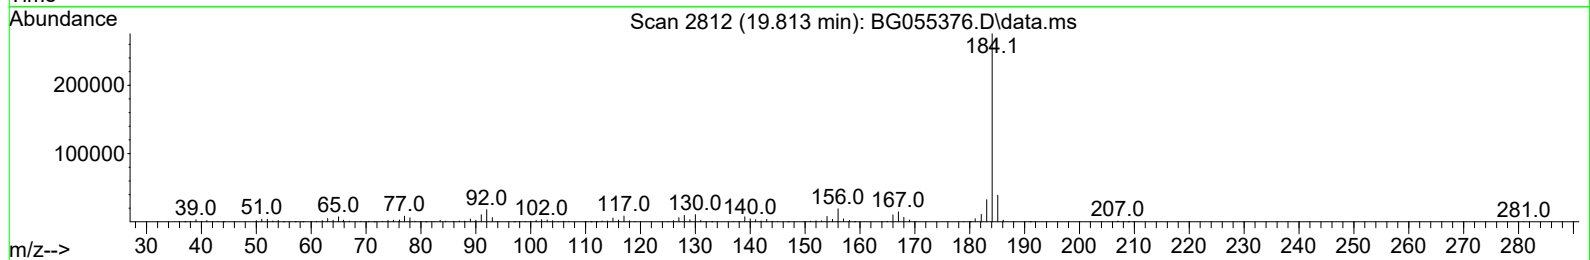


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103122\
Data File : BG055376.D
Acq On : 31 Oct 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 18:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration

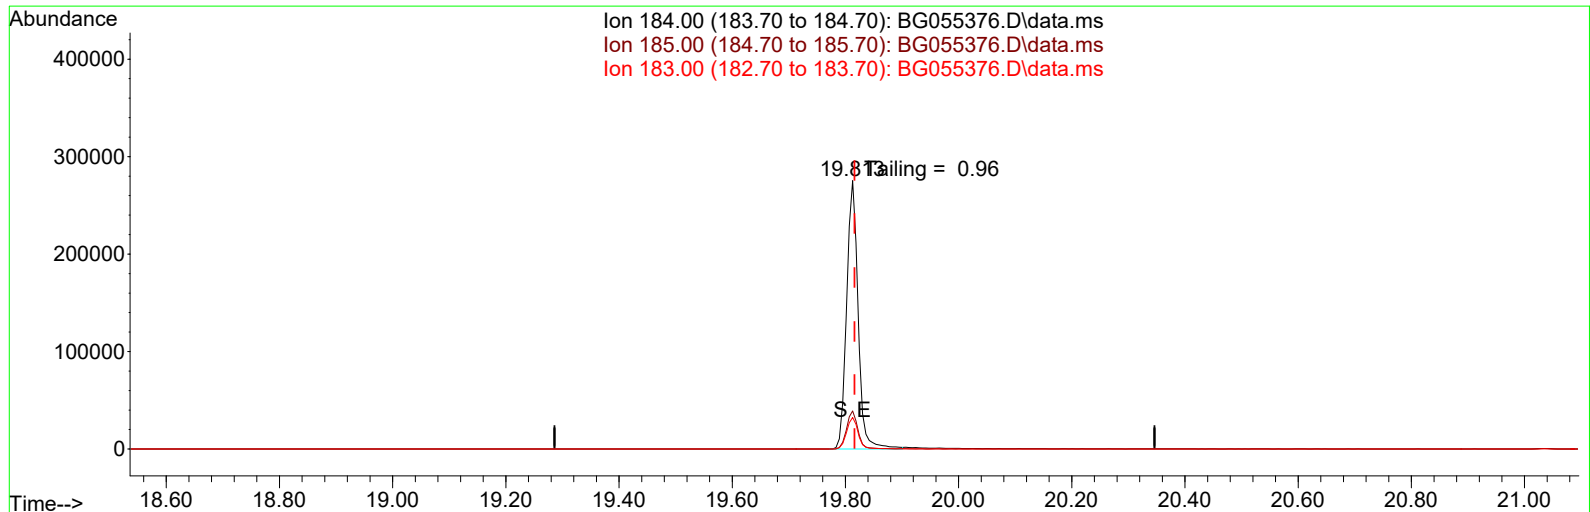

TIC: BG055376.D\data.ms

(77) Benzidine




19.813min (-0.003) 0.00 ng

response 392550

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.21
183.00	12.50	11.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103122\
Data File : BG055376.D
Acq On : 31 Oct 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 31 18:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration

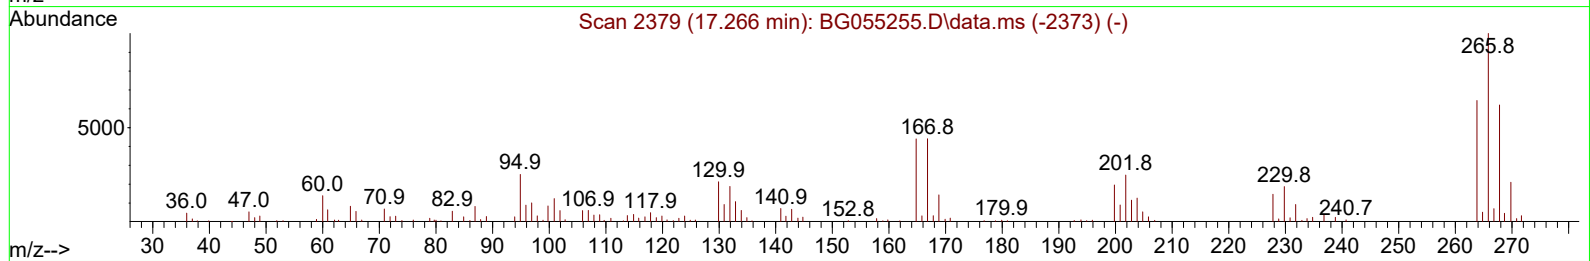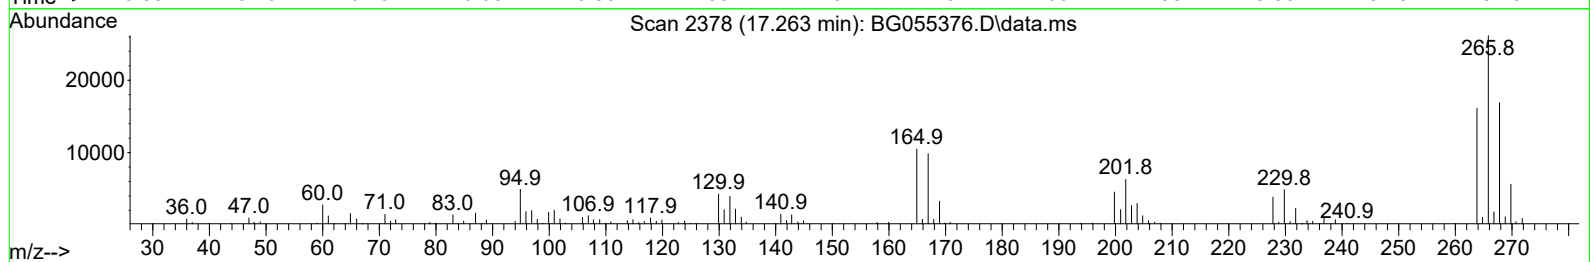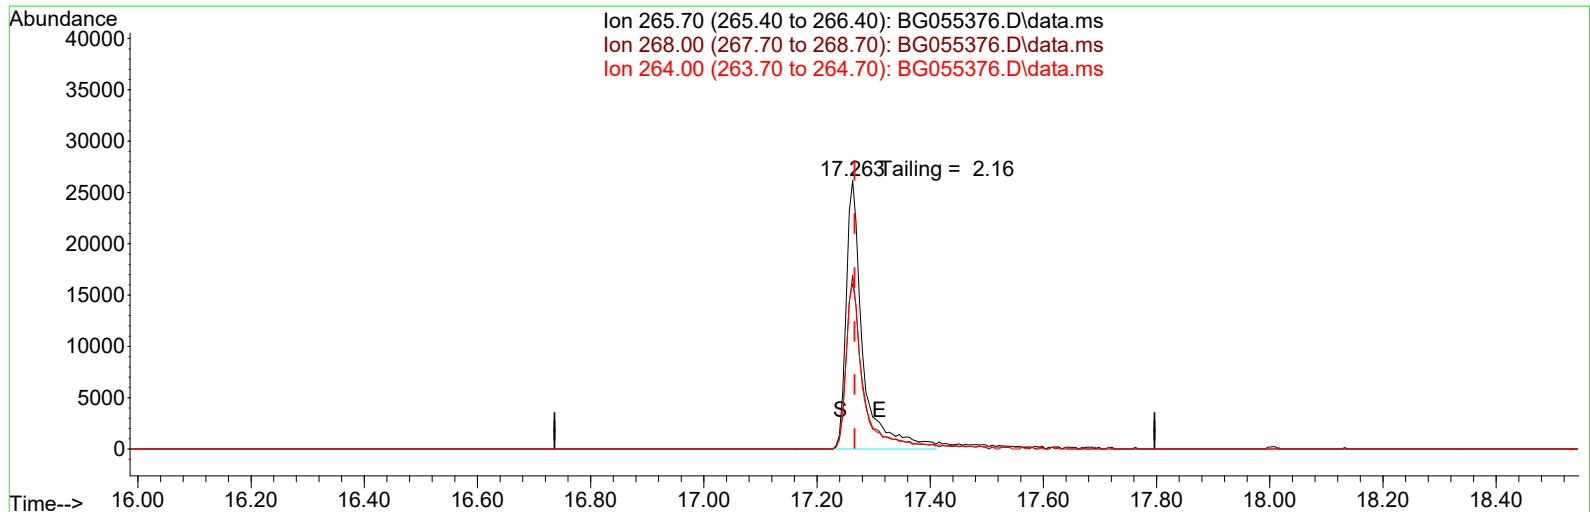

TIC: BG055376.D\data.ms

(70) Pentachlorophenol (C)

17.263min (-0.003) 153644.96 ng

response 54163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	64.61
264.00	64.40	61.71
0.00	0.00	0.00