

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103122\
 Data File : BG055384.D
 Acq On : 31 Oct 2022 18:29
 Operator : CG/JU
 Sample : N5313-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMPOSITE-NW-QUARTER

Quant Time: Nov 01 06:50:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 29 04:52:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.261	152	33031	20.000	ng	0.00
21) Naphthalene-d8	11.087	136	136285	20.000	ng	# 0.00
39) Acenaphthene-d10	14.871	164	90330	20.000	ng	0.00
64) Phenanthrene-d10	17.609	188	197520	20.000	ng	# 0.00
76) Chrysene-d12	21.881	240	193895	20.000	ng	0.00
86) Perylene-d12	25.277	264	206078	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.794	112	276125	146.374	ng	0.00
7) Phenol-d6	7.409	99	333812	122.141	ng	0.00
23) Nitrobenzene-d5	9.436	82	243051	91.066	ng	0.00
42) 2,4,6-Tribromophenol	16.352	330	186054	189.471	ng	0.00
45) 2-Fluorobiphenyl	13.502	172	577754	104.687	ng	0.00
79) Terphenyl-d14	20.183	244	965923	103.504	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103122\
Data File : BG055384.D
Acq On : 31 Oct 2022 18:29
Operator : CG/JU
Sample : N5313-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMPOSITE-NW-QUARTER

Quant Time: Nov 01 06:50:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration




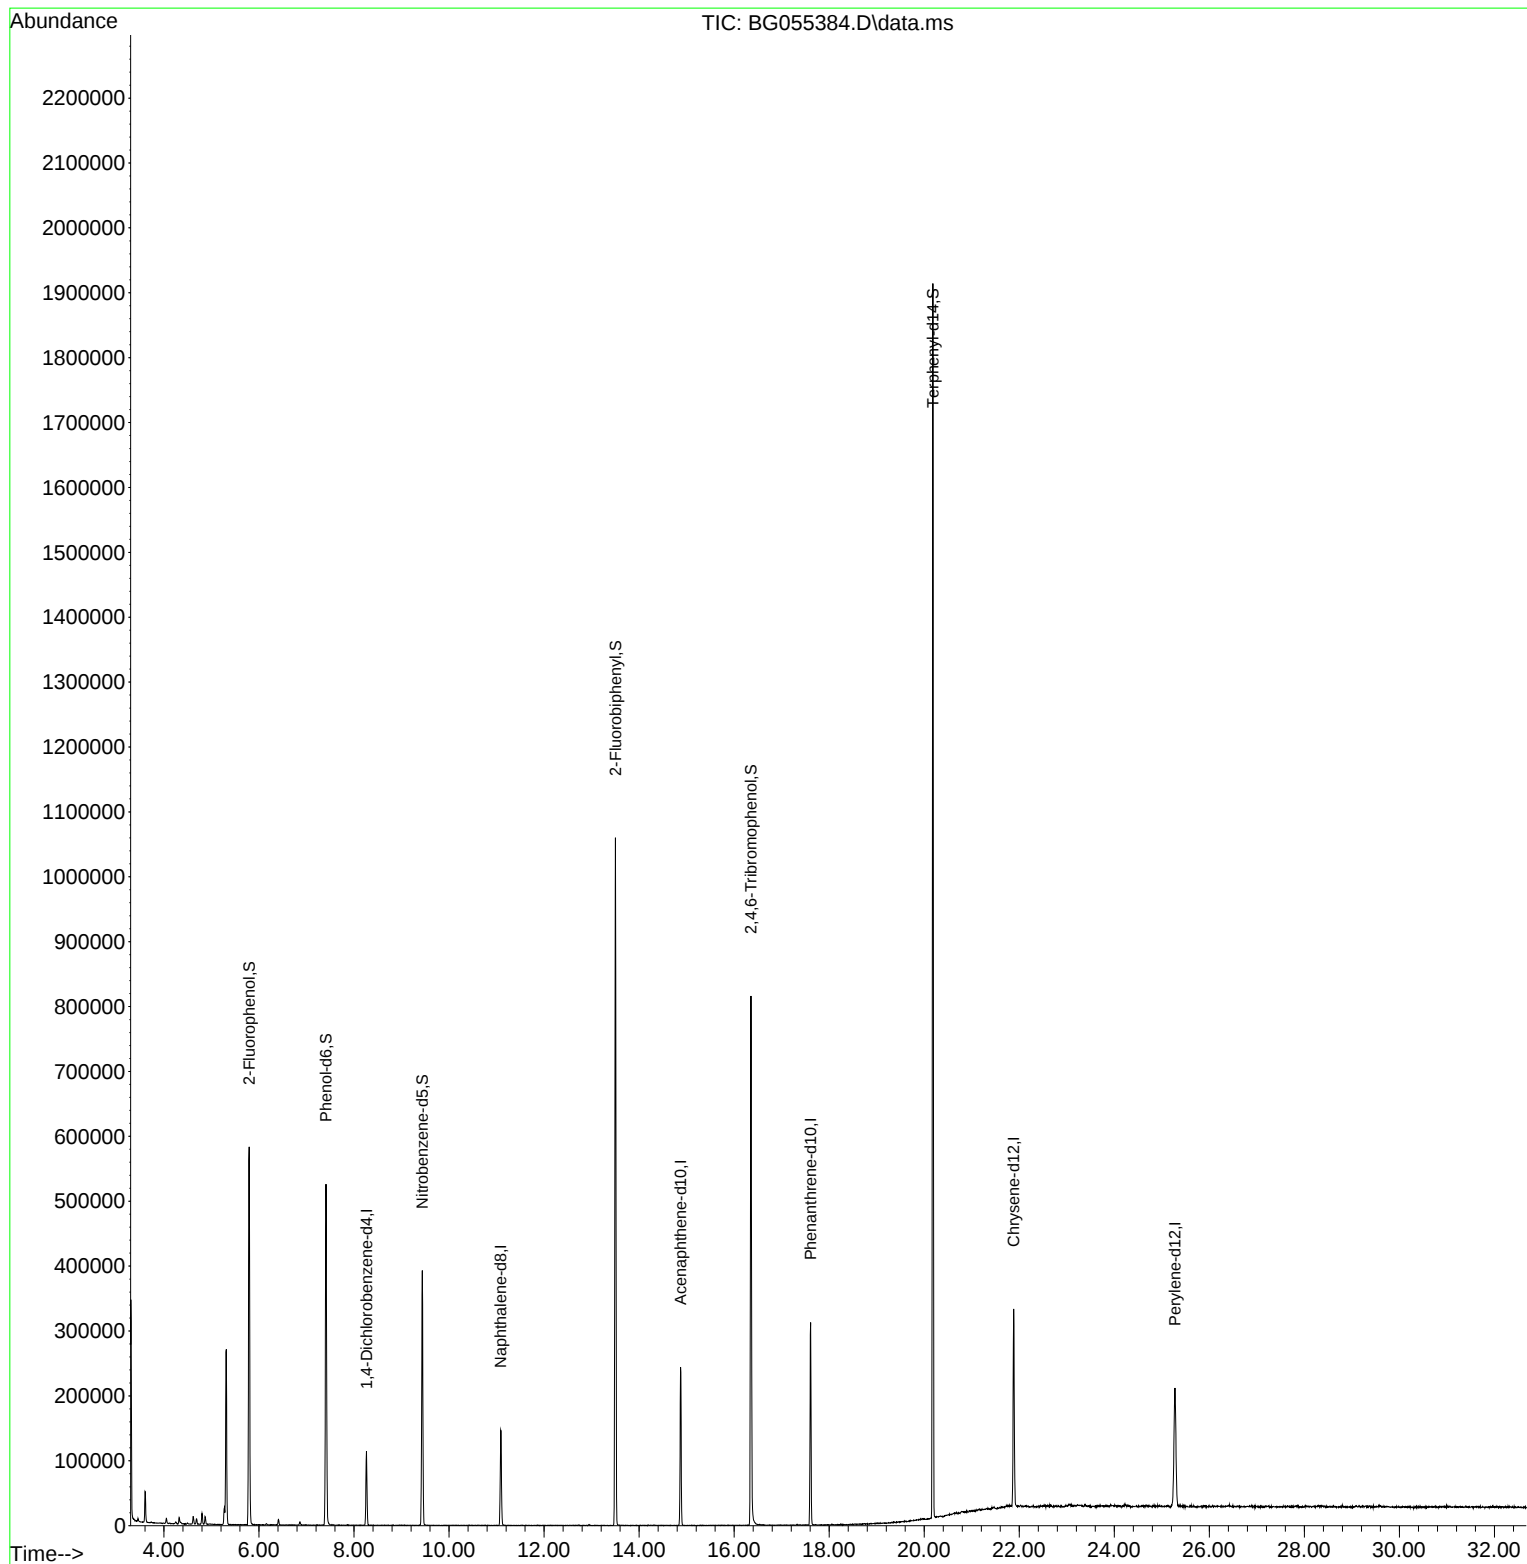


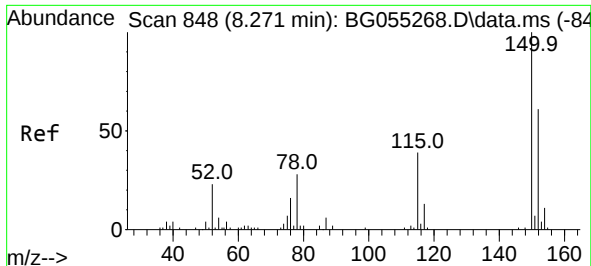

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.261 min Scan# 84
Delta R.T. -0.004 min
Lab File: BG055384.D
Acq: 31 Oct 2022 18:29




Instrument :
BNA_G
ClientSampleId :
COMPOSITE-NW-QUARTER


Tgt Ion:152 Resp: 33031
Ion Ratio Lower Upper
152 100
150 156.7 118.2 177.4
115 55.9 44.5 66.7

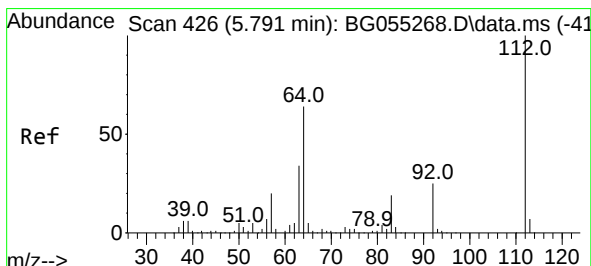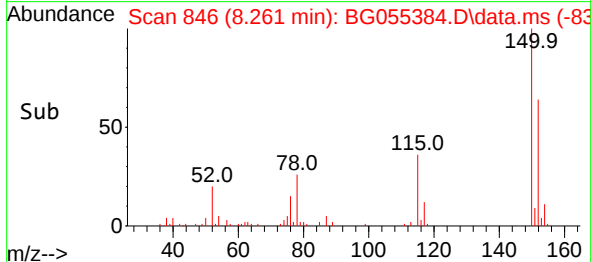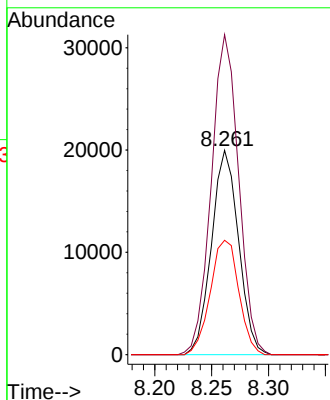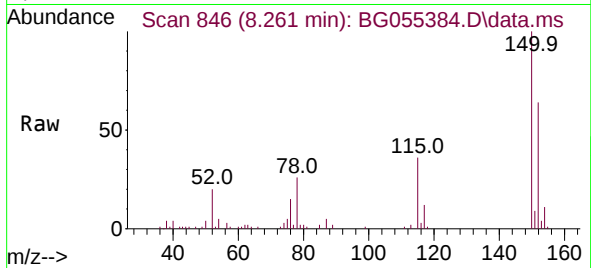

#5
2-Fluorophenol
Concen: 146.374 ng
RT: 5.794 min Scan# 426
Delta R.T. 0.008 min
Lab File: BG055384.D
Acq: 31 Oct 2022 18:29

Tgt Ion:112 Resp: 276125
Ion Ratio Lower Upper
112 100
64 59.1 52.6 78.8
63 31.5 27.1 40.7


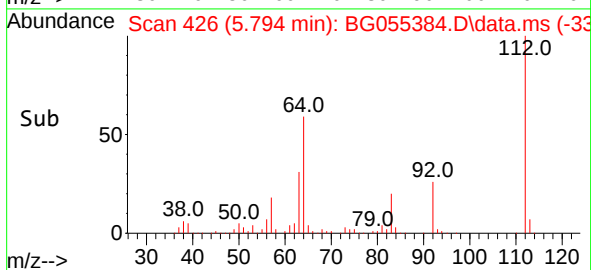
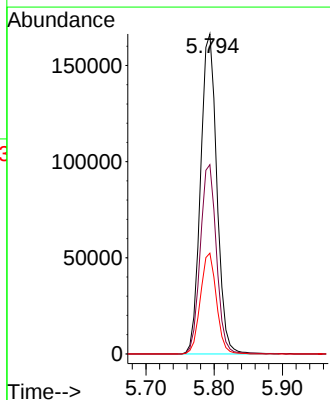
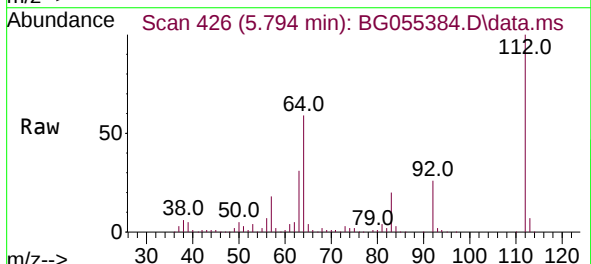


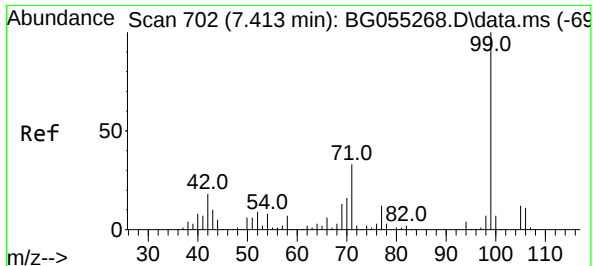

#7
Phenol-d6
Concen: 122.141 ng
RT: 7.409 min Scan# 70
Delta R.T. -0.003 min
Lab File: BG055384.D
Acq: 31 Oct 2022 18:29




Instrument :
BNA_G
ClientSampleId :
COMPOSITE-NW-QUARTER


Tgt Ion: 99 Resp: 333812
Ion Ratio Lower Upper
99 100
42 17.0 15.2 22.8
71 34.6 26.2 39.4

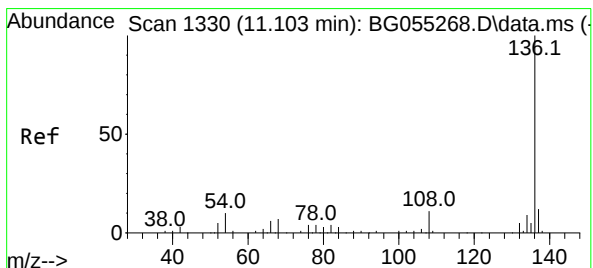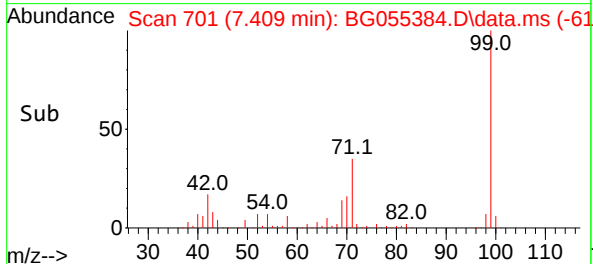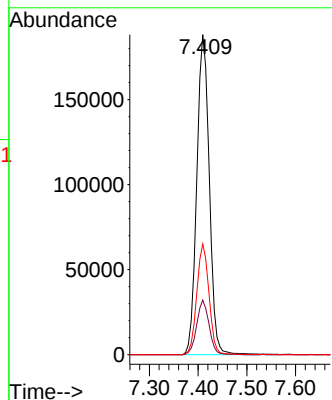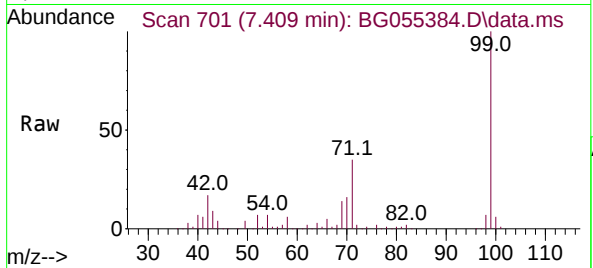

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.087 min Scan# 1327
Delta R.T. -0.009 min
Lab File: BG055384.D
Acq: 31 Oct 2022 18:29

Tgt Ion:136 Resp: 136285
Ion Ratio Lower Upper
136 100
137 11.2 9.2 13.8
54 7.7 7.8 11.8#
68 6.0 5.8 8.6

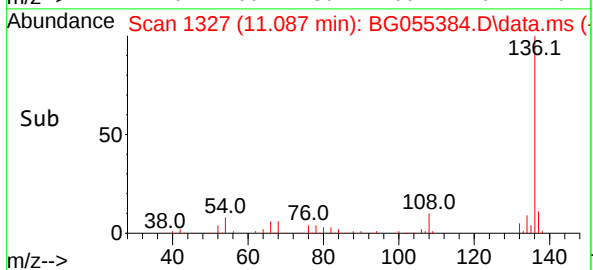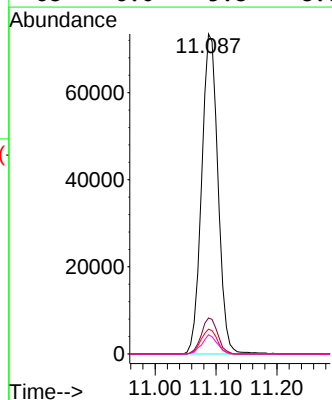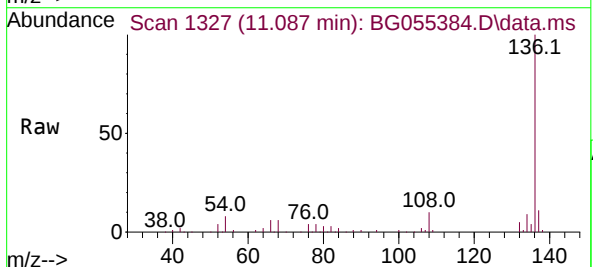

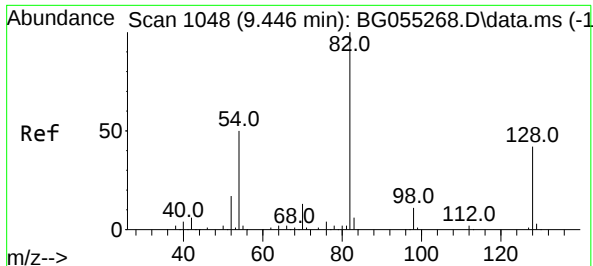

#23

Nitrobenzene-d5

Concen: 91.066 ng

RT: 9.436 min Scan# 1046

Delta R.T. -0.003 min

Lab File: BG055384.D

Acq: 31 Oct 2022 18:29

Instrument :

BNA_G

ClientSampleId :

COMPOSITE-NW-QUARTER





Tgt Ion: 82 Resp: 243051

Ion Ratio Lower Upper

82 100

128 45.4 32.0 48.0

54 48.1 40.9 61.3

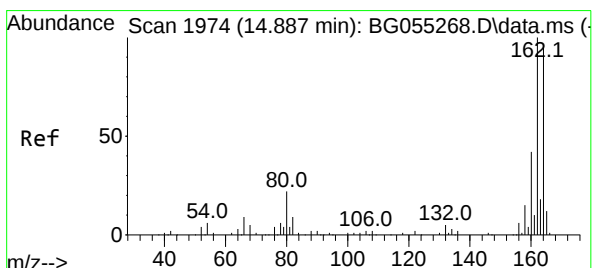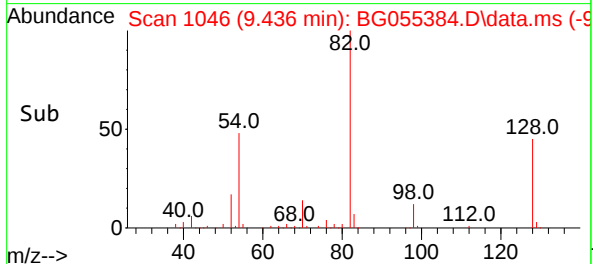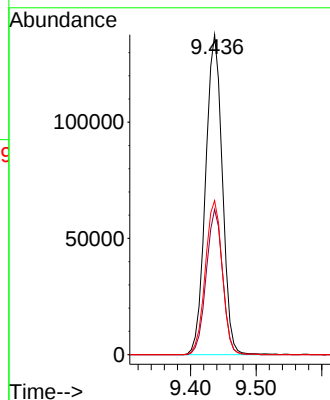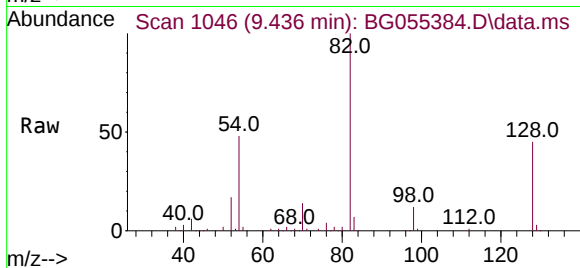

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.871 min Scan# 1971

Delta R.T. -0.009 min

Lab File: BG055384.D

Acq: 31 Oct 2022 18:29




Tgt Ion:164 Resp: 90330


Ion Ratio Lower Upper

164 100

162 105.4 84.0 126.0

160 44.2 36.7 55.1

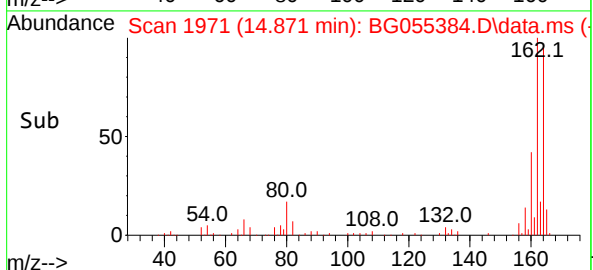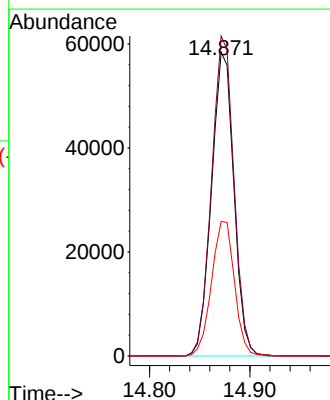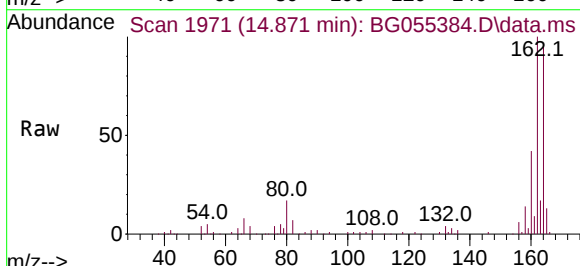

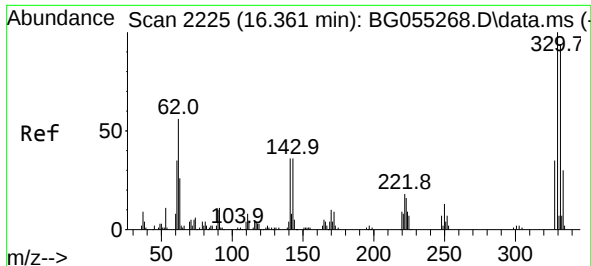

#42

2,4,6-Tribromophenol

Concen: 189.471 ng

RT: 16.352 min Scan# 21

Delta R.T. -0.009 min

Lab File: BG055384.D


Acq: 31 Oct 2022 18:29

Instrument :

BNA_G

ClientSampleId :

COMPOSITE-NW-QUARTER

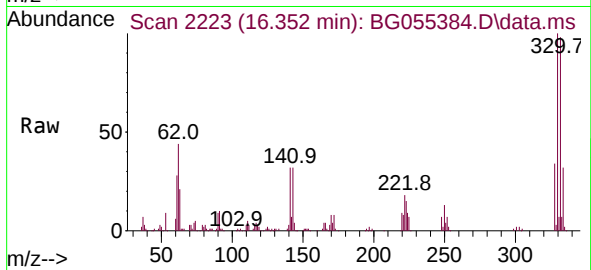




Tgt Ion:330 Resp: 186054

Ion Ratio Lower Upper

330 100

332 96.8 77.4 116.0

141 30.3 29.8 44.8

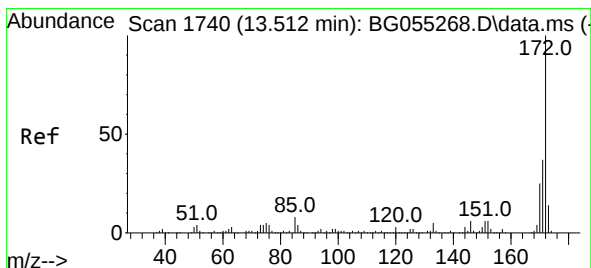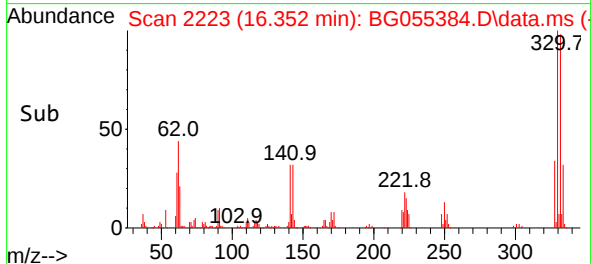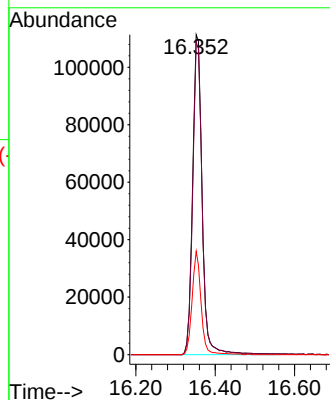

#45

2-Fluorobiphenyl

Concen: 104.687 ng

RT: 13.502 min Scan# 1738

Delta R.T. -0.009 min

Lab File: BG055384.D

Acq: 31 Oct 2022 18:29




Tgt Ion:172 Resp: 577754


Ion Ratio Lower Upper

172 100

171 36.5 29.7 44.5

170 24.8 20.2 30.2


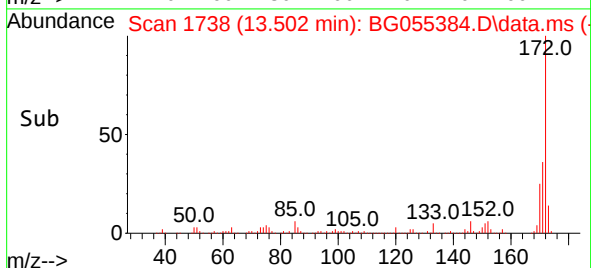
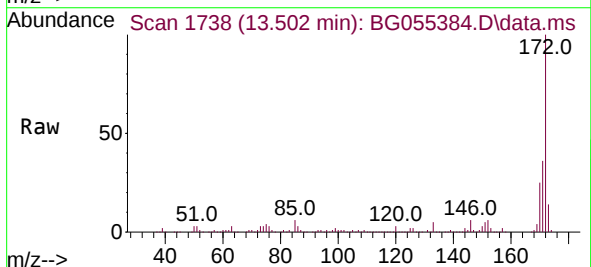
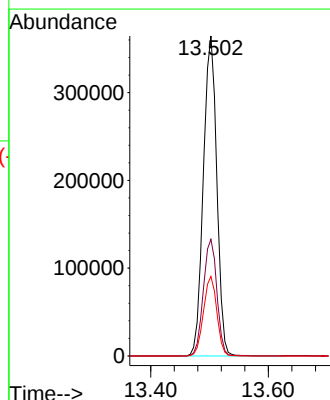


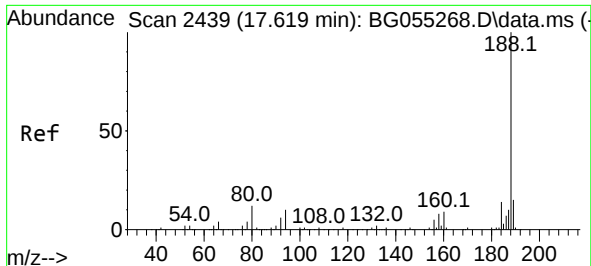

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.609 min Scan# 2439
Delta R.T. -0.003 min
Lab File: BG055384.D
Acq: 31 Oct 2022 18:29




Instrument :
BNA_G
ClientSampleId :
COMPOSITE-NW-QUARTER


Tgt Ion:188 Resp: 197520
Ion Ratio Lower Upper
188 100
94 7.5 8.2 12.4#
80 9.2 10.1 15.1#

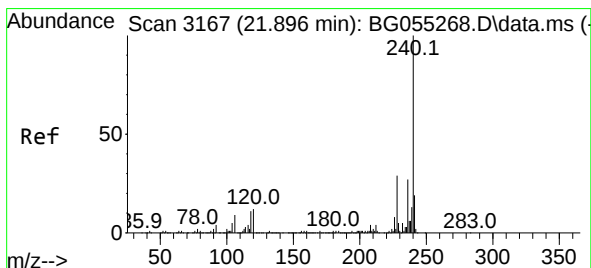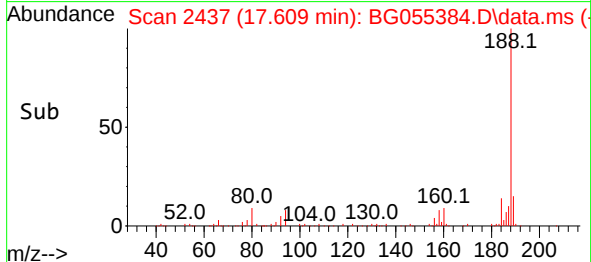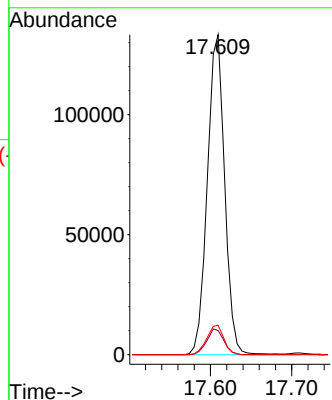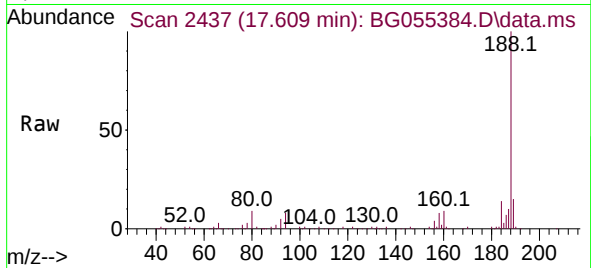

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.881 min Scan# 3164
Delta R.T. -0.009 min
Lab File: BG055384.D
Acq: 31 Oct 2022 18:29

Tgt Ion:240 Resp: 193895
Ion Ratio Lower Upper
240 100
120 9.2 8.9 13.3
236 25.6 21.0 31.4


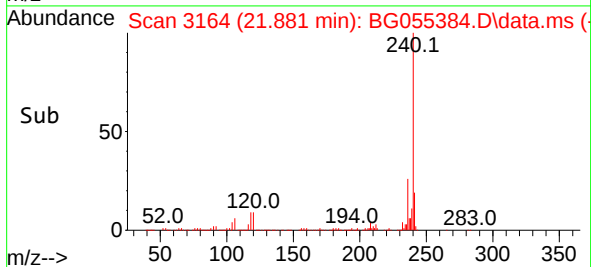
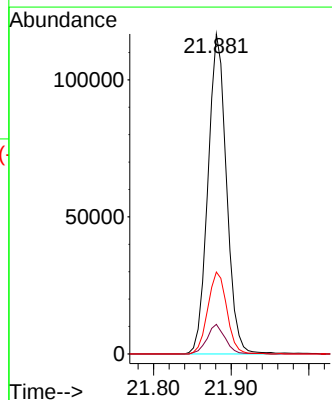
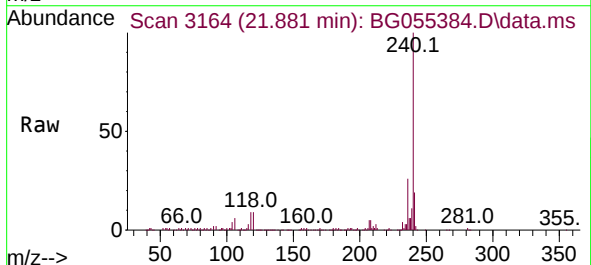


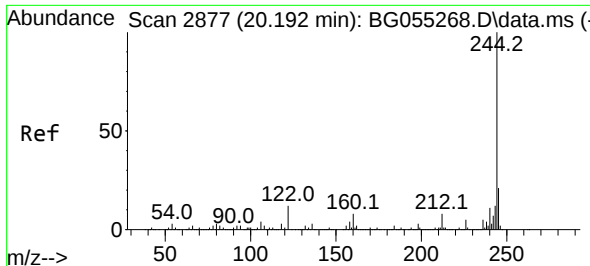

#79
 Terphenyl-d14
 Concen: 103.504 ng
 RT: 20.183 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BG055384.D
 Acq: 31 Oct 2022 18:29

Instrument :
 BNA_G
 ClientSampleId :
 COMPOSITE-NW-QUARTER

Tgt Ion:244 Resp: 965923
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.0 9.0
 122 9.3 9.6 14.4#

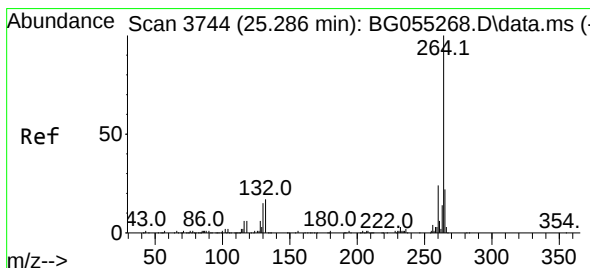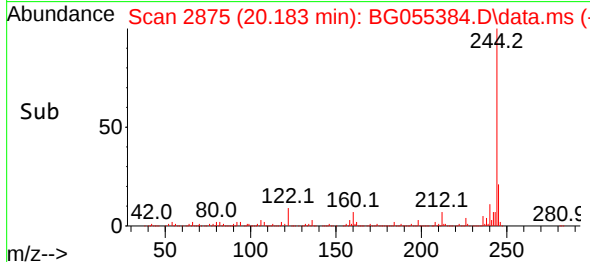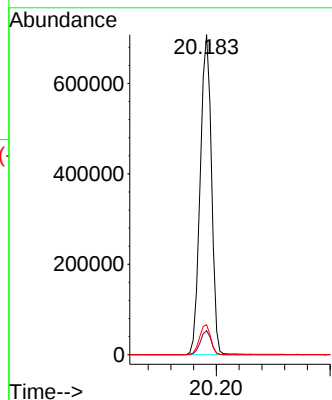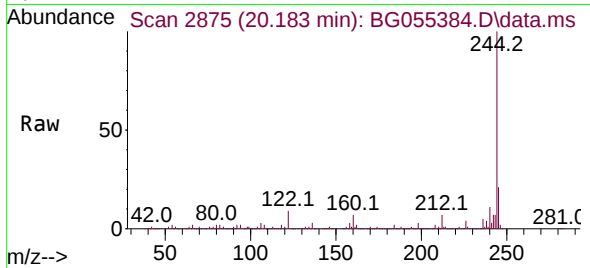

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.277 min Scan# 3742
 Delta R.T. -0.009 min
 Lab File: BG055384.D
 Acq: 31 Oct 2022 18:29

Tgt Ion:264 Resp: 206078
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.5 29.3
 265 21.2 17.4 26.2

