
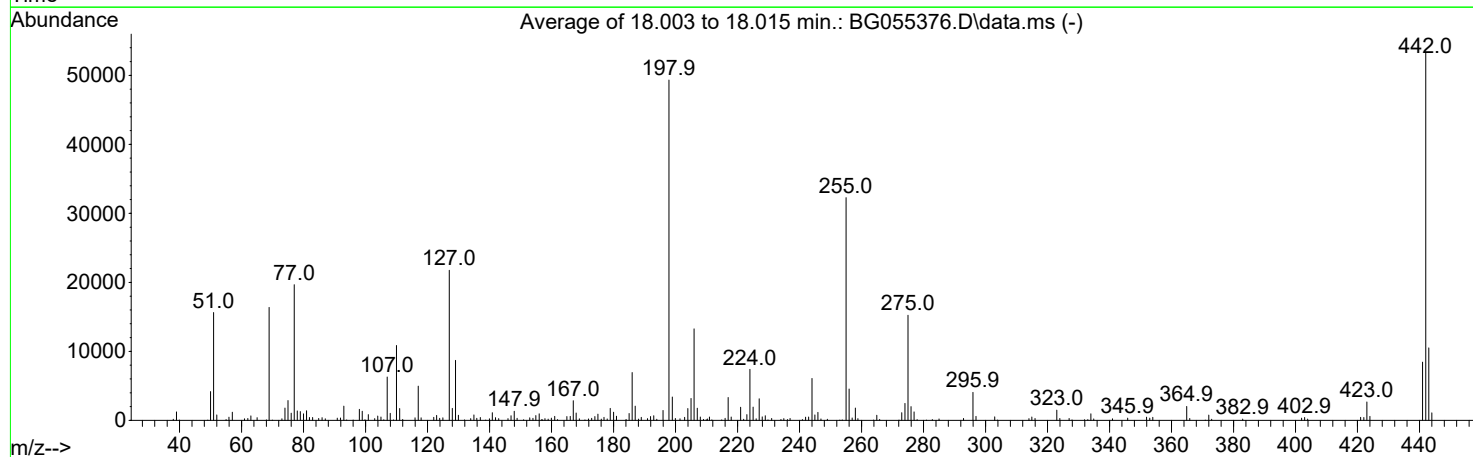


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103122\
 Data File : BG055376.D
 Acq On : 31 Oct 2022 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 29 04:52:38 2022

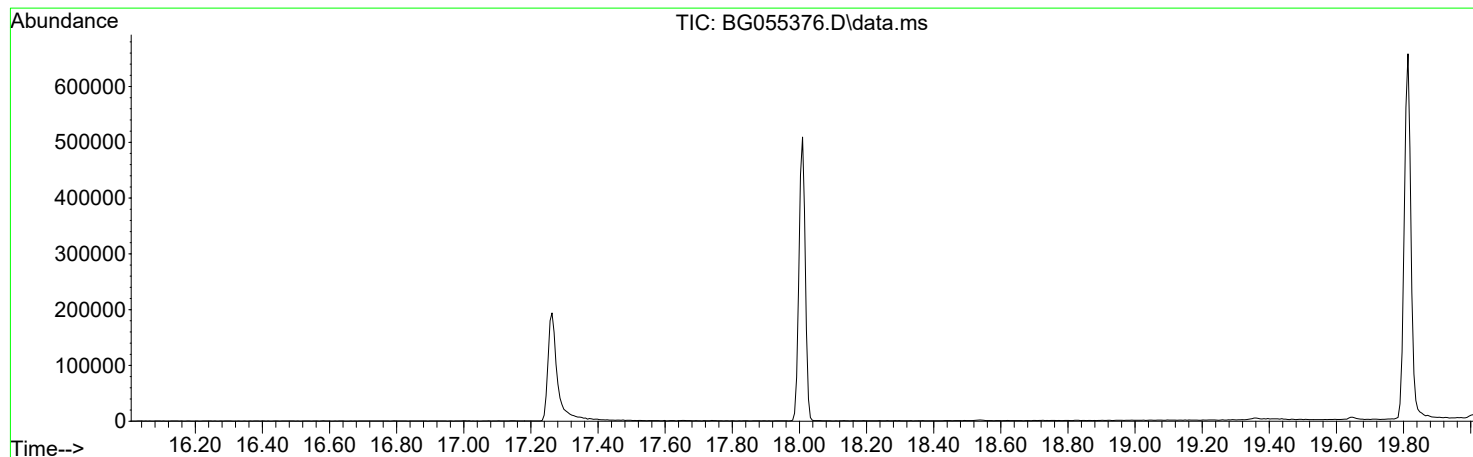




AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	15628	PASS
68	69	0.00	2	0.5	78	PASS
69	198	0.00	100	33.2	16363	PASS
70	69	0.00	2	0.3	53	PASS
127	198	10	80	44.1	21744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49315	PASS
199	198	5	9	6.9	3384	PASS
275	198	10	60	30.9	15226	PASS
365	198	1	100	4.1	2021	PASS
441	198	0.01	100	17.1	8439	PASS
442	442	50	100	100.0	53315	PASS
443	442	15	24	19.7	10504	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103122\
Data File : BG055376.D
Acq On : 31 Oct 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 31 18:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration

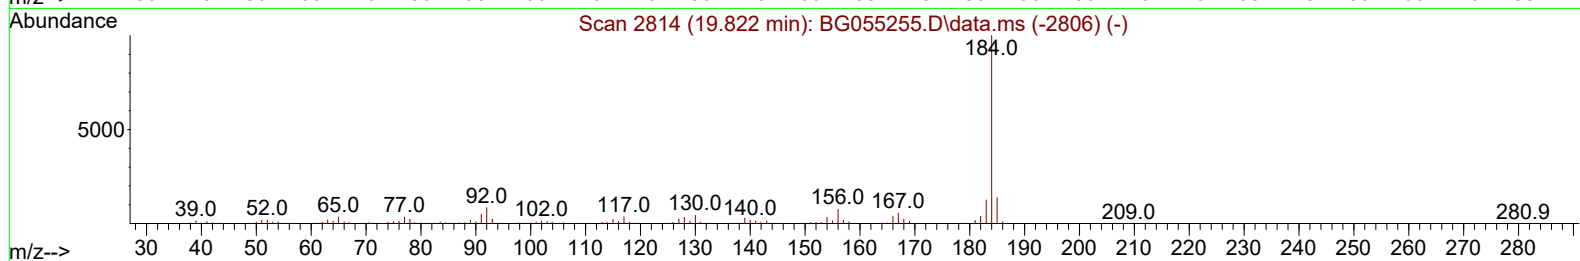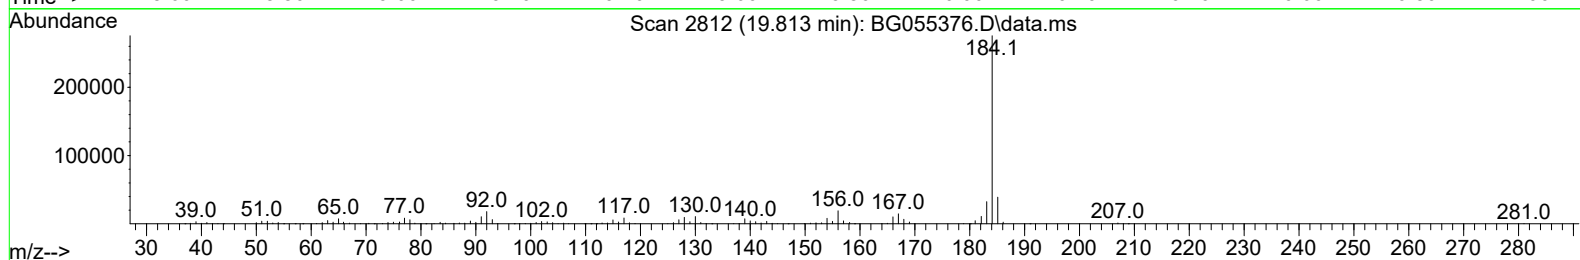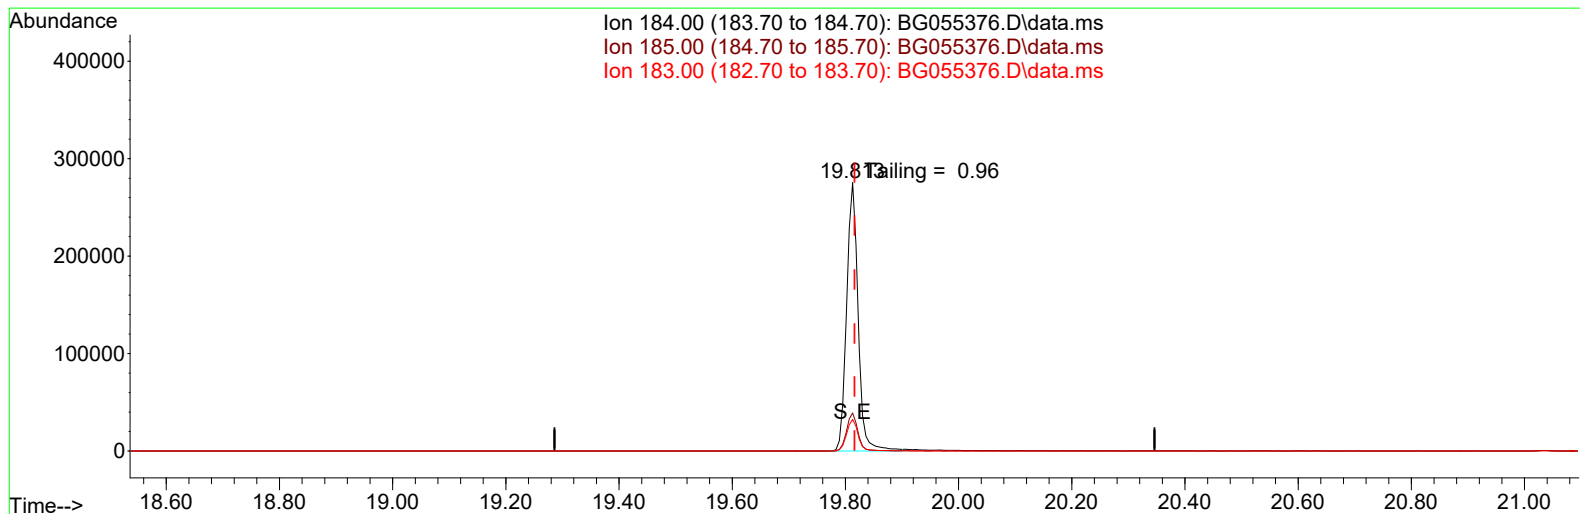

TIC: BG055376.D\data.ms

(77) Benzidine

19.813min (-0.003) 0.00 ng




response 392550

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.21
183.00	12.50	11.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103122\
Data File : BG055376.D
Acq On : 31 Oct 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 31 18:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 04:52:38 2022
Response via : Initial Calibration

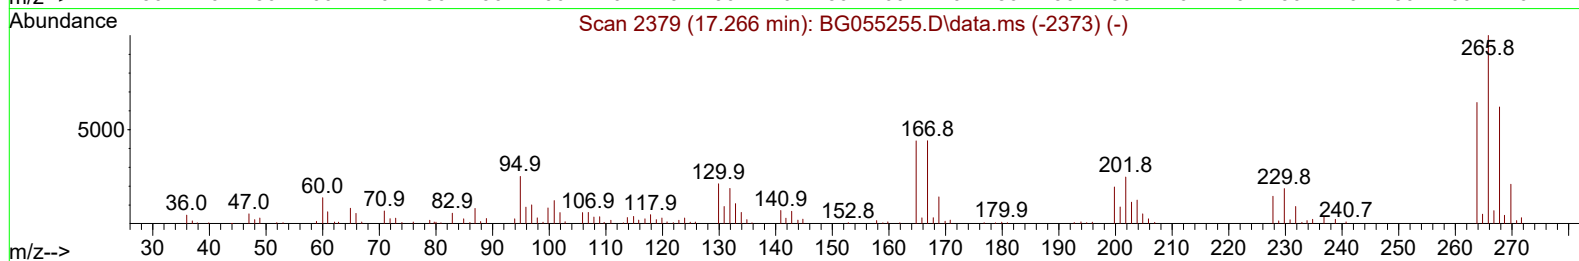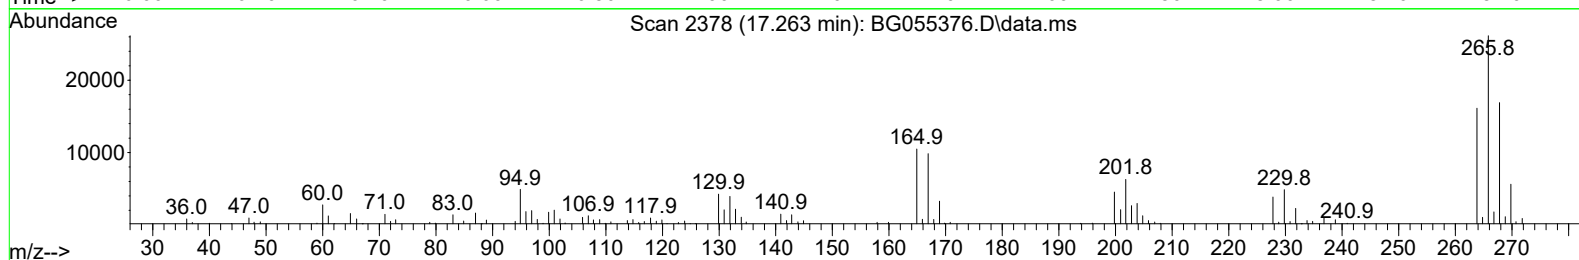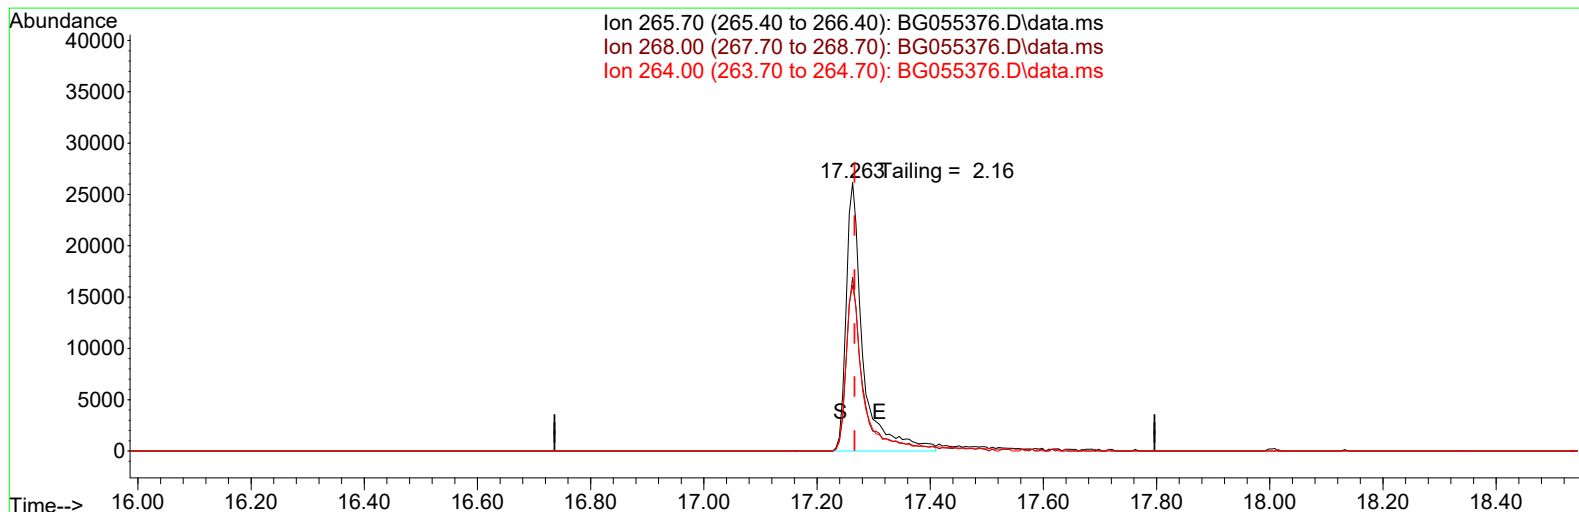

TIC: BG055376.D\data.ms

(70) Pentachlorophenol (C)

17.263min (-0.003) 153644.96 ng

response 54163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	64.61
264.00	64.40	61.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/31/2022	BNA_G	<u>BG055376.D</u>
Compound Name	Response	Retention Time
DDT	177149	21.036
DDD	4094	20.588
DDE	319	20.089
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4413	181562	2.43

Instrument :
BNA_G
ClientSampleId :
DFTPP