
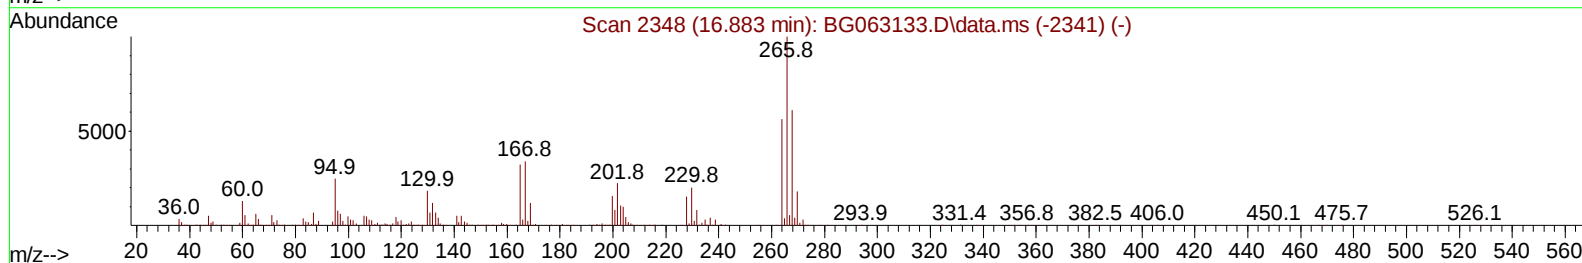
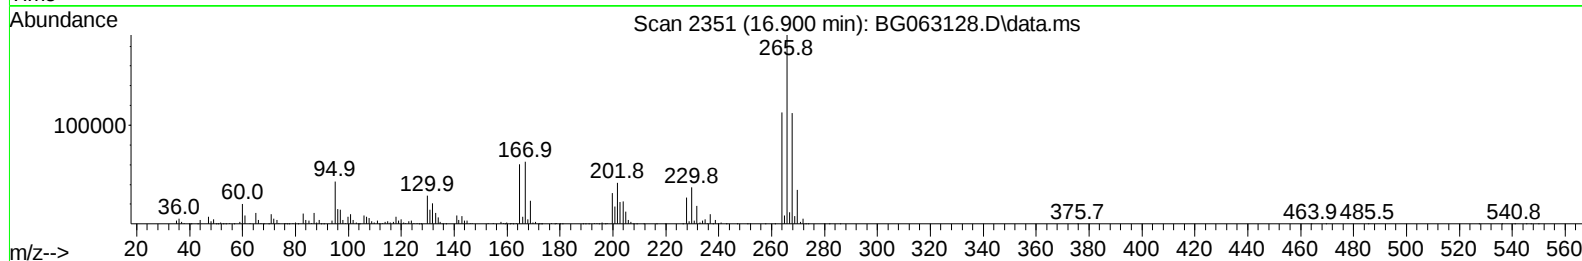


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103124\
Data File : BG063128.D
Acq On : 31 Oct 2024 9:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 03:16:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 01 05:13:40 2024
Response via : Initial Calibration

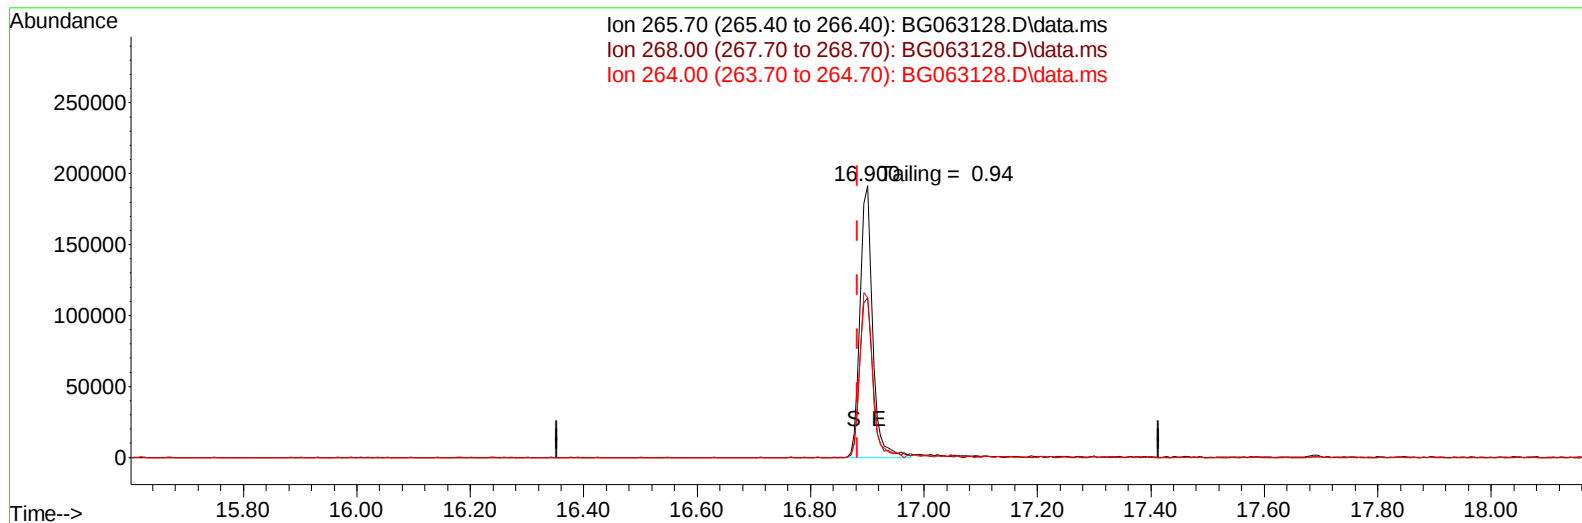

TIC: BG063128.D\data.ms

(70) Pentachlorophenol (C)




16.900min (+ 0.017) 99816.69 ng

response 298245

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	58.72
264.00	56.20	58.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG103124\
Data File : BG063128.D
Acq On : 31 Oct 2024 9:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 04 03:16:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG103124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 01 05:13:40 2024
Response via : Initial Calibration

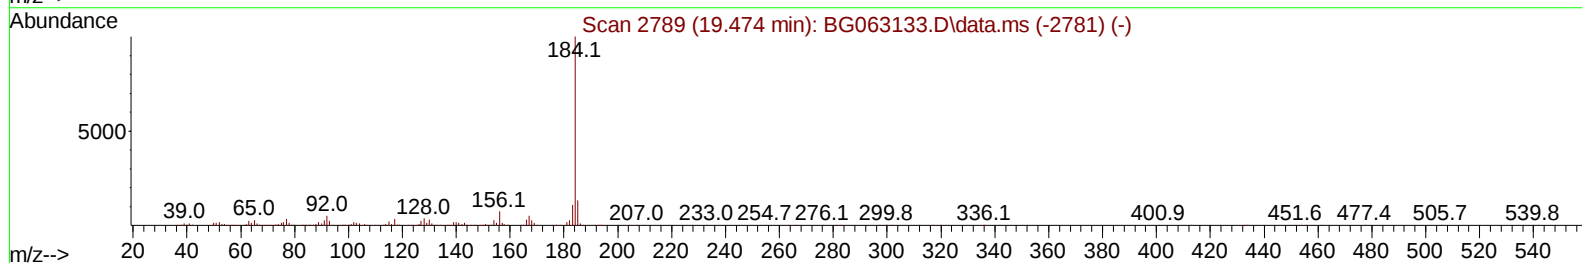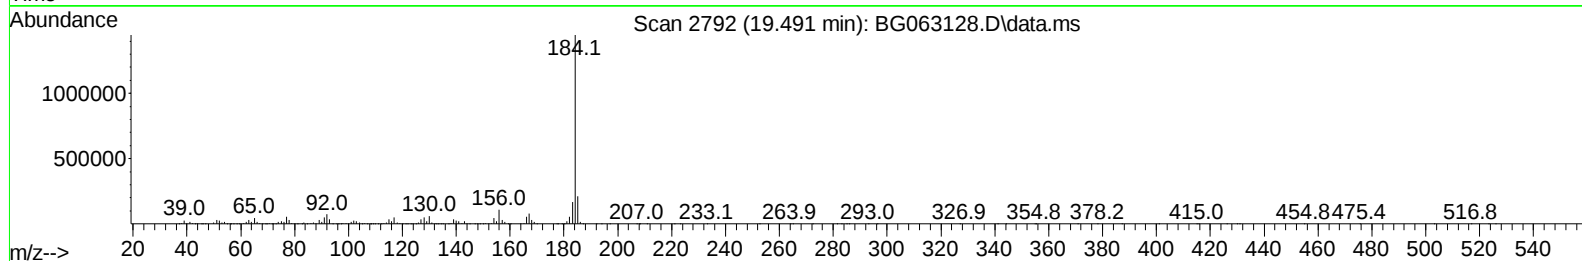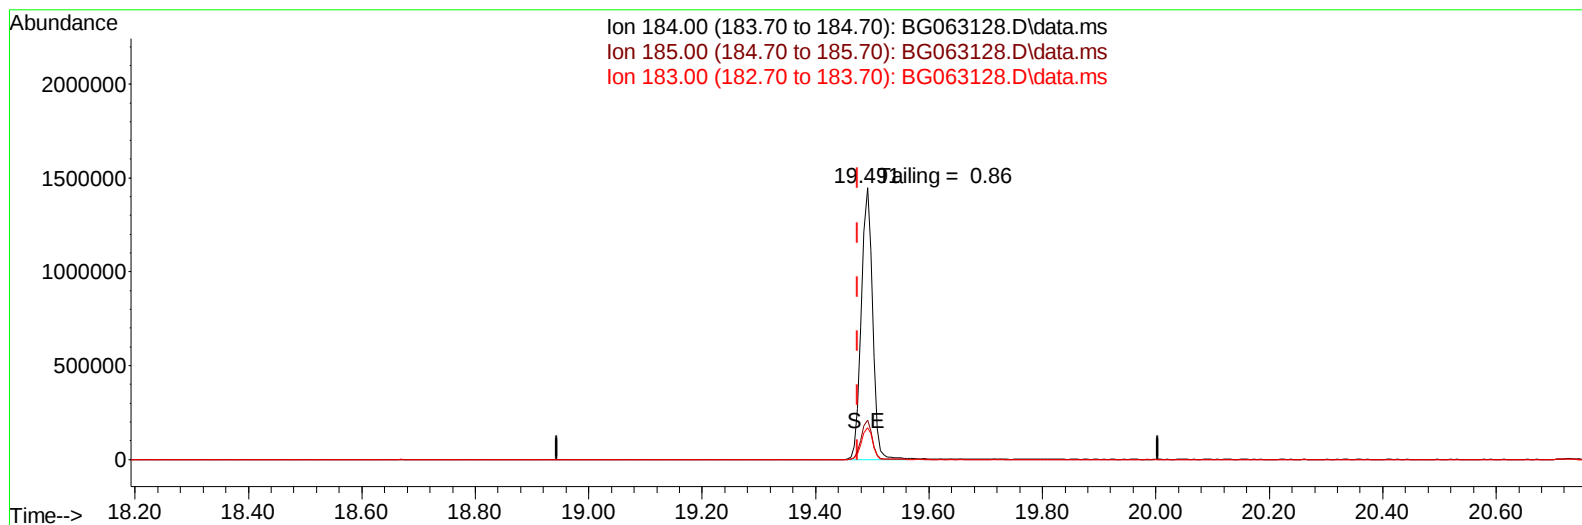

TIC: BG063128.D\data.ms

(77) Benzidine**19.491min (+ 0.017) 238302.28 ng****response 2004718**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.52
183.00	10.70	11.71
0.00	0.00	0.00