
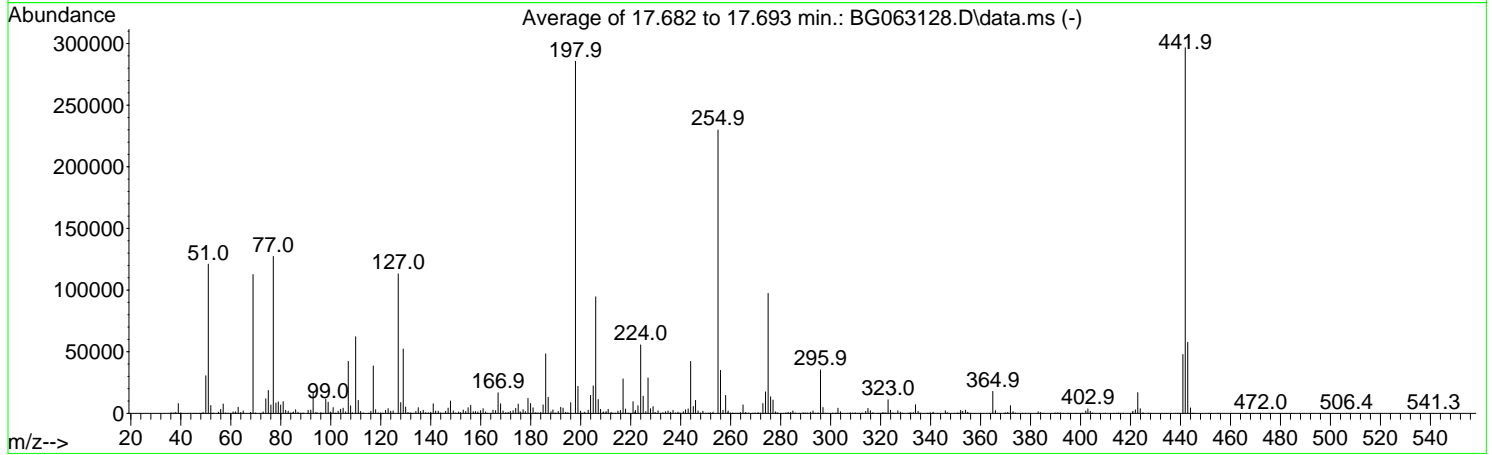


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG103124\  
 Data File : BG063128.D  
 Acq On : 31 Oct 2024 9:02  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_G  
**ClientSampleId :**  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG103124.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Nov 01 05:13:40 2024

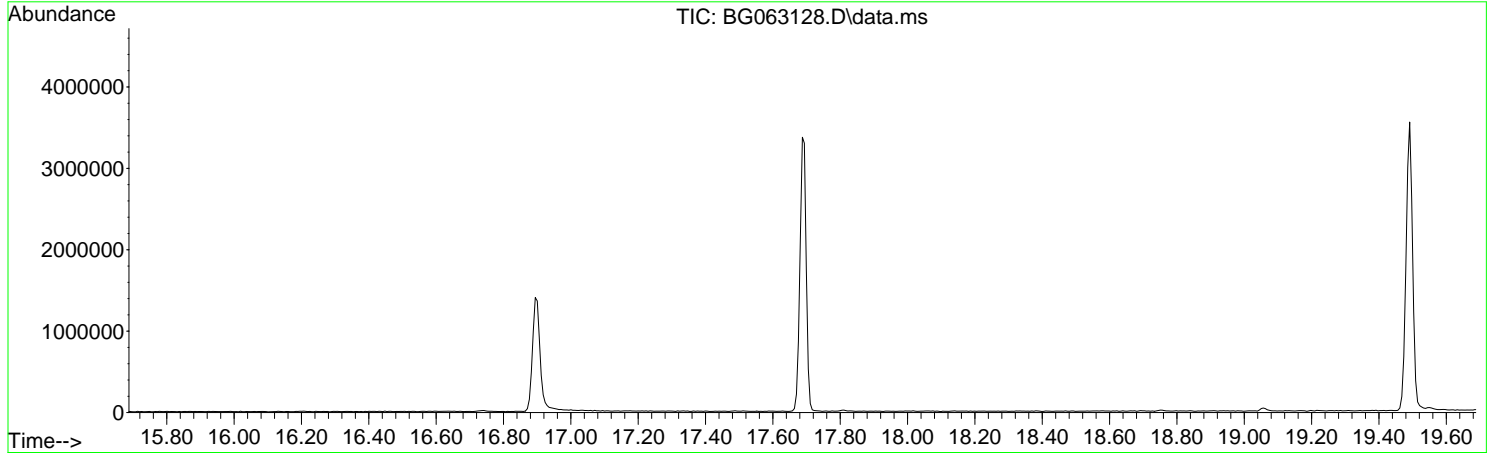




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	121053	PASS
68	69	0.00	2	0.7	792	PASS
69	198	0.00	100	39.4	112653	PASS
70	69	0.00	2	0.3	372	PASS
127	198	10	80	39.6	113163	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	285589	PASS
199	198	5	9	7.7	21956	PASS
275	198	10	60	34.1	97328	PASS
365	198	1	100	6.2	17849	PASS
441	198	0.01	100	16.7	47800	PASS
442	442	50	100	100.0	296619	PASS
443	442	15	24	19.4	57683	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG103124\  
 Data File : BG063128.D  
 Acq On : 31 Oct 2024 9:02  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_G  
**ClientSampleId :**  
 DFTPP

Quant Time: Nov 04 03:16:12 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG103124.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Nov 01 05:13:40 2024  
 Response via : Initial Calibration

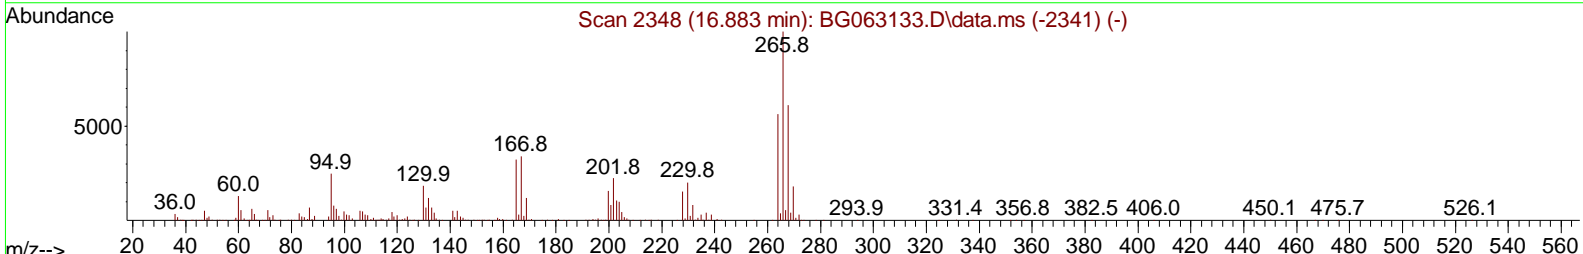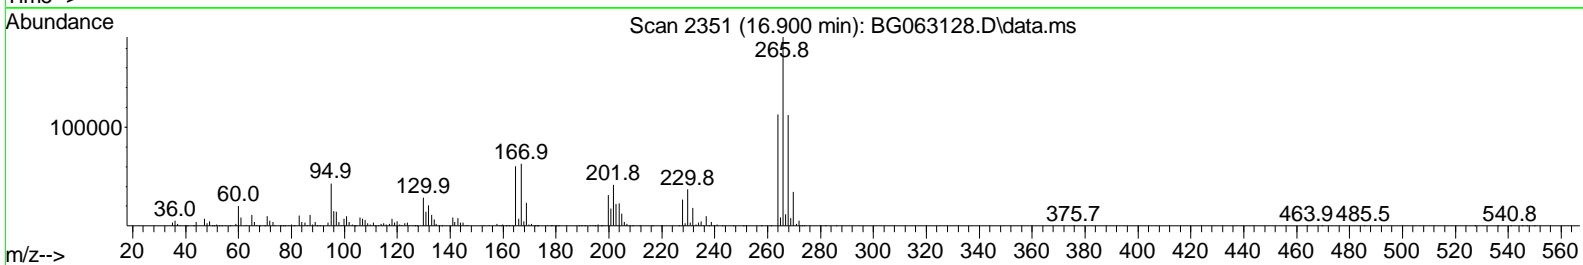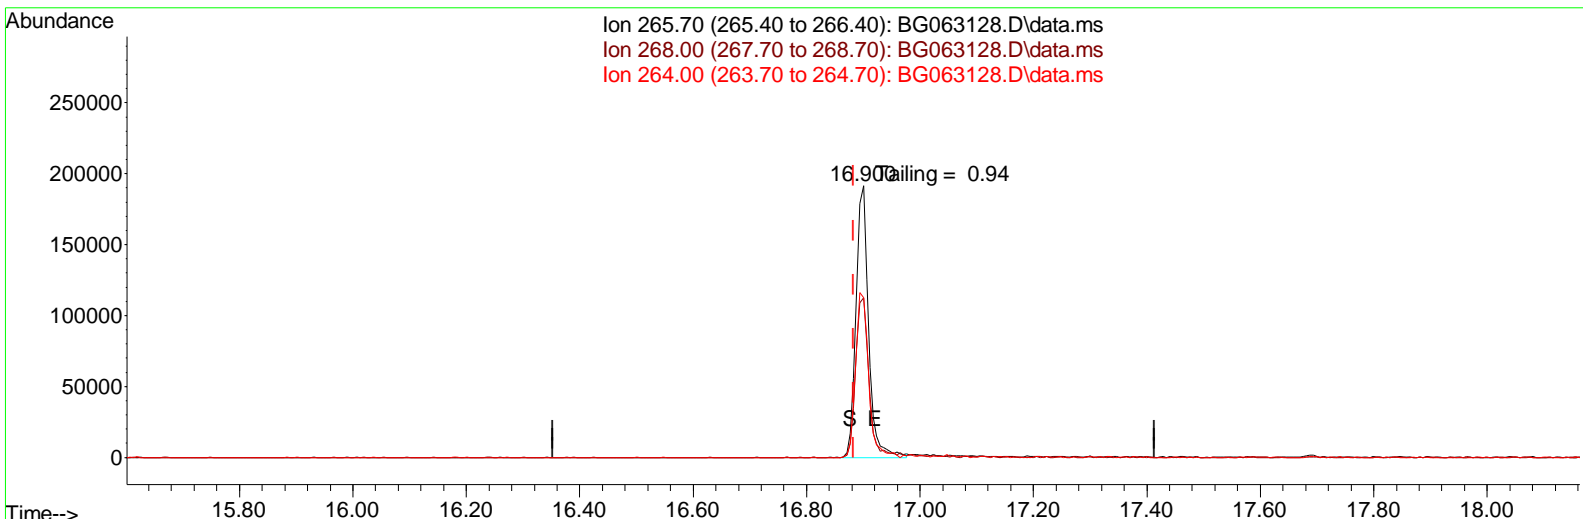

TIC: BG063128.D\data.ms

(70) Pentachlorophenol (C)

16.900min (+ 0.017) 99816.69 ng




response 298245

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	58.72
264.00	56.20	58.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG103124\  
 Data File : BG063128.D  
 Acq On : 31 Oct 2024 9:02  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_G  
**ClientSampleId :**  
 DFTPP

Quant Time: Nov 04 03:16:12 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG103124.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Nov 01 05:13:40 2024  
 Response via : Initial Calibration

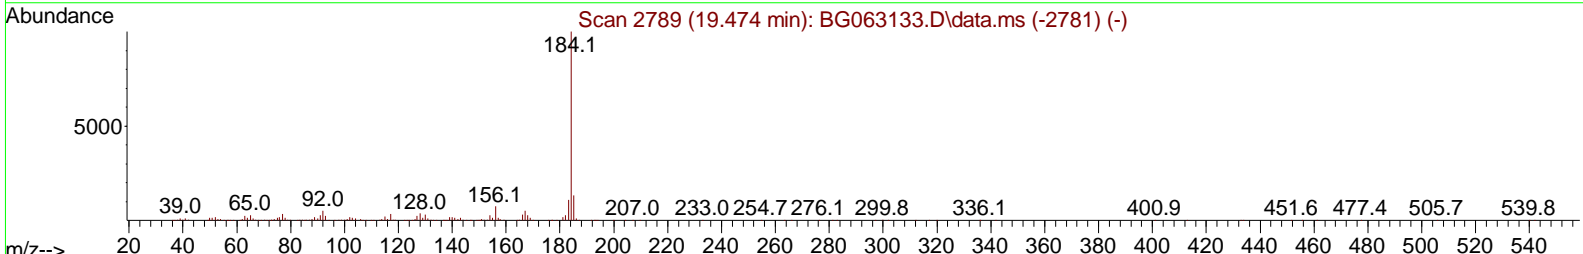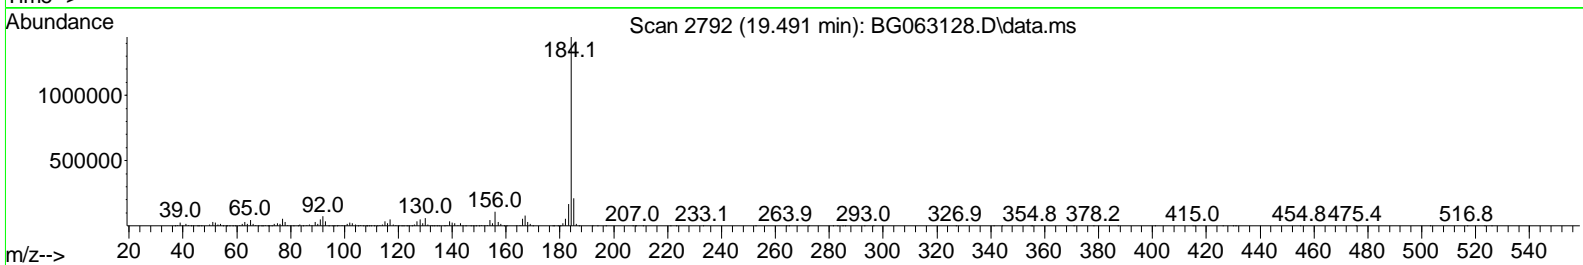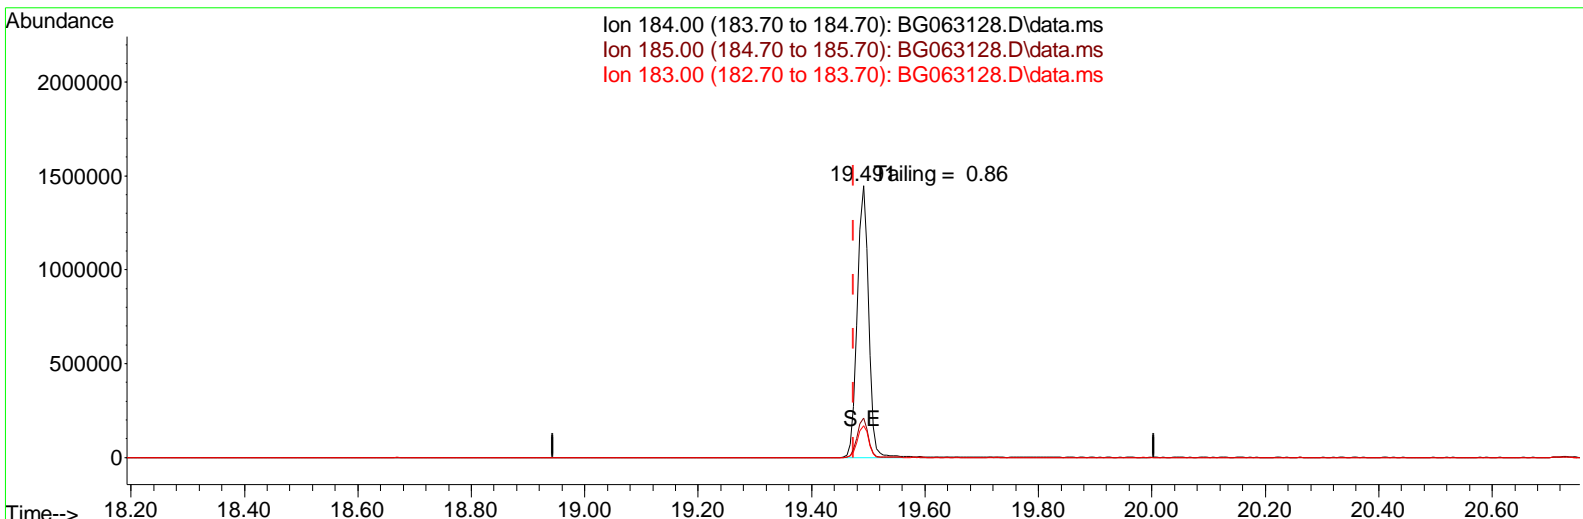

TIC: BG063128.D\data.ms

(77) Benzidine

19.491min (+ 0.017) 238302.28 ng

response 2004718

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.52
183.00	10.70	11.71
0.00	0.00	0.00

**DDT Breakdown**

Date	Instrument Name	DFTPP Data File
10/31/2024	BNA_G	<u>BG063128.D</u>
Compound Name	Response	Retention Time
DDT	1082788	20.725
DDD	18145	20.343
DDE	0	19.77
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18145	1100933	1.65

Instrument :  
 BNA\_G  
 ClientSampled :  
 DFTPP