

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110116\
 Data File : BG024603.D
 Acq On : 1 Nov 2016 21:44
 Operator : UM/SJ
 Sample : H5489-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-71-0.5-1.0

Quant Time: Nov 02 02:20:44 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	121171	20.00	ng	0.00
21) Naphthalene-d8	11.09	136	469746	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	355815	20.00	ng	0.00
63) Phenanthrene-d10	17.63	188	782301	20.00	ng	0.00
75) Chrysene-d12	21.92	240	1080542	20.00	ng	-0.01
86) Perylene-d12	25.35	264	1137268	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	1149932	155.54	ng	0.00
7) Phenol-d6	7.40	99	1648589	162.56	ng	0.00
23) Nitrobenzene-d5	9.44	82	1165134	112.93	ng	0.00
41) 2,4,6-Tribromophenol	16.37	330	848640	159.65	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	2310683	107.94	ng	0.00
78) Terphenyl-d14	20.21	244	3477083	96.15	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.32	163	628254	24.87	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110116\
Data File : BG024603.D
Acq On : 1 Nov 2016 21:44
Operator : UM/SJ
Sample : H5489-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-71-0.5-1.0

Quant Time: Nov 02 02:20:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

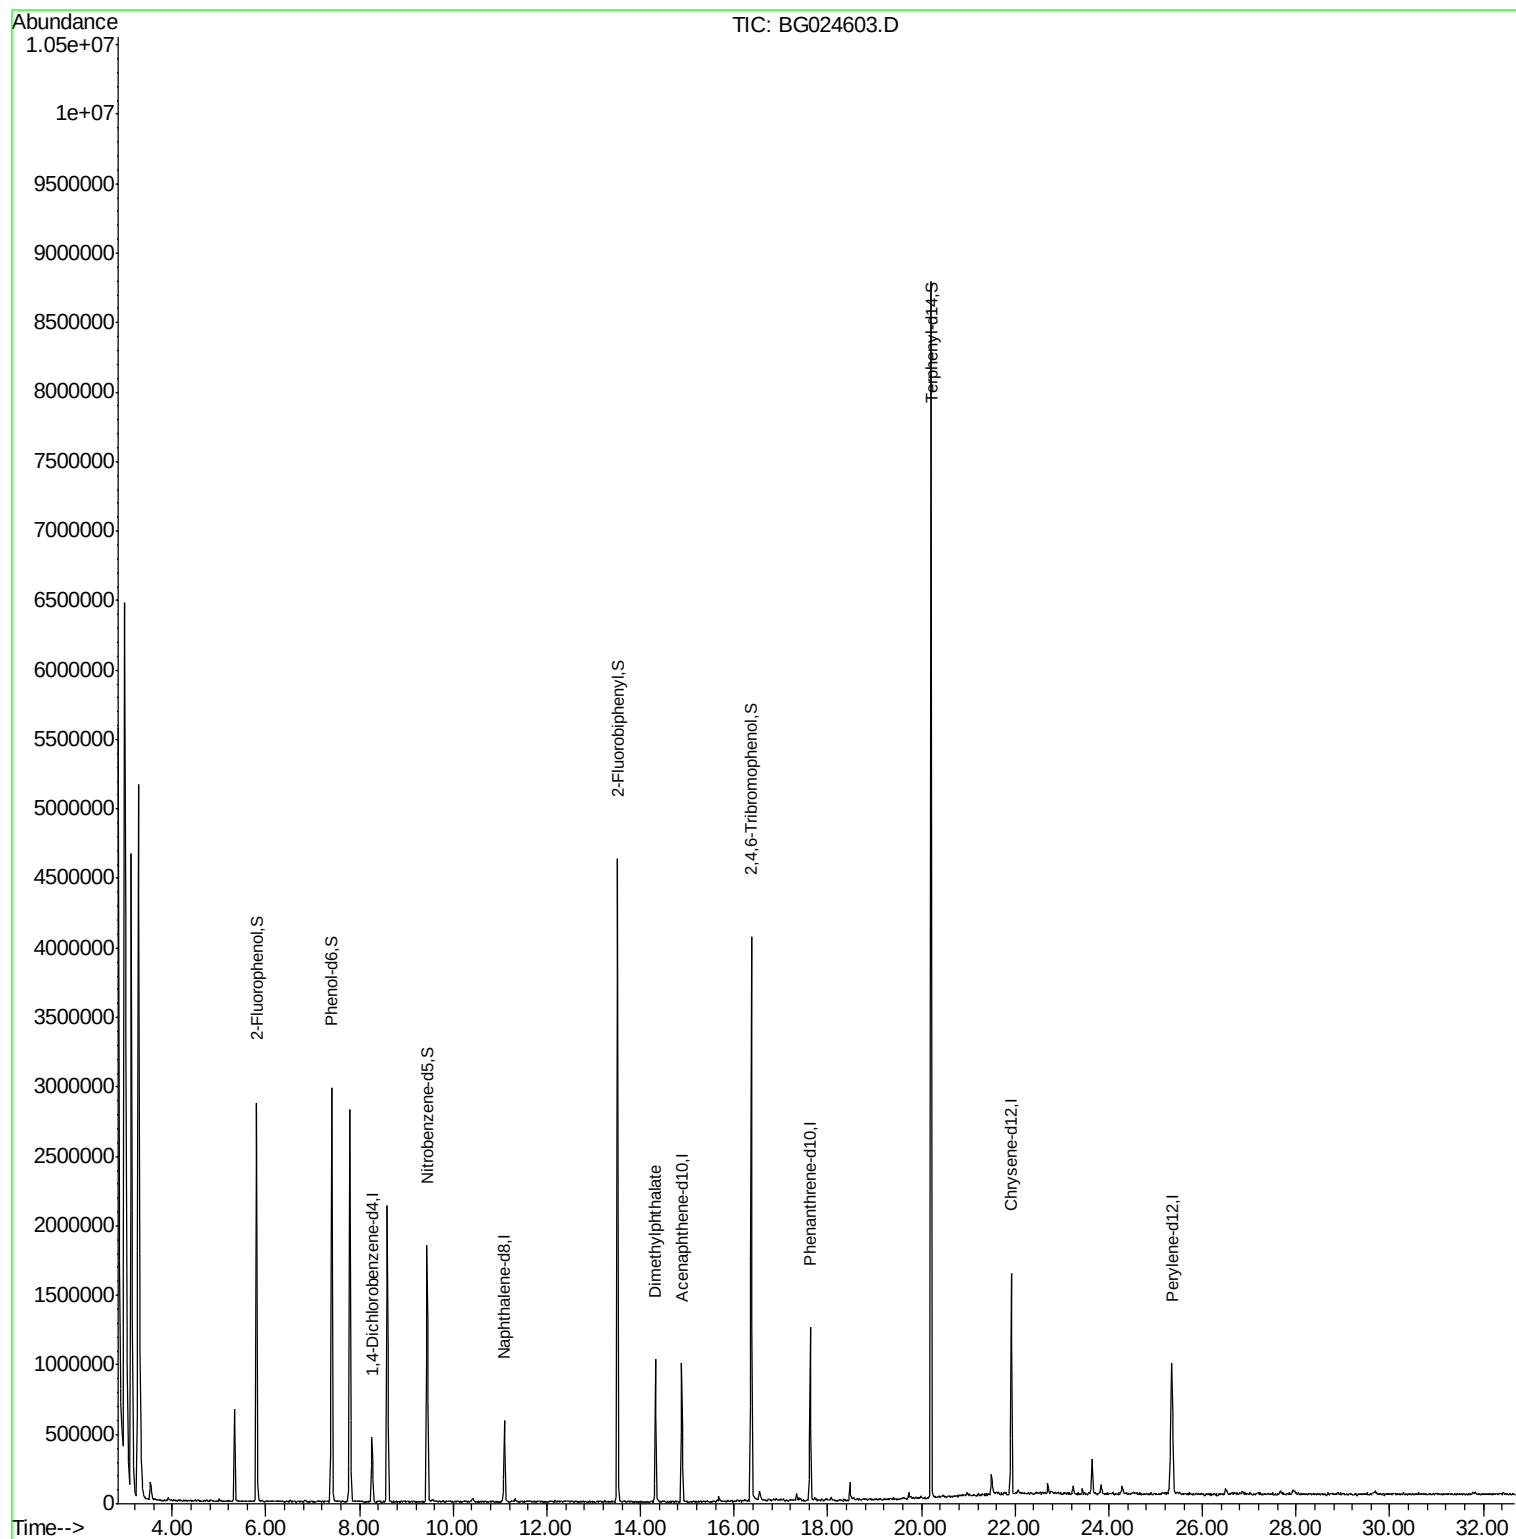







#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.27 min Scan# 924
Delta R.T. -0.00 min
Lab File: BG024603.D
Acq: 1 Nov 2016 21:44

Instrument :
BNA_G
ClientSampleId :
SB-71-0.5-1.0




Tgt Ion:152 Resp: 121171
Ion Ratio Lower Upper
152 100
150 162.9 114.0 171.0
115 61.7 48.1 72.1

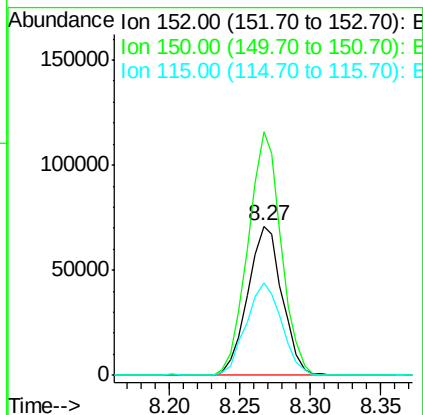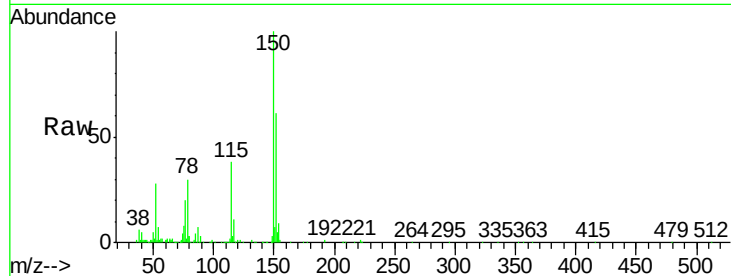


#5

2-Fluorophenol
Concen: 155.54 ng
RT: 5.80 min Scan# 504
Delta R.T. 0.00 min
Lab File: BG024603.D
Acq: 1 Nov 2016 21:44

Tgt Ion:112 Resp: 1149932
Ion Ratio Lower Upper
112 100
64 74.8 61.8 92.6
63 43.5 37.2 55.8

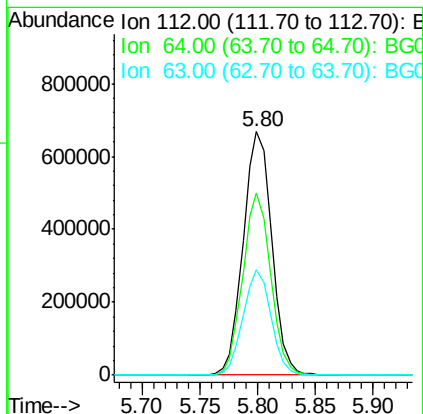

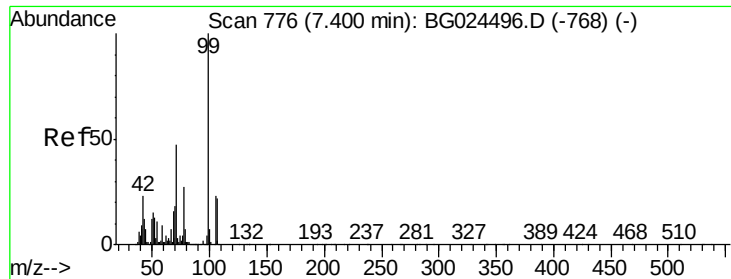

#7

Phenol-d6

Concen: 162.56 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024603.D

Acq: 1 Nov 2016 21:44

Instrument :

BNA_G

ClientSampleId :

SB-71-0.5-1.0


Tgt Ion: 99 Resp: 1648589

Ion Ratio Lower Upper




99 100

42 22.3 20.5 30.7

71 47.8 37.6 56.4



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

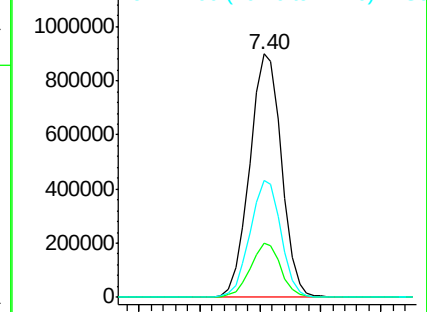

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.09 min Scan# 1405

Delta R.T. -0.01 min

Lab File: BG024603.D

Acq: 1 Nov 2016 21:44

Tgt Ion: 136 Resp: 469746


Ion Ratio Lower Upper

136 100



137 11.2 8.9 13.3


54 10.0 9.3 13.9

68 5.7 5.1 7.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




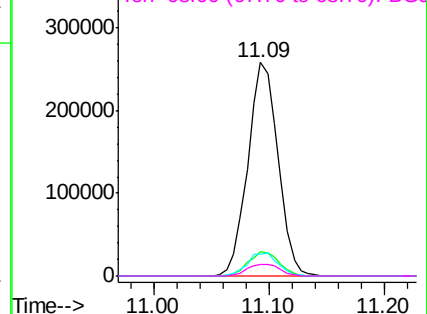


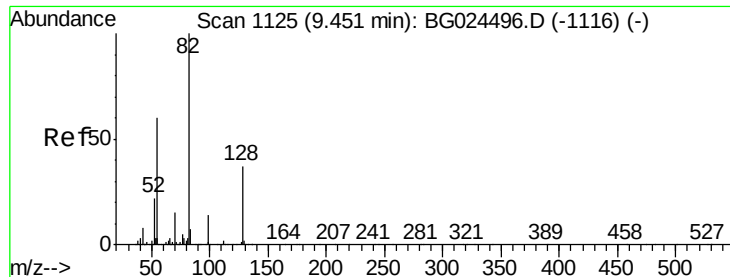

#23
 Nitrobenzene-d5
 Concen: 112.93 ng
 RT: 9.44 min Scan# 1124
 Delta R.T. -0.01 min
 Lab File: BG024603.D
 Acq: 1 Nov 2016 21:44




Instrument :
 BNA_G
 ClientSampleId :
 SB-71-0.5-1.0


Tgt Ion: 82 Resp: 1165134
 Ion Ratio Lower Upper
 82 100
 128 34.0 26.4 39.6
 54 53.4 49.4 74.2

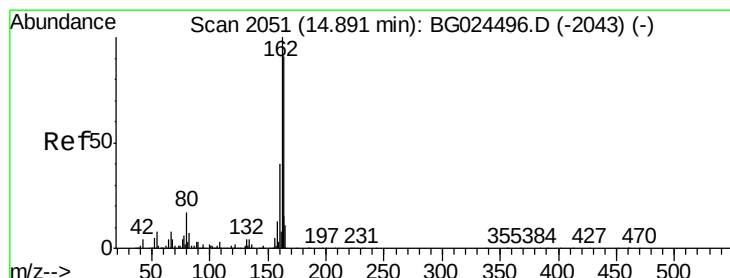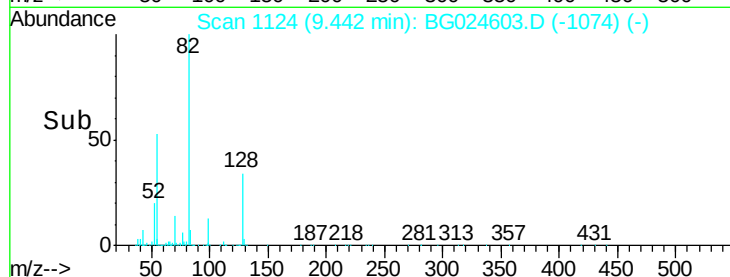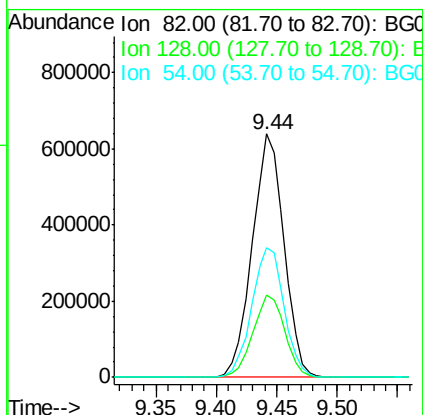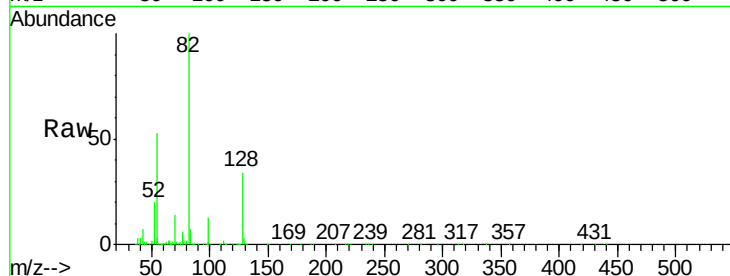

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.88 min Scan# 2050
 Delta R.T. -0.01 min
 Lab File: BG024603.D
 Acq: 1 Nov 2016 21:44

Tgt Ion: 164 Resp: 355815
 Ion Ratio Lower Upper
 164 100
 162 102.4 85.1 127.7
 160 40.4 34.7 52.1

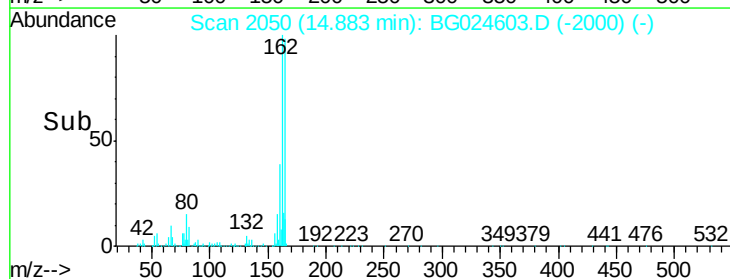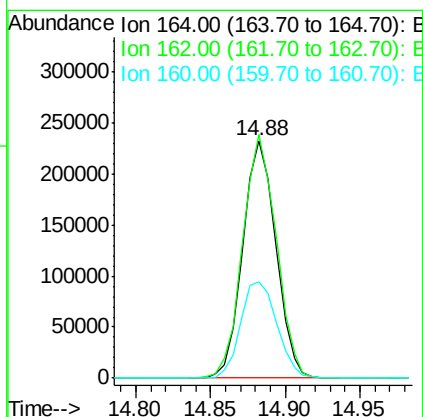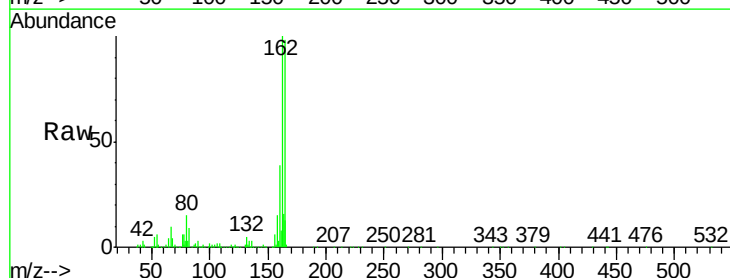



#41

2,4,6-Tribromophenol

Concen: 159.65 ng

RT: 16.37 min Scan# 2303

Delta R.T. -0.00 min

Lab File: BG024603.D

Acq: 1 Nov 2016 21:44

Instrument :

BNA_G

ClientSampleId :

SB-71-0.5-1.0


Tgt Ion:330 Resp: 848640

Ion Ratio Lower Upper

330 100

332 98.0 77.3 115.9




141 31.8 32.1 48.1#

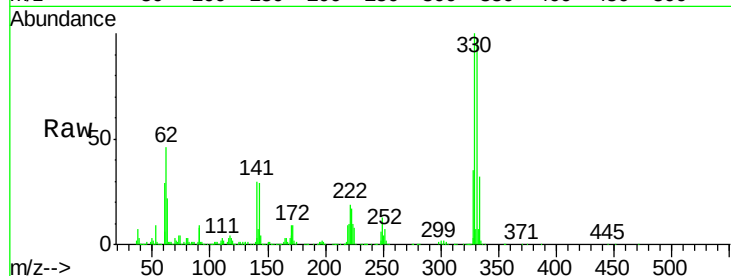

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

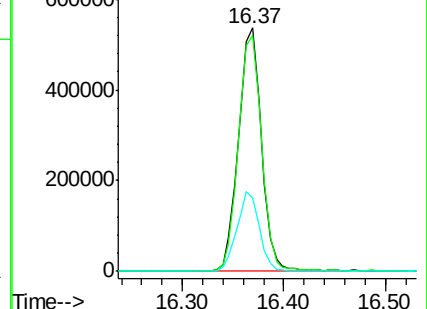

#44

2-Fluorobiphenyl

Concen: 107.94 ng

RT: 13.51 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BG024603.D

Acq: 1 Nov 2016 21:44


Tgt Ion:172 Resp: 2310683

Ion Ratio Lower Upper

172 100

171 40.8 32.2 48.2



170 26.4 21.8 32.6




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

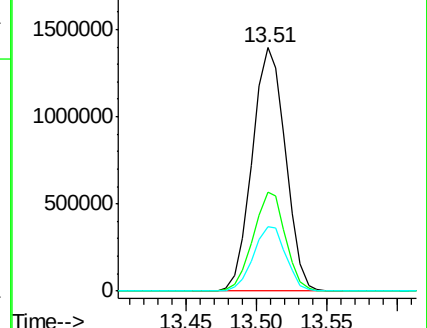



#49

Dimethylphthalate

Concen: 24.87 ng

RT: 14.32 min Scan# 1955

Delta R.T. -0.01 min

Lab File: BG024603.D

Acq: 1 Nov 2016 21:44

Instrument :

BNA_G

ClientSampleId :

SB-71-0.5-1.0


Tgt Ion:163 Resp: 628254

Ion Ratio Lower Upper

163 100

194 4.9 3.8 5.6




164 9.9 9.3 13.9

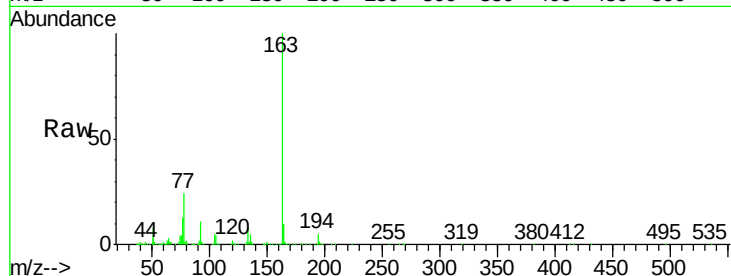

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

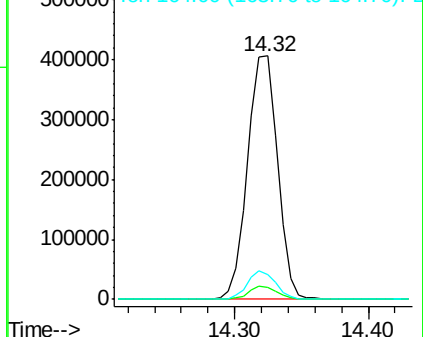

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.63 min Scan# 2517

Delta R.T. -0.00 min

Lab File: BG024603.D

Acq: 1 Nov 2016 21:44


Tgt Ion:188 Resp: 782301

Ion Ratio Lower Upper

188 100

94 7.5 5.8 8.8



80 8.8 7.5 11.3




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



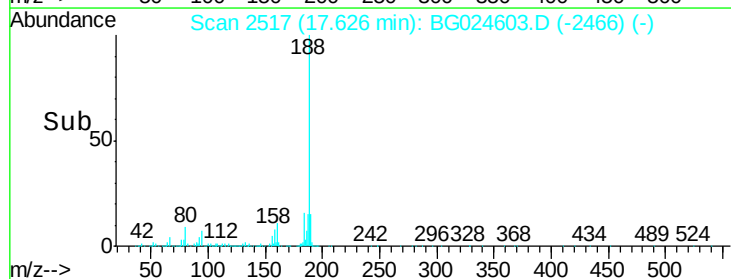
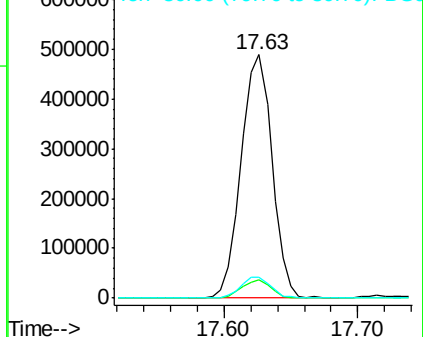


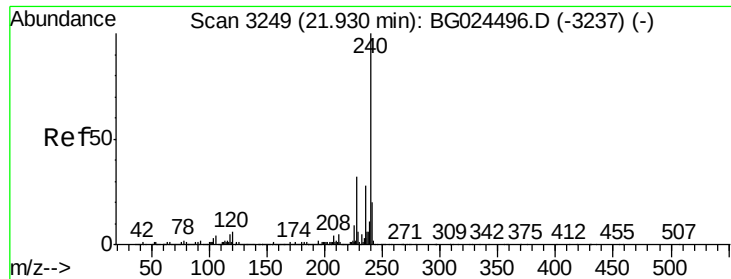

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.92 min Scan# 3247
Delta R.T. -0.01 min
Lab File: BG024603.D
Acq: 1 Nov 2016 21:44




Instrument :
BNA_G
ClientSampleId :
SB-71-0.5-1.0


Tgt Ion:240 Resp: 1080542
Ion Ratio Lower Upper
240 100
120 6.7 5.7 8.5
236 27.2 22.2 33.4

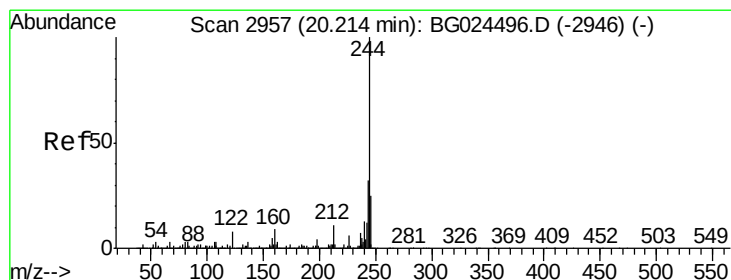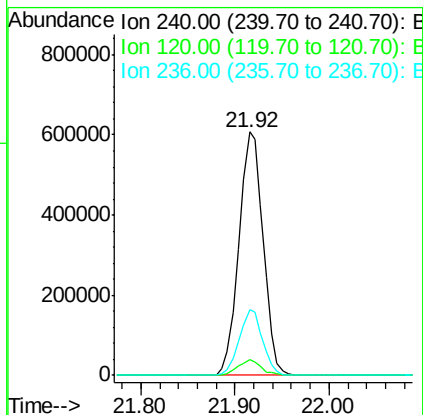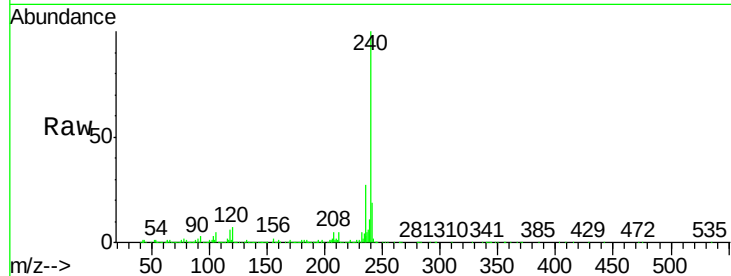

#78
Terphenyl-d14
Concen: 96.15 ng
RT: 20.21 min Scan# 2956
Delta R.T. -0.01 min
Lab File: BG024603.D
Acq: 1 Nov 2016 21:44

Tgt Ion:244 Resp: 3477083
Ion Ratio Lower Upper
244 100
212 12.3 10.0 15.0
122 10.5 8.6 12.8

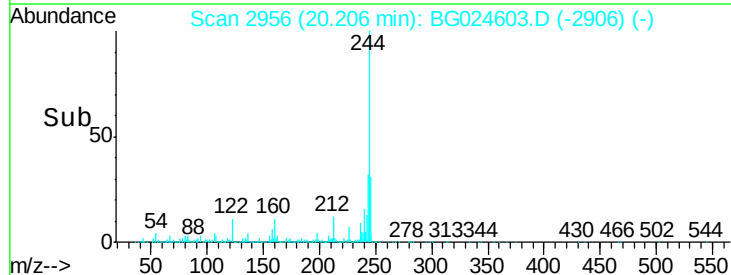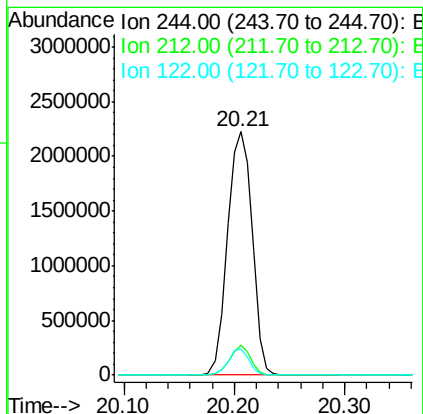

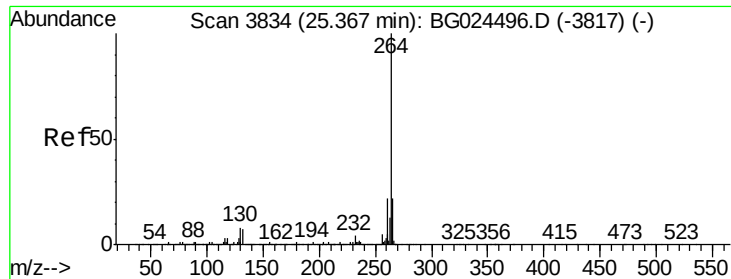

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.35 min Scan# 3831
Delta R.T. -0.02 min
Lab File: BG024603.D
Acq: 1 Nov 2016 21:44

Instrument :
BNA_G
ClientSampleId :
SB-71-0.5-1.0

Tgt Ion:264 Resp: 1137268

Ion	Ratio	Lower	Upper
264	100		
260	23.1	21.8	32.8
265	20.6	18.2	27.4

