
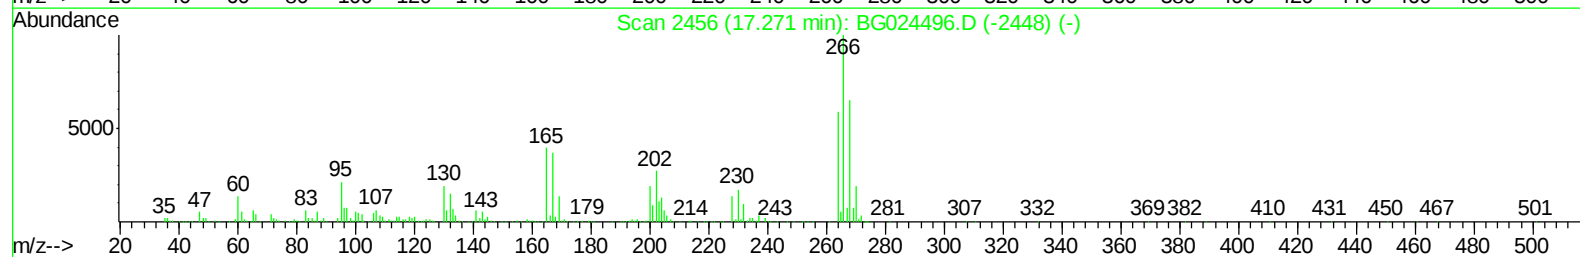
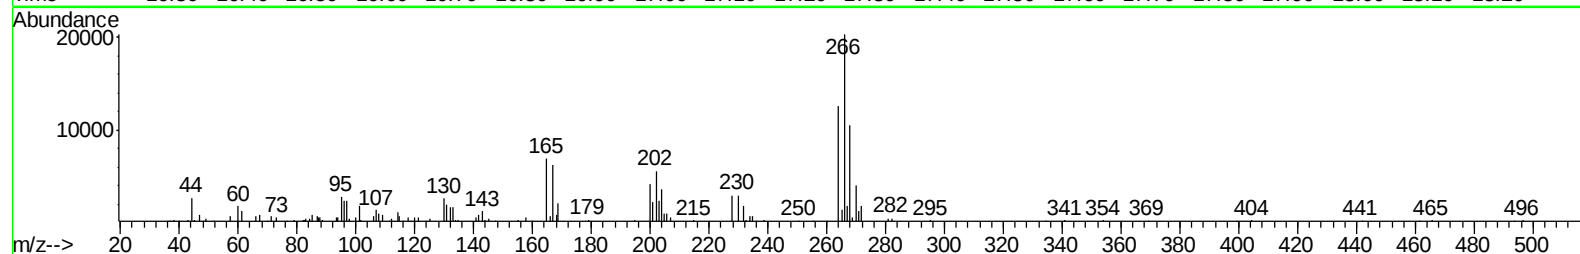


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110116\
Data File : BG024608.D
Acq On : 2 Nov 2016 1:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:15:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

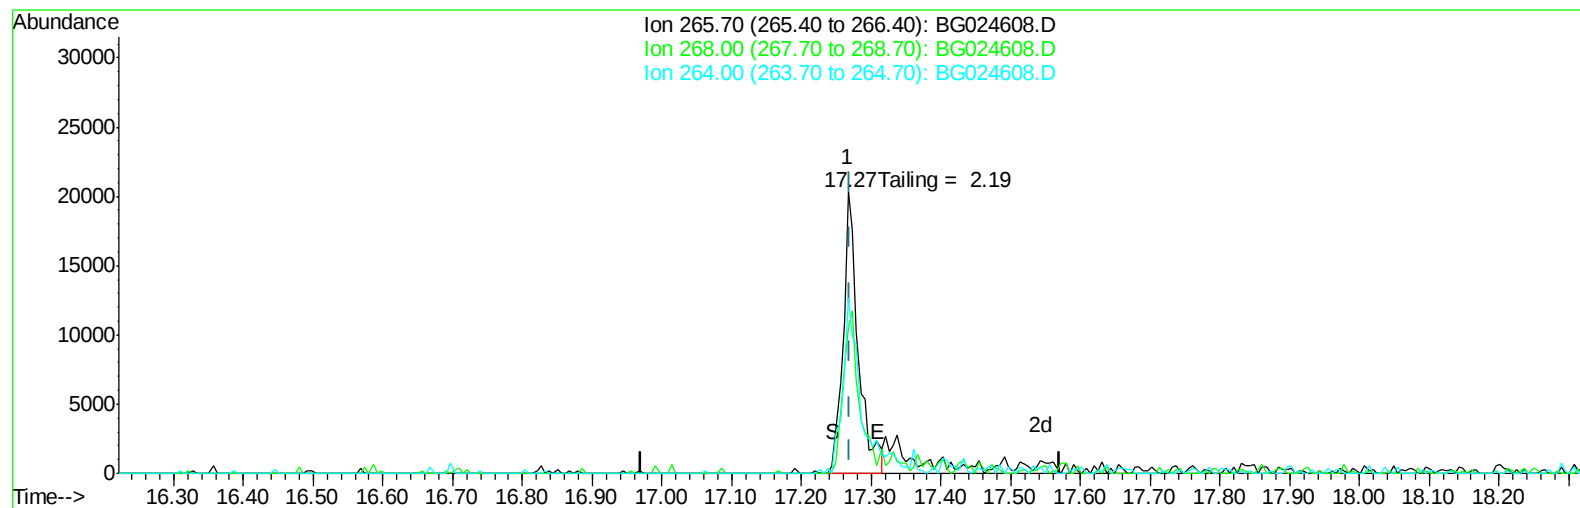

TIC: BG024608.D

(69) Pentachlorophenol (C)




17.267min (-0.004) 45106.98ng

response 29545

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	52.05
264.00	62.60	62.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG110116\
Data File : BG024608.D
Acq On : 2 Nov 2016 1:35
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:15:58 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

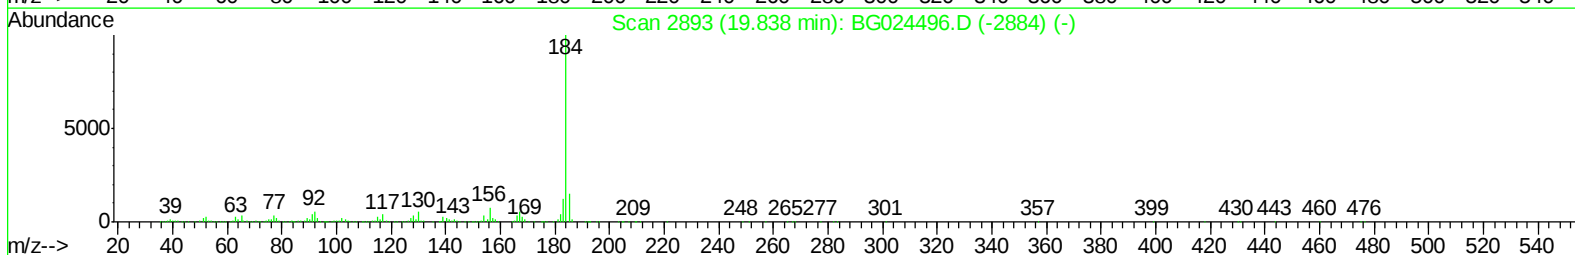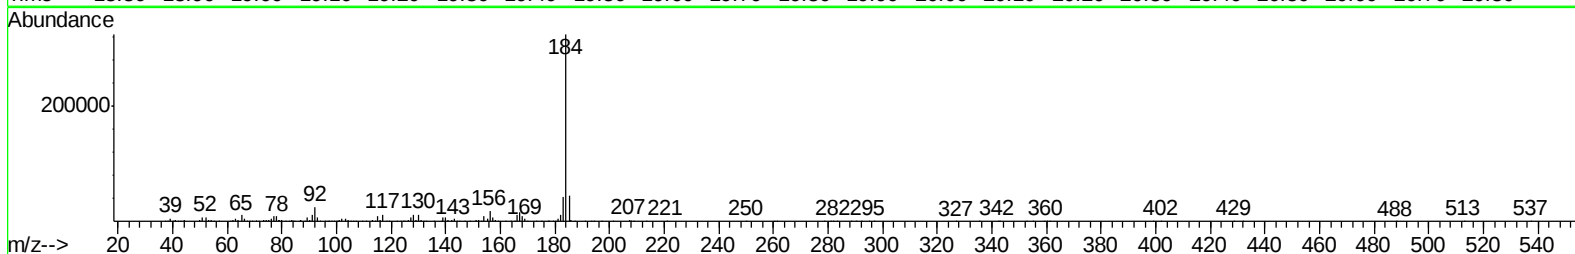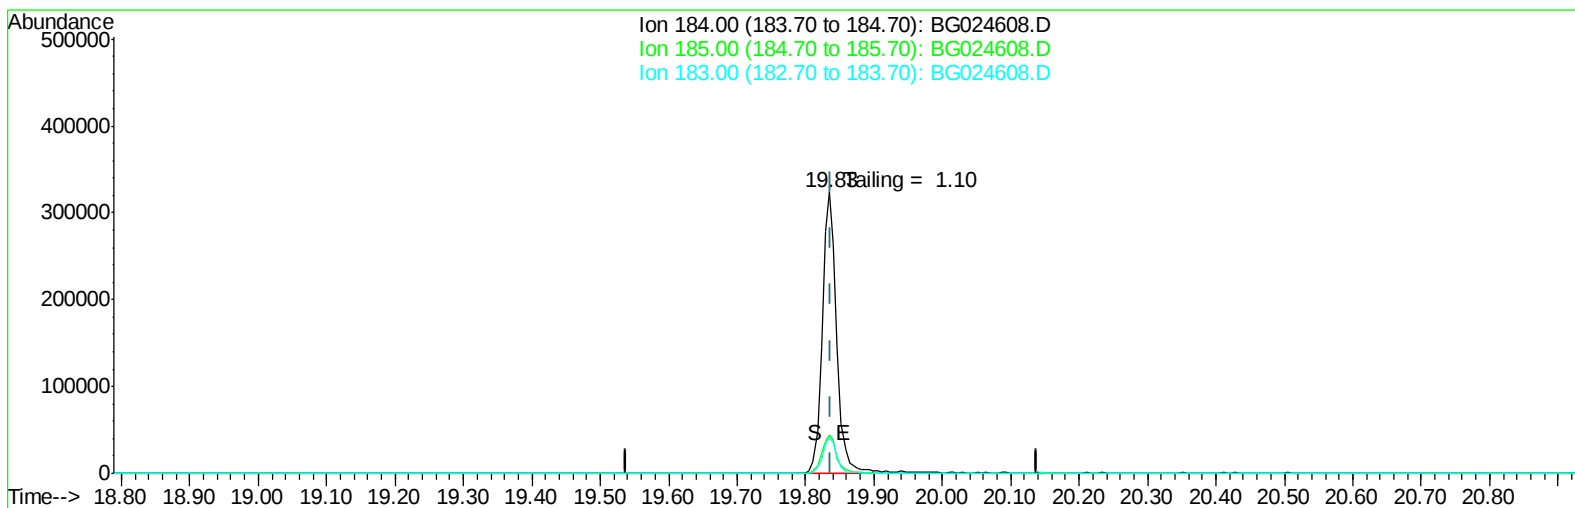

TIC: BG024608.D

(76) Benzidine

19.835min (-0.004) 107703.45ng

response 479610

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.85
183.00	13.80	12.87
0.00	0.00	0.00