

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110116\
 Data File : BG024617.D
 Acq On : 2 Nov 2016 7:39
 Operator : UM/SJ
 Sample : H5489-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-69-11.5-12.0

Quant Time: Nov 02 08:18:26 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 11:14:13 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	124103	20.00	ng	0.00
21) Naphthalene-d8	11.09	136	497145	20.00	ng	0.00
38) Acenaphthene-d10	14.88	164	387655	20.00	ng	0.00
63) Phenanthrene-d10	17.62	188	811427	20.00	ng	0.00
75) Chrysene-d12	21.92	240	1082304	20.00	ng	-0.01
86) Perylene-d12	25.35	264	1110925	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.80	112	794339	104.91	ng	0.00
7) Phenol-d6	7.40	99	1114023	107.26	ng	0.00
23) Nitrobenzene-d5	9.44	82	775702	71.04	ng	0.00
41) 2,4,6-Tribromophenol	16.36	330	580237	100.19	ng	0.00
44) 2-Fluorobiphenyl	13.51	172	1648683	70.69	ng	0.00
78) Terphenyl-d14	20.20	244	2600933	71.81	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	14.32	163	531809	19.32	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110116\
Data File : BG024617.D
Acq On : 2 Nov 2016 7:39
Operator : UM/SJ
Sample : H5489-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-69-11.5-12.0

Quant Time: Nov 02 08:18:26 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

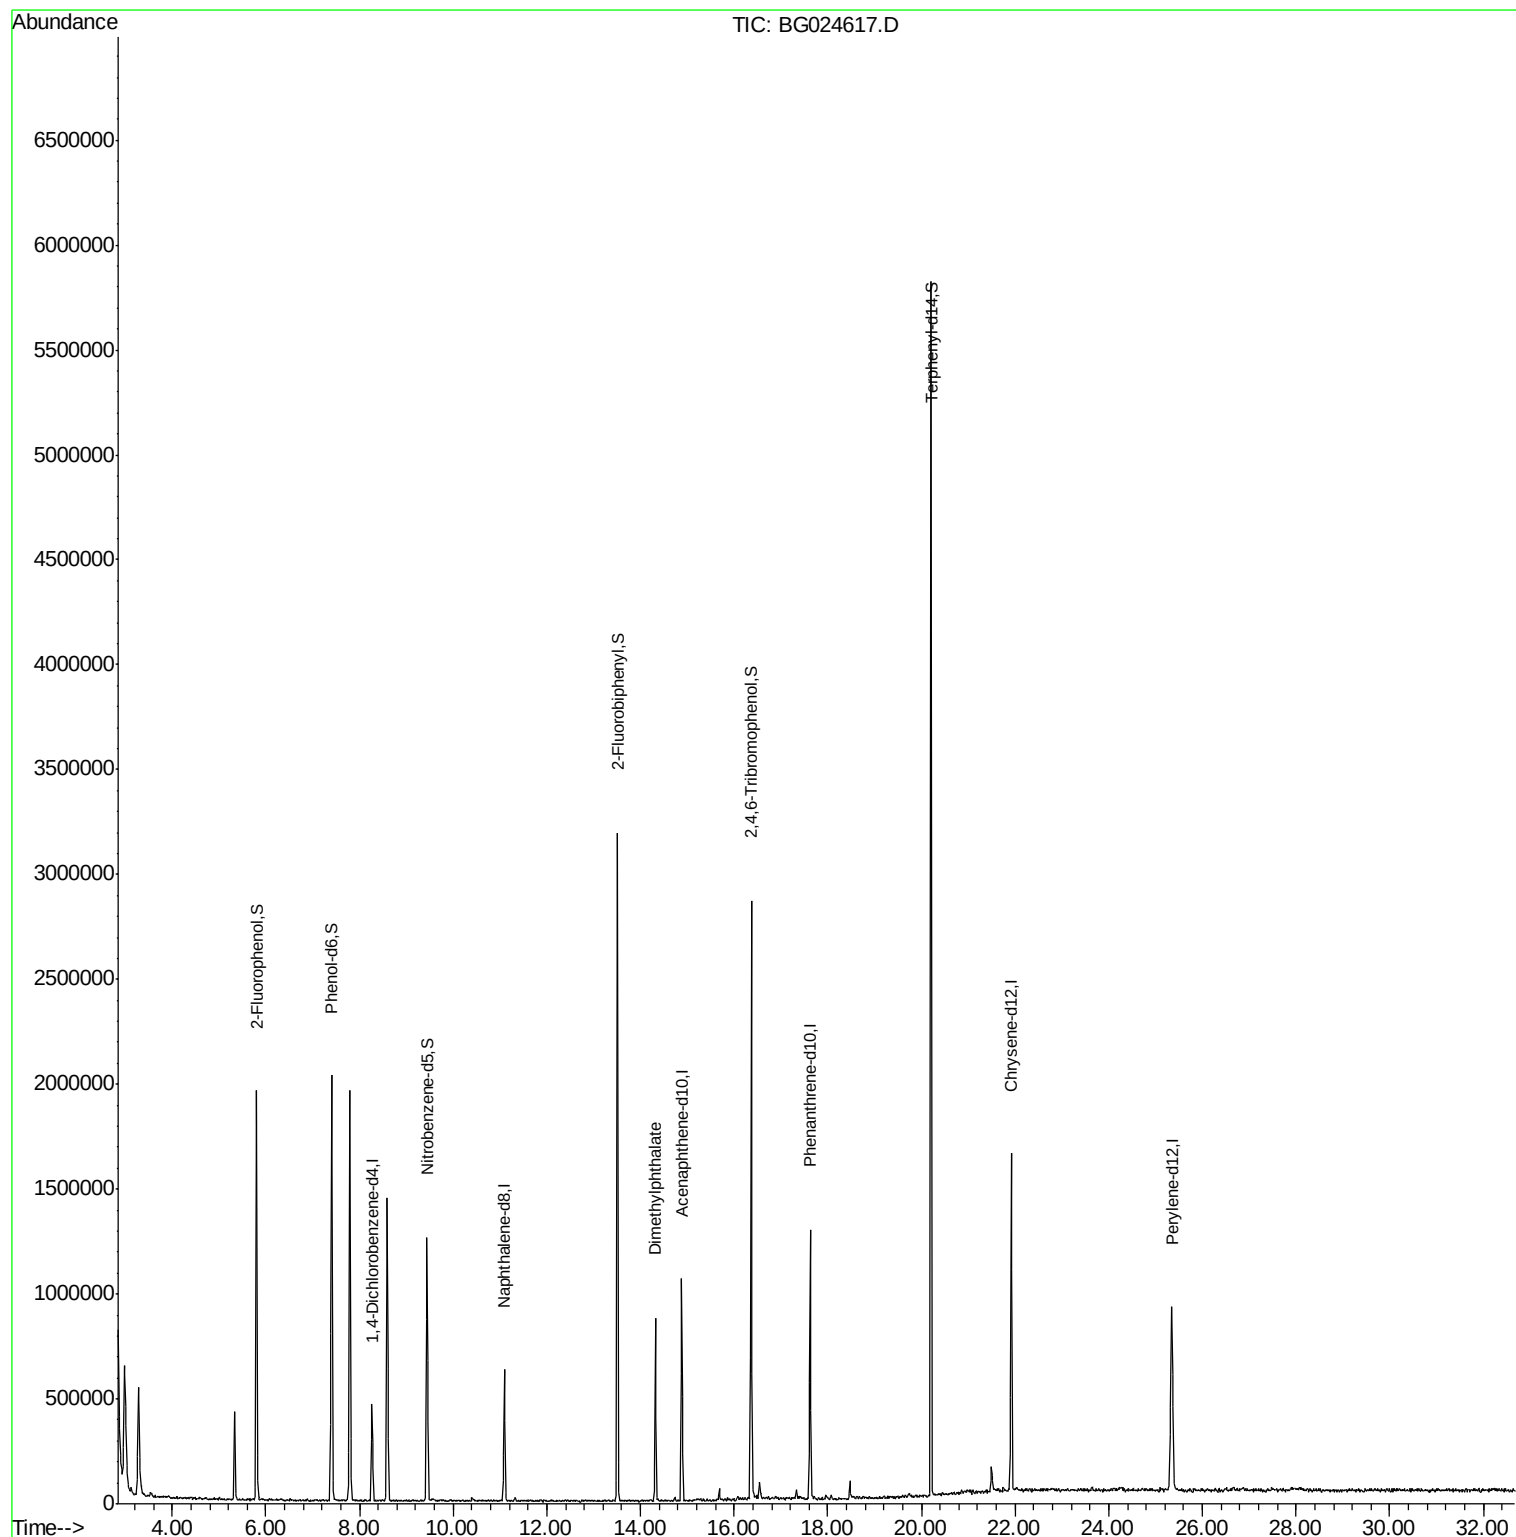



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.27 min Scan# 924

Delta R.T. -0.00 min

Lab File: BG024617.D

Acq: 2 Nov 2016 7:39

Instrument :

BNA_G

ClientSampleId :

SB-69-11.5-12.0


Tot Ion:152 Resp: 124103

Ion Ratio Lower Upper

152 100

150 155.9 114.0 171.0




115 60.5 48.1 72.1

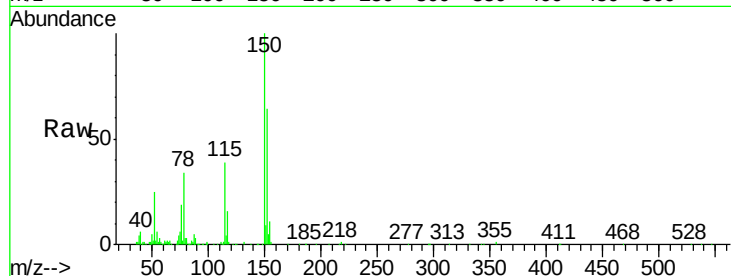

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

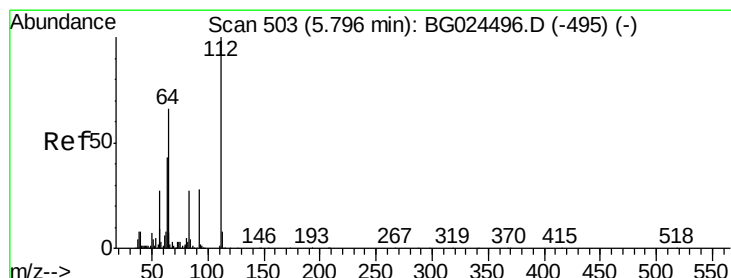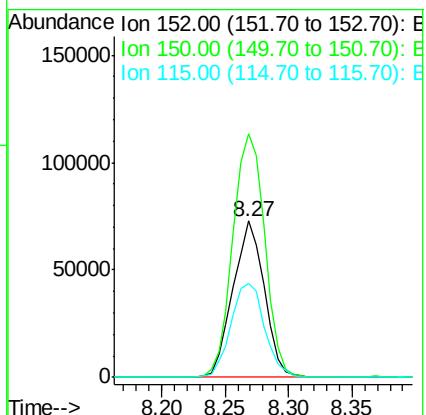

#5

2-Fluorophenol

Concen: 104.91 ng

RT: 5.80 min Scan# 504

Delta R.T. 0.00 min

Lab File: BG024617.D

Acq: 2 Nov 2016 7:39


Tgt Ion:112 Resp: 794339

Ion Ratio Lower Upper

112 100

64 74.3 61.8 92.6



63 42.2 37.2 55.8

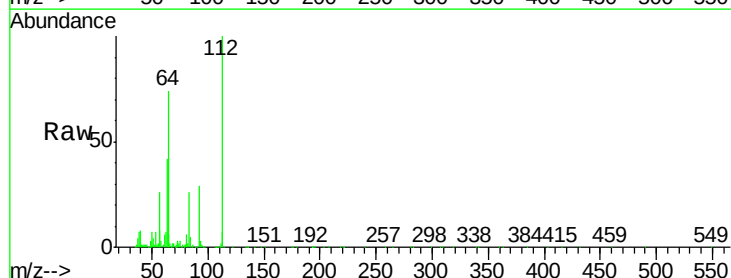


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

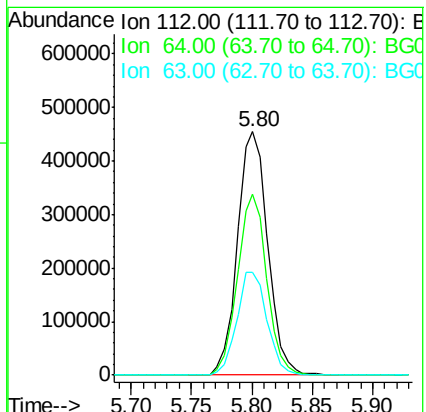

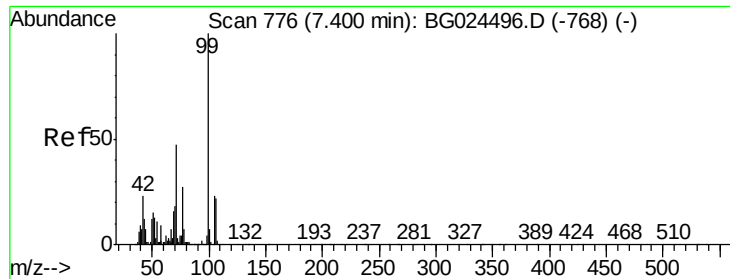

#7

Phenol-d6

Concen: 107.26 ng

RT: 7.40 min Scan# 777

Delta R.T. 0.00 min

Lab File: BG024617.D

Acq: 2 Nov 2016 7:39

Instrument :

BNA_G

ClientSampleId :

SB-69-11.5-12.0


Tot Ion: 99 Resp: 1114023

Ion Ratio Lower Upper




99 100

42 22.0 20.5 30.7

71 45.5 37.6 56.4

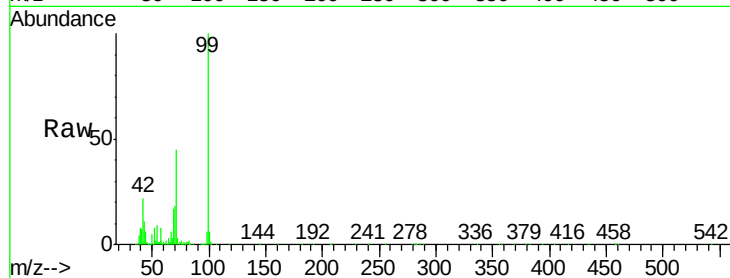

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

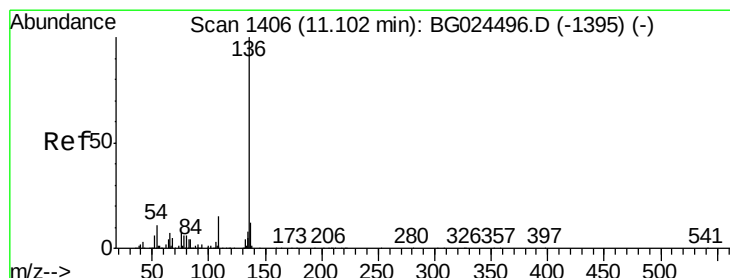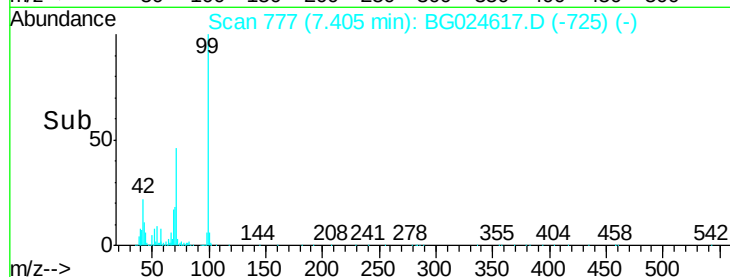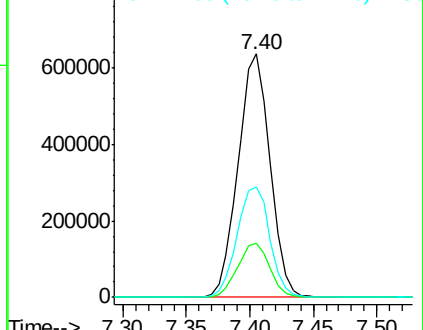

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.09 min Scan# 1405

Delta R.T. -0.01 min

Lab File: BG024617.D

Acq: 2 Nov 2016 7:39

Tgt Ion: 136 Resp: 497145


Ion Ratio Lower Upper

136 100



137 11.5 8.9 13.3


54 10.5 9.3 13.9

68 5.3 5.1 7.7

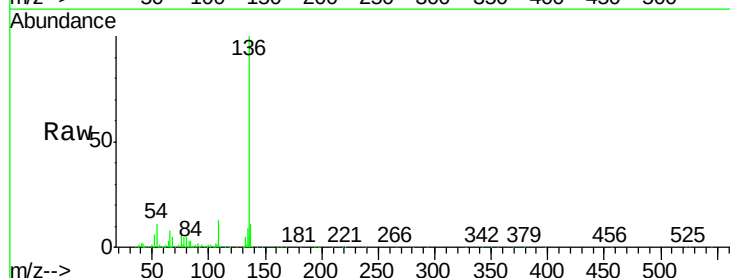

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



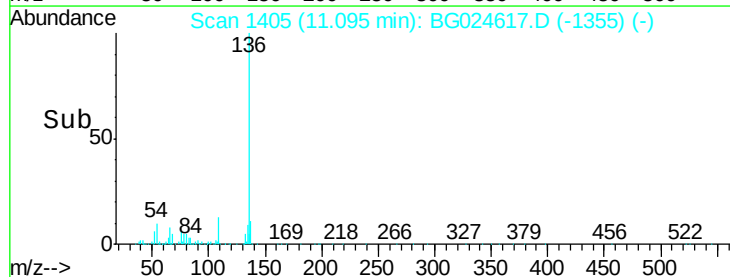
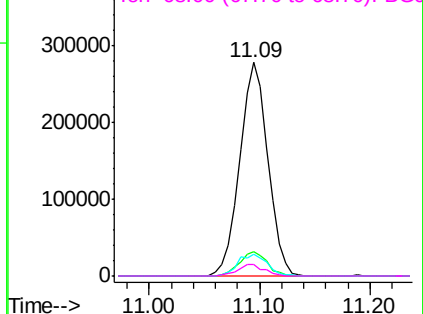


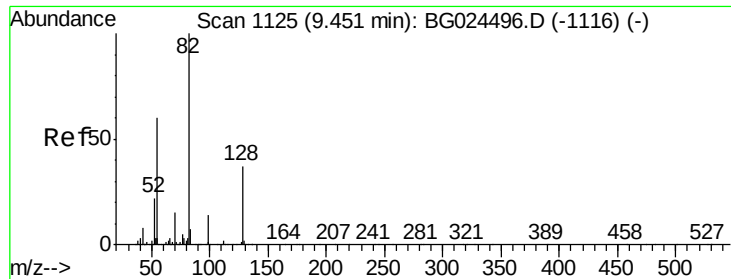

#23
 Nitrobenzene-d5
 Concen: 71.04 ng
 RT: 9.44 min Scan# 1124
 Delta R.T. -0.01 min
 Lab File: BG024617.D
 Acq: 2 Nov 2016 7:39




Instrument :
 BNA_G
 ClientSampleId :
 SB-69-11.5-12.0


Tot Ion	82	Resp	775702
Ion Ratio	Lower	Upper	
82	100		
128	35.4	26.4	39.6
54	56.9	49.4	74.2

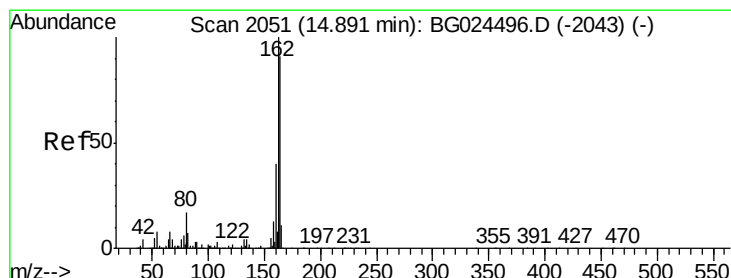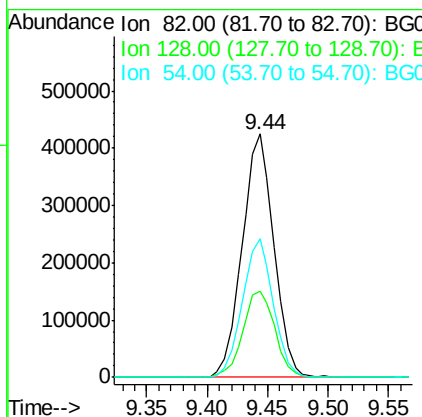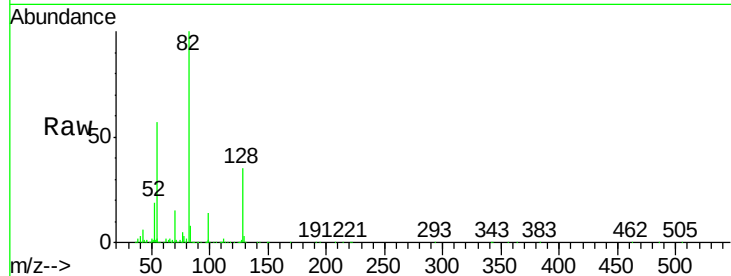

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.88 min Scan# 2050
 Delta R.T. -0.01 min
 Lab File: BG024617.D
 Acq: 2 Nov 2016 7:39

Tgt Ion	164	Resp	387655
Ion Ratio	Lower	Upper	
164	100		
162	101.2	85.1	127.7
160	46.4	34.7	52.1

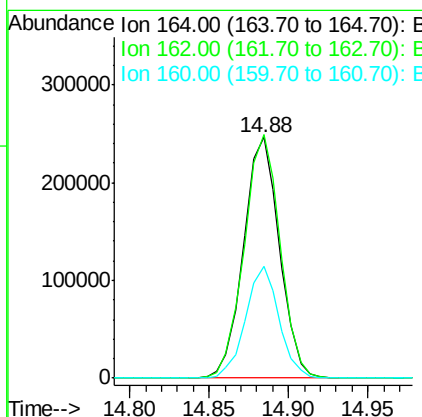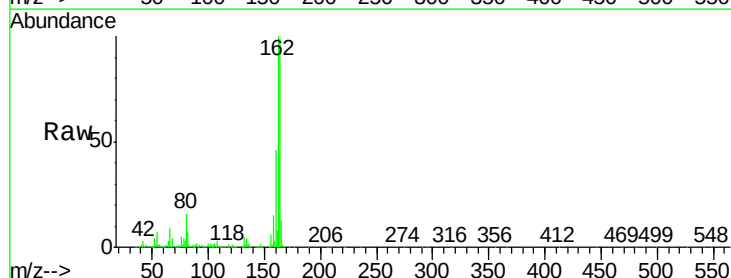




#41
2,4,6-Tribromophenol
Concen: 100.19 ng
RT: 16.36 min Scan# 2302
Delta R.T. -0.01 min
Lab File: BG024617.D
Acq: 2 Nov 2016 7:39

Instrument :
BNA_G
ClientSampleId :
SB-69-11.5-12.0

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.3	77.3	115.9
141	32.1	32.1	48.1



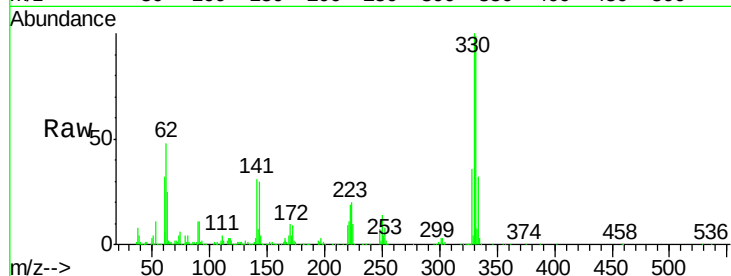


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

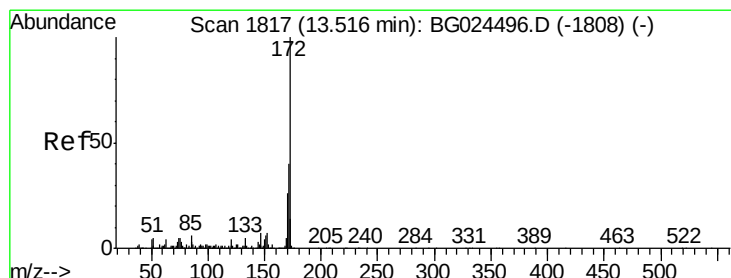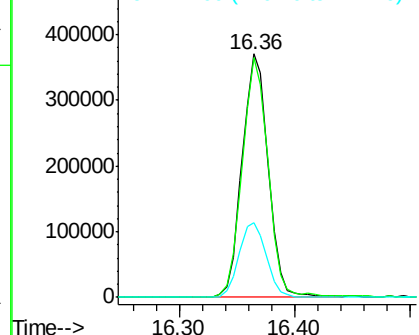

#44
2-Fluorobiphenyl
Concen: 70.69 ng
RT: 13.51 min Scan# 1816
Delta R.T. -0.01 min
Lab File: BG024617.D
Acq: 2 Nov 2016 7:39

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.3	32.2	48.2
170	25.9	21.8	32.6


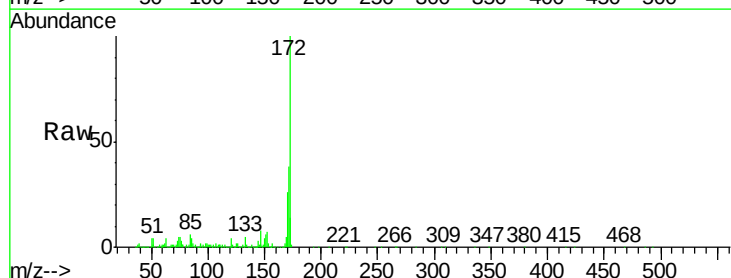



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

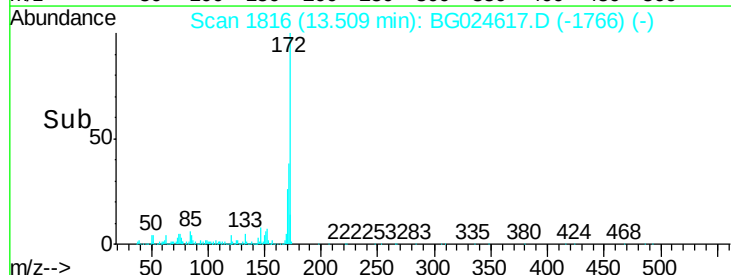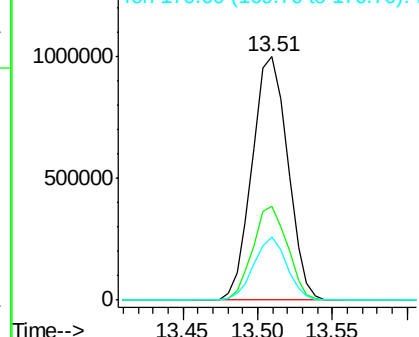

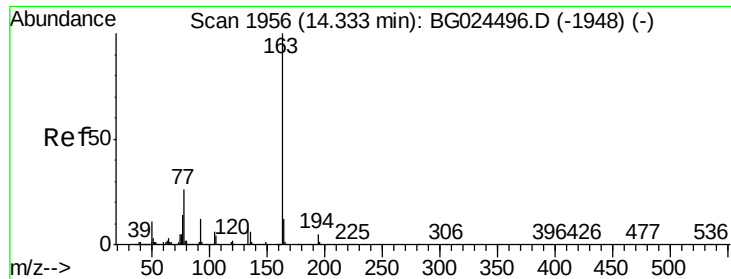

#49

Dimethylphthalate

Concen: 19.32 ng

RT: 14.32 min Scan# 1954

Delta R.T. -0.01 min

Lab File: BG024617.D

Acq: 2 Nov 2016 7:39

Instrument :

BNA_G

ClientSampleId :

SB-69-11.5-12.0


Tot Ion:163 Resp: 531809

Ion Ratio Lower Upper

163 100

194 4.1 3.8 5.6




164 11.5 9.3 13.9

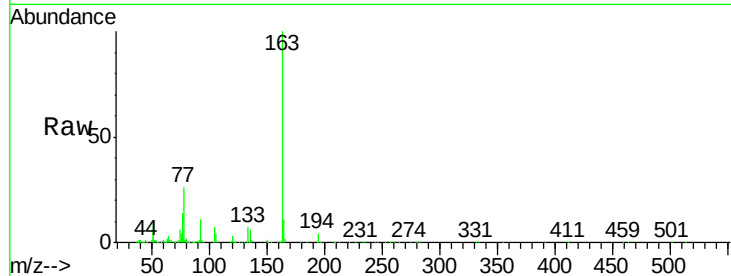

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

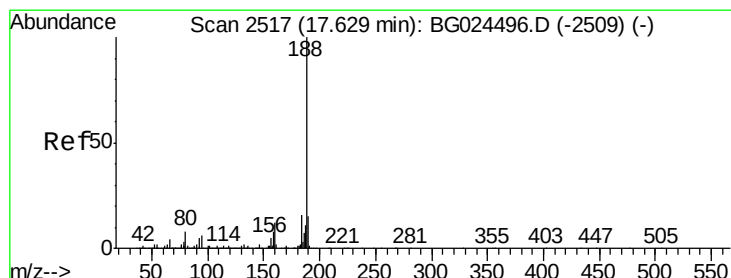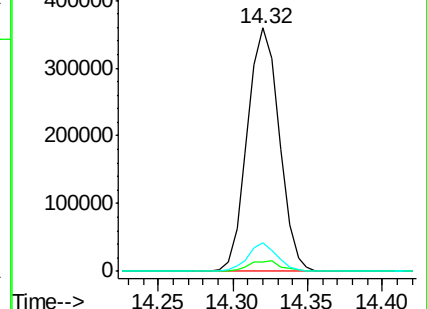

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.62 min Scan# 2516

Delta R.T. -0.01 min

Lab File: BG024617.D

Acq: 2 Nov 2016 7:39


Tgt Ion:188 Resp: 811427

Ion Ratio Lower Upper

188 100

94 6.1 5.8 8.8



80 8.2 7.5 11.3

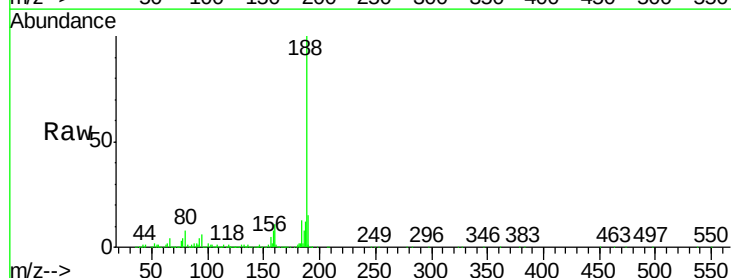


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



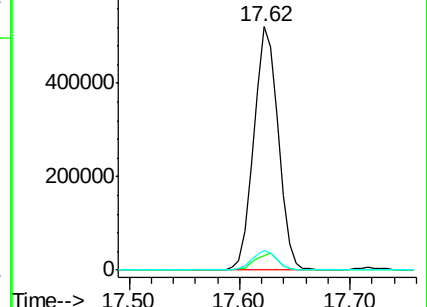



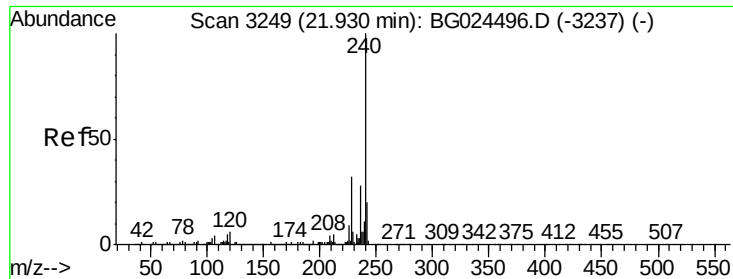

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 21.92 min Scan# 3247
 Delta R.T. -0.01 min
 Lab File: BG024617.D
 Acq: 2 Nov 2016 7:39




Instrument :
 BNA_G
 ClientSampleId :
 SB-69-11.5-12.0


Tot Ion:240 Resp: 1082304
 Ion Ratio Lower Upper
 240 100
 120 5.7 5.7 8.5
 236 27.5 22.2 33.4

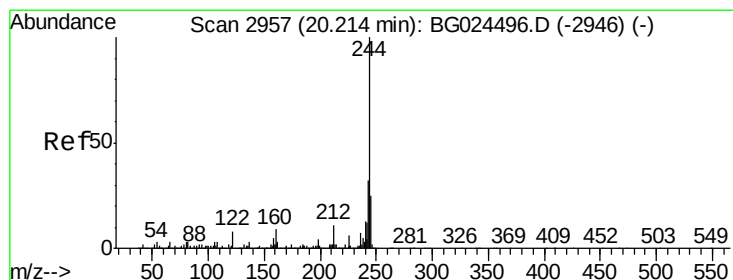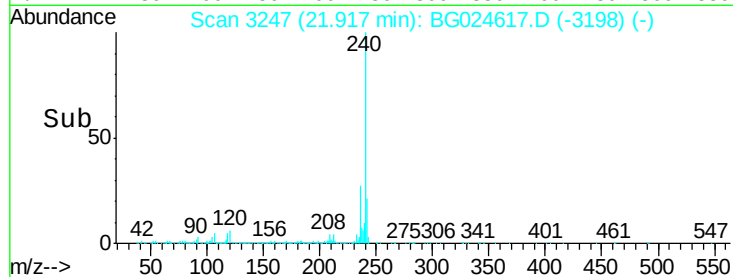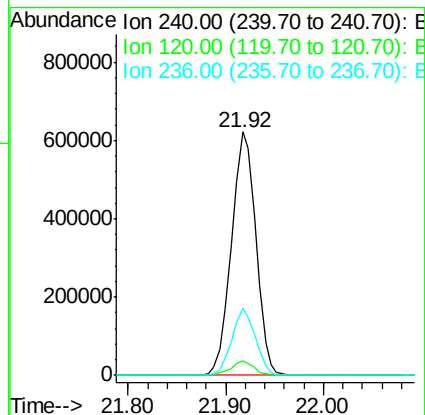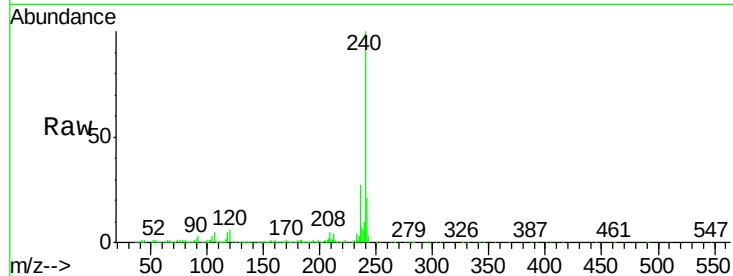

#78
 Terphenyl-d14
 Concen: 71.81 ng
 RT: 20.20 min Scan# 2955
 Delta R.T. -0.01 min
 Lab File: BG024617.D
 Acq: 2 Nov 2016 7:39

Tgt Ion:244 Resp: 2600933
 Ion Ratio Lower Upper
 244 100
 212 10.2 10.0 15.0
 122 7.8 8.6 12.8#

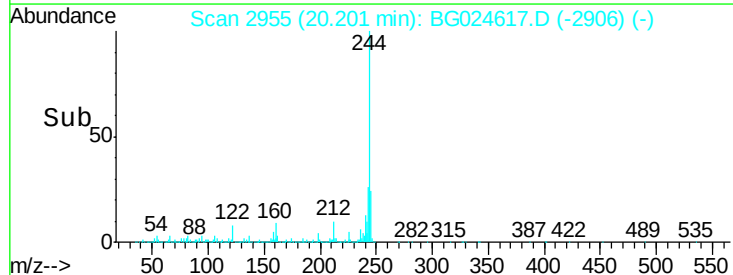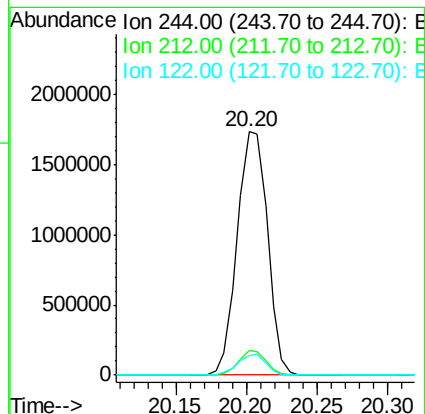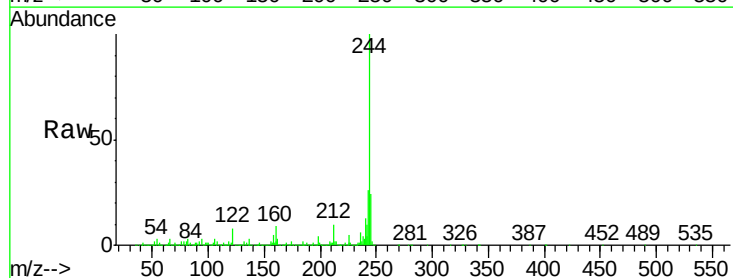



#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 25.35 min Scan# 3831
 Delta R.T. -0.02 min
 Lab File: BG024617.D
 Acq: 2 Nov 2016 7:39

Instrument :
 BNA_G
 ClientSampleId :
 SB-69-11.5-12.0

Tot Ion:264 Resp: 1110925
 Ion Ratio Lower Upper
 264 100
 260 23.2 21.8 32.8
 265 21.0 18.2 27.4

