
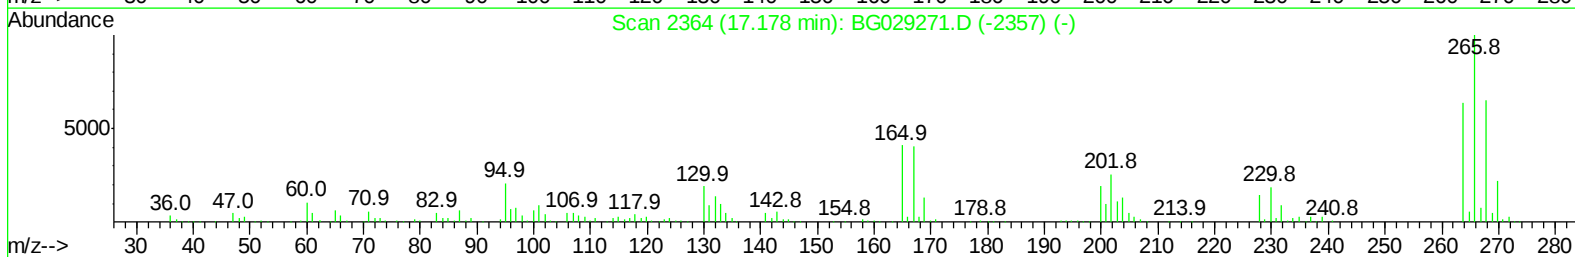
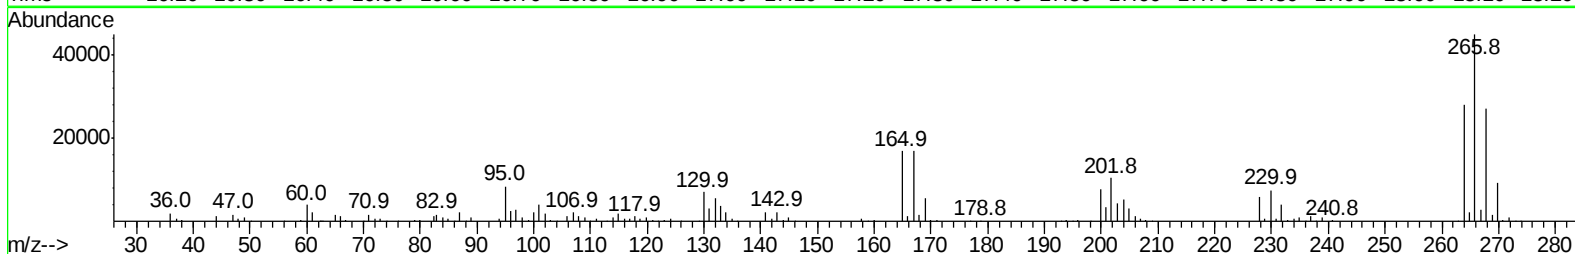


Data Path : Z:\HPCHEM1\BNA G\DATA\BG110117\
Data File : BG030625.D
Acq On : 1 Nov 2017 8:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:09:13 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

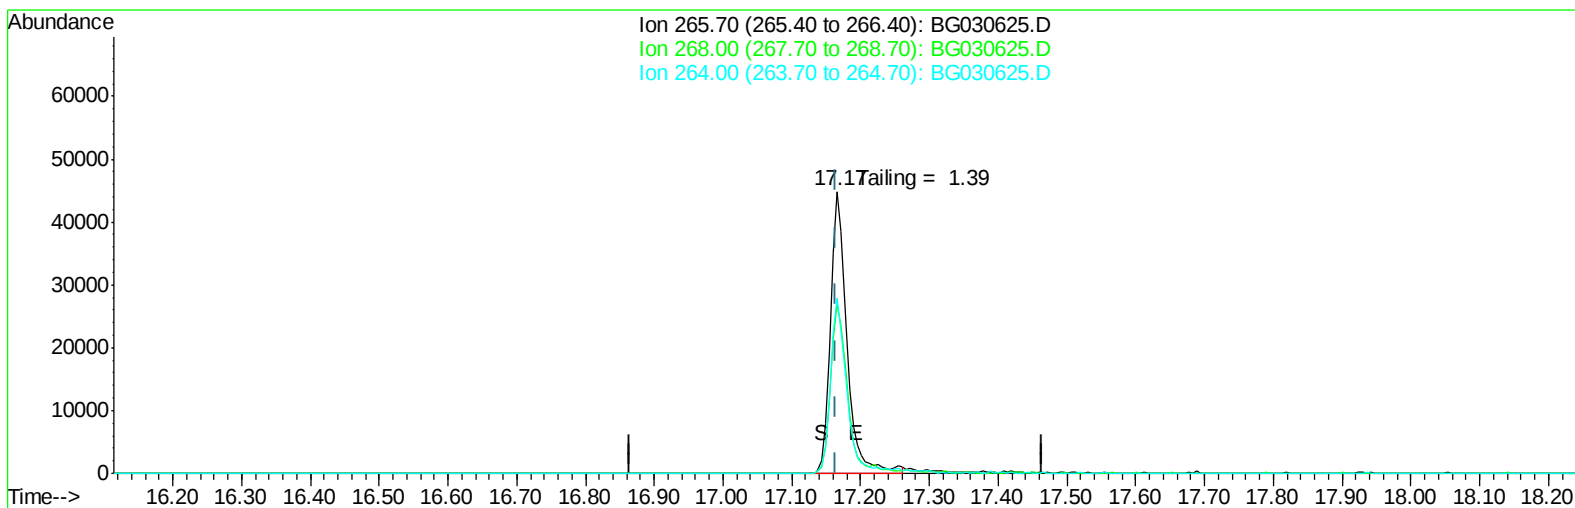

TIC: BG030625.D

(69) Pentachlorophenol (C)




17.166min (+0.001) 59221.71ng

response 73403

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.15
264.00	62.00	62.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG110117\
Data File : BG030625.D
Acq On : 1 Nov 2017 8:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 07:09:13 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

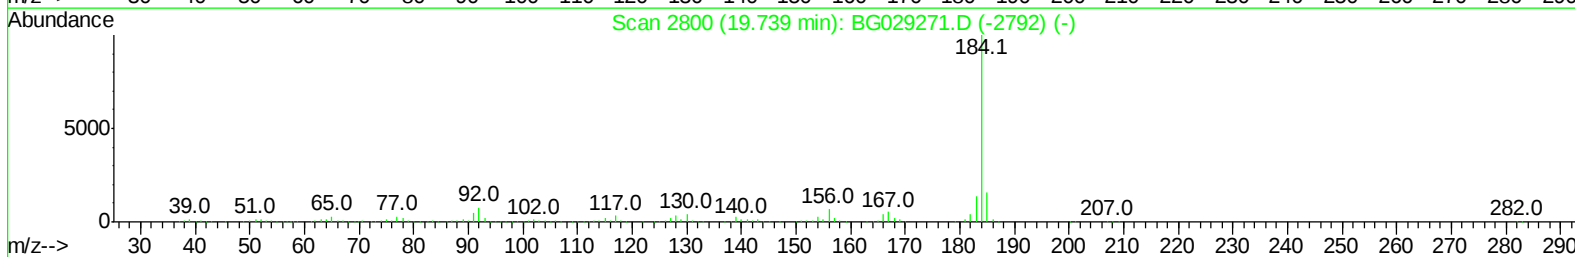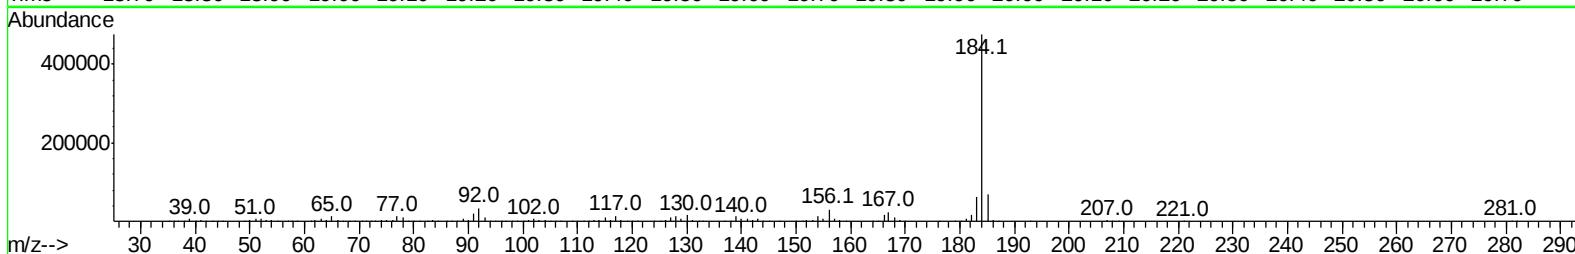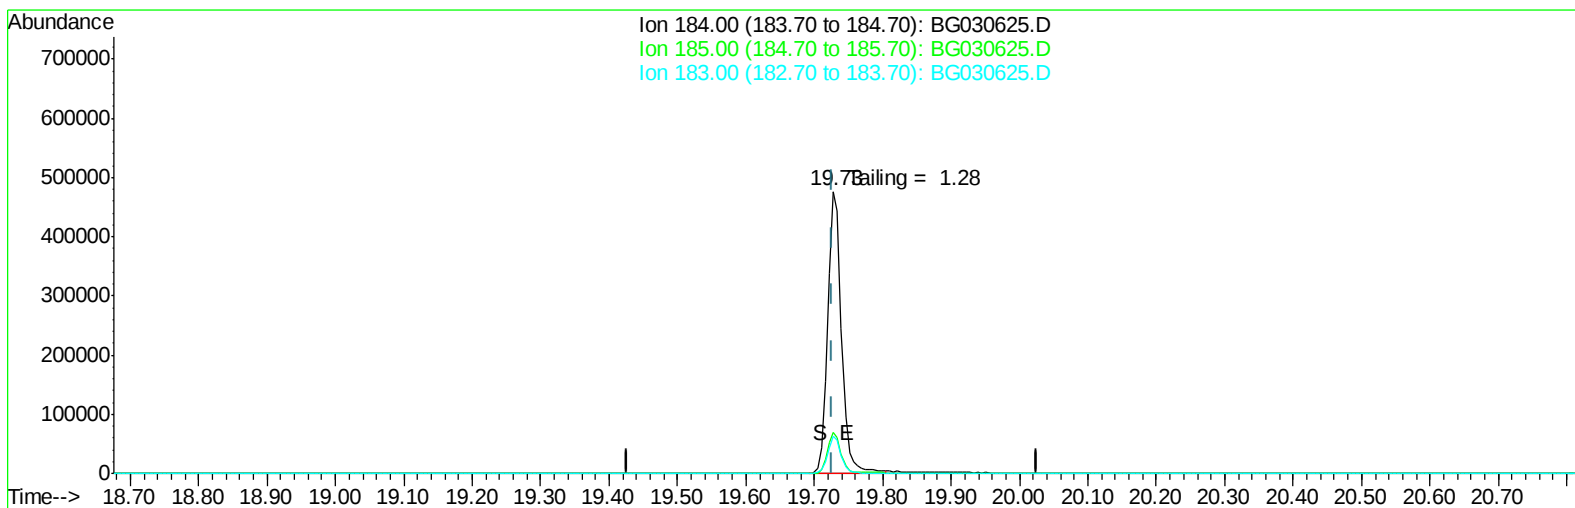

TIC: BG030625.D

(76) Benzidine

19.728min (+0.001) 334673.58ng

response 677035

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.52
183.00	13.30	12.97
0.00	0.00	0.00