

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110117\
 Data File : BG030653.D
 Acq On : 2 Nov 2017 3:01
 Operator : SJ/JU
 Sample : I6205-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 102517-TIDO-F-U-B

Quant Time: Nov 02 06:02:46 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 01 17:41:24 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	71695	20.00	ng	0.00
21) Naphthalene-d8	10.97	136	329667	20.00	ng	0.00
38) Acenaphthene-d10	14.78	164	228830	20.00	ng	0.00
63) Phenanthrene-d10	17.51	188	519165	20.00	ng	0.00
75) Chrysene-d12	21.79	240	558956	20.00	ng	0.00
86) Perylene-d12	25.09	264	561407	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	206878	48.20	ng	0.00
7) Phenol-d6	7.31	99	180192	29.91	ng	0.00
23) Nitrobenzene-d5	9.32	82	541753	104.43	ng	0.00
41) 2,4,6-Tribromophenol	16.26	330	296584	100.39	ng	0.00
44) 2-Fluorobiphenyl	13.40	172	1502139	96.28	ng	0.00
78) Terphenyl-d14	20.11	244	2277189	92.68	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110117\
Data File : BG030653.D
Acq On : 2 Nov 2017 3:01
Operator : SJ/JU
Sample : I6205-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B

Quant Time: Nov 02 06:02:46 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 01 17:41:24 2017
Response via : Initial Calibration

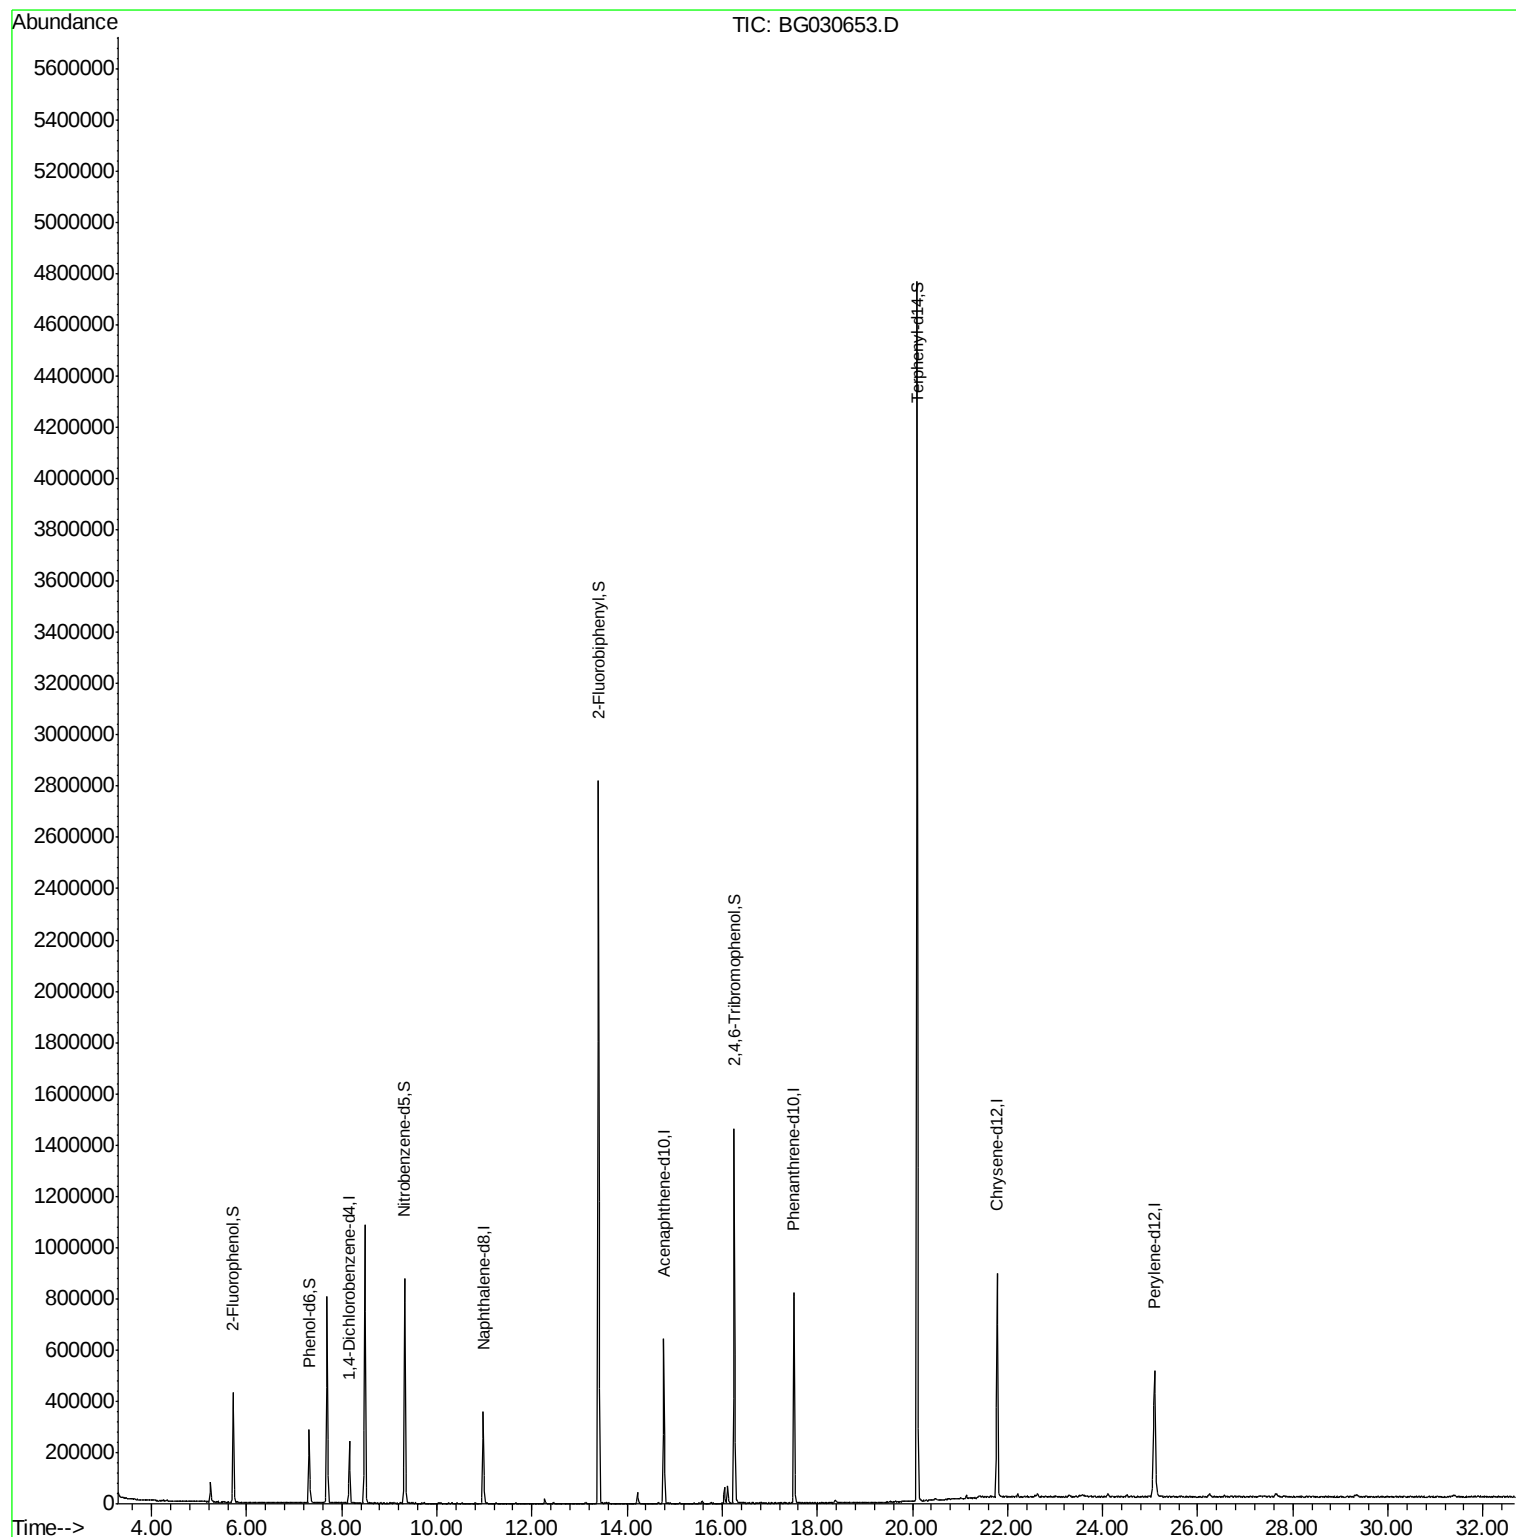

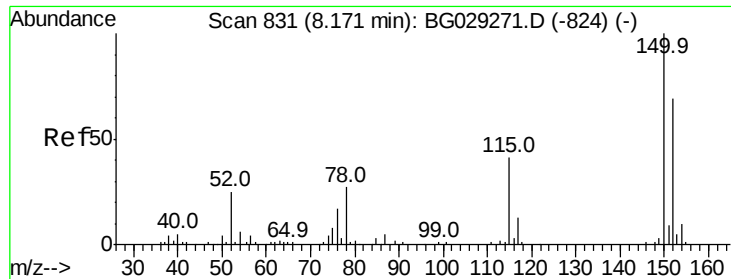


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 829
Delta R.T. 0.00 min
Lab File: BG030653.D
Acq: 2 Nov 2017 3:01

Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B

Tot Ion:152 Resp: 71695
Ion Ratio Lower Upper
152 100
150 150.8 126.6 189.8
115 56.9 53.0 79.4

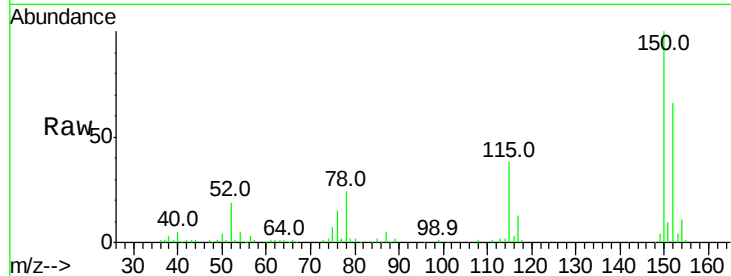


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

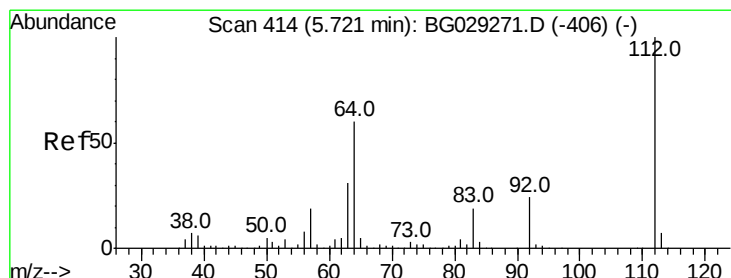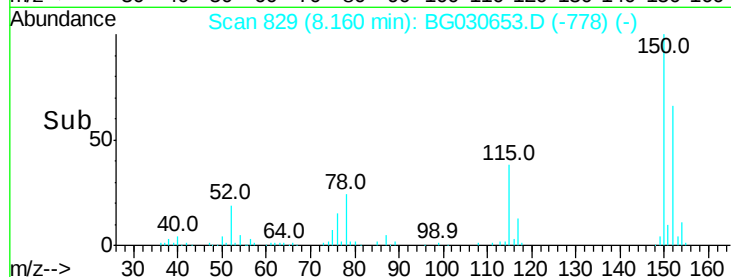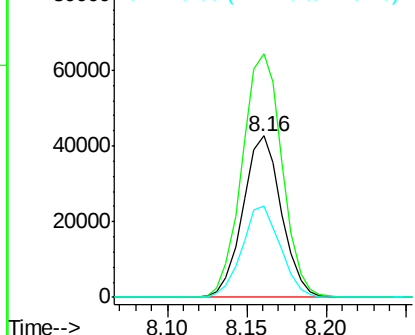



#5


2-Fluorophenol
Concen: 48.204 ng
RT: 5.72 min Scan# 413
Delta R.T. 0.00 min
Lab File: BG030653.D
Acq: 2 Nov 2017 3:01

Tgt Ion:112 Resp: 206878
Ion Ratio Lower Upper
112 100
64 56.8 56.3 84.5
63 29.9 30.1 45.1#

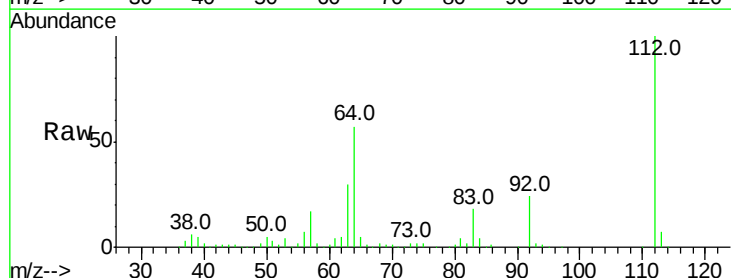

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

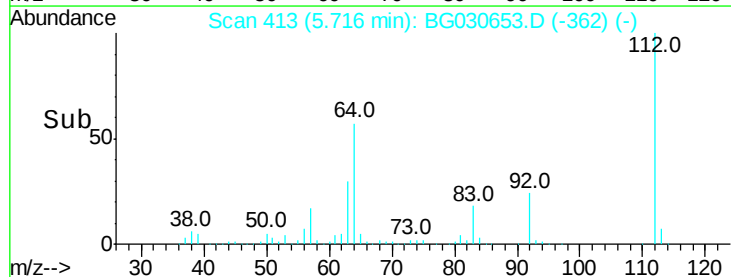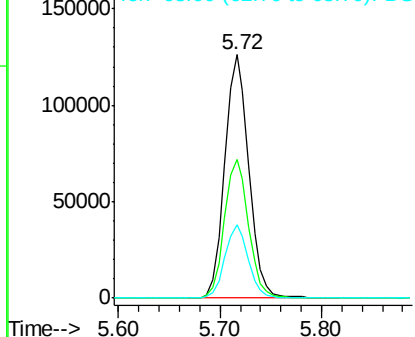

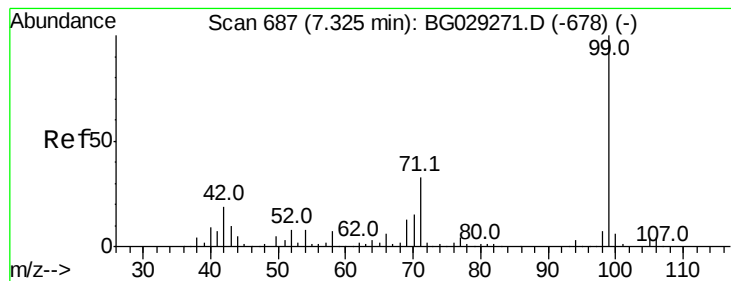

#7

Phenol-d6

Concen: 29.912 ng

RT: 7.31 min Scan# 685

Delta R.T. -0.00 min

Lab File: BG030653.D

Acq: 2 Nov 2017 3:01

Instrument :

BNA_G

ClientSampleId :

102517-TIDO-F-U-B


Tot Ion: 99 Resp: 180192

Ion Ratio Lower Upper




99 100

42 18.3 14.1 21.1

71 31.7 26.1 39.1

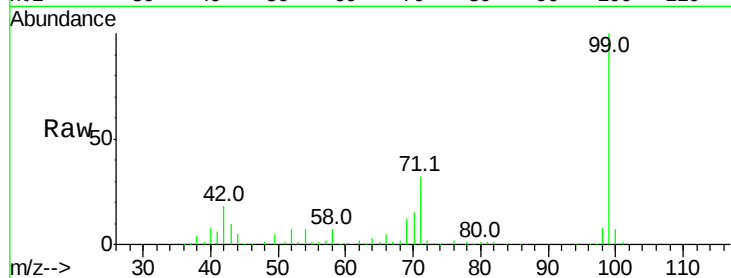

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

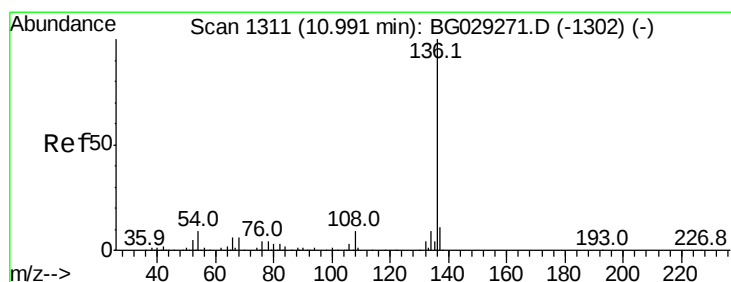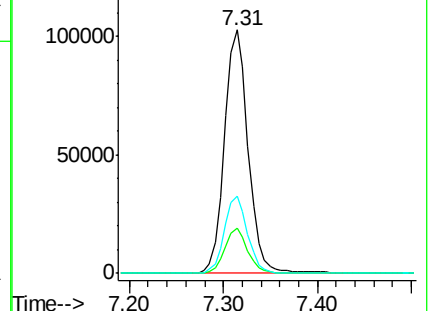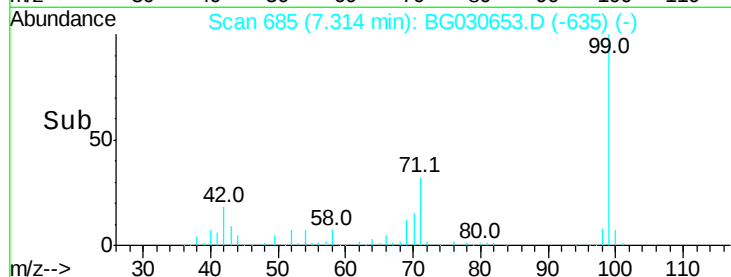

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.97 min Scan# 1308

Delta R.T. 0.00 min

Lab File: BG030653.D

Acq: 2 Nov 2017 3:01

Tgt Ion: 136 Resp: 329667


Ion Ratio Lower Upper

136 100



137 11.2 9.2 13.8


54 7.7 10.3 15.5#

68 6.3 4.5 6.7

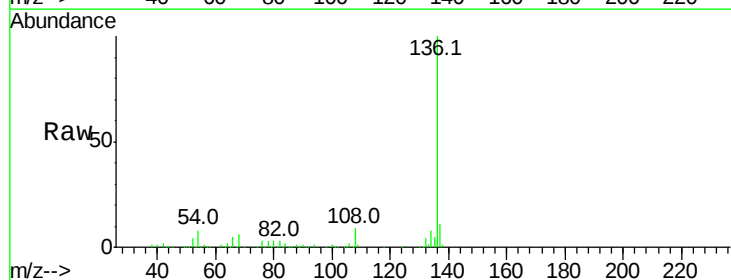

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



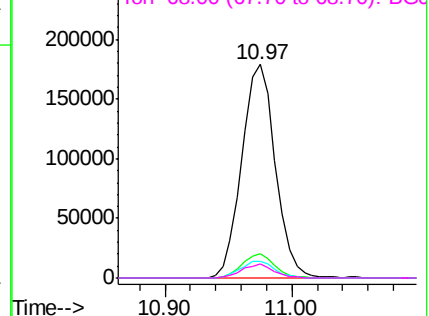
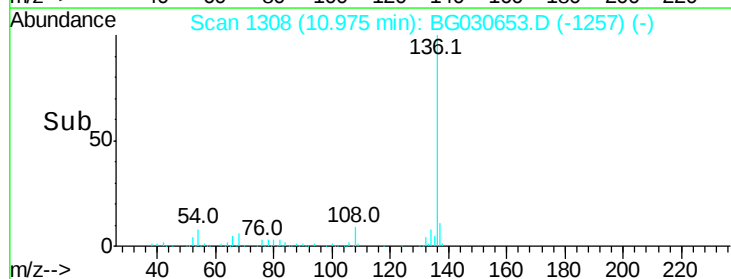


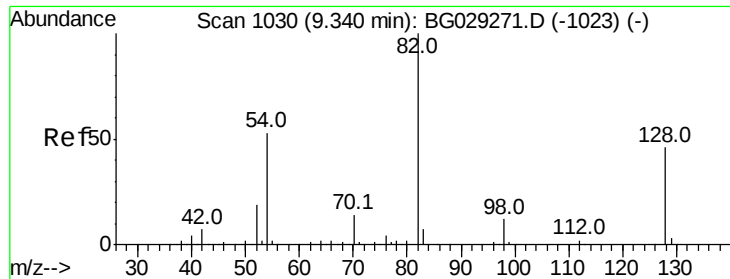

#23
Nitrobenzene-d5
Concen: 104.429 ng
RT: 9.32 min Scan# 1027
Delta R.T. -0.00 min
Lab File: BG030653.D
Acq: 2 Nov 2017 3:01




Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B


Tot Ion: 82 Resp: 541753
Ion Ratio Lower Upper
82 100
128 46.5 29.7 44.5#
54 51.3 43.1 64.7

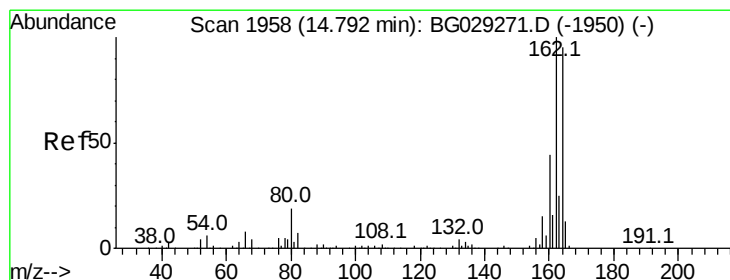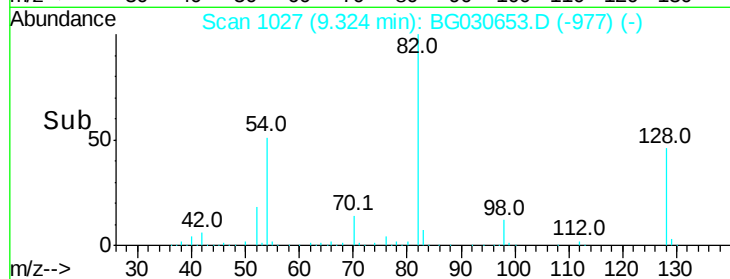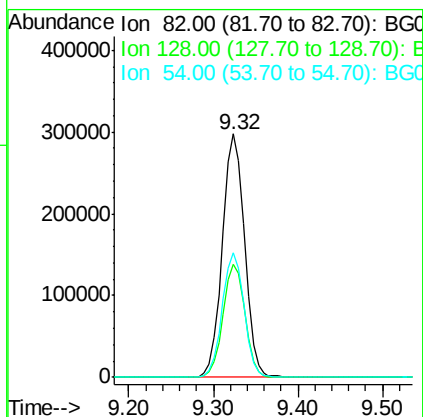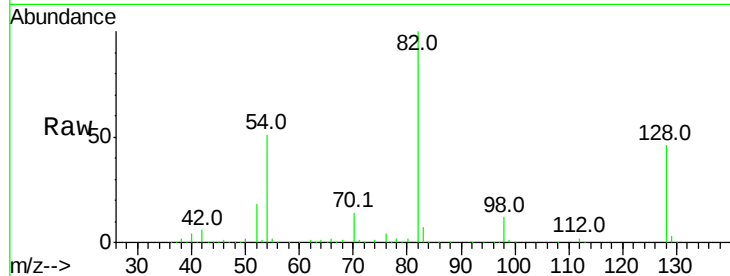

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.78 min Scan# 1955
Delta R.T. 0.00 min
Lab File: BG030653.D
Acq: 2 Nov 2017 3:01

Tgt Ion:164 Resp: 228830
Ion Ratio Lower Upper
164 100
162 103.7 78.8 118.2
160 44.3 35.4 53.0

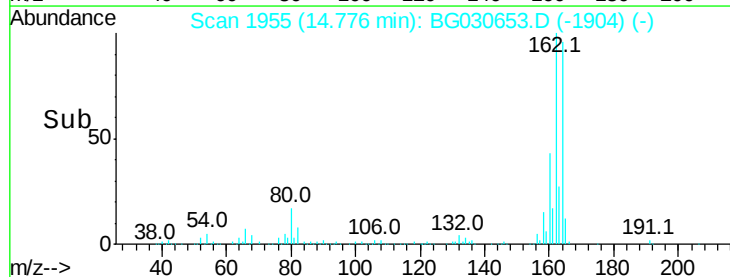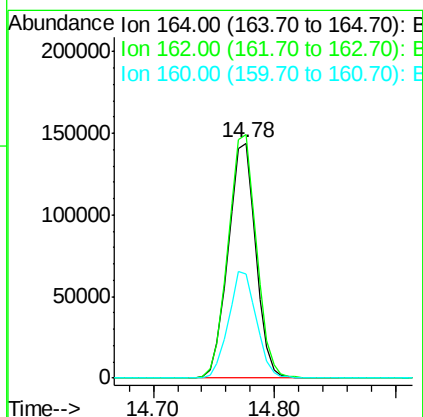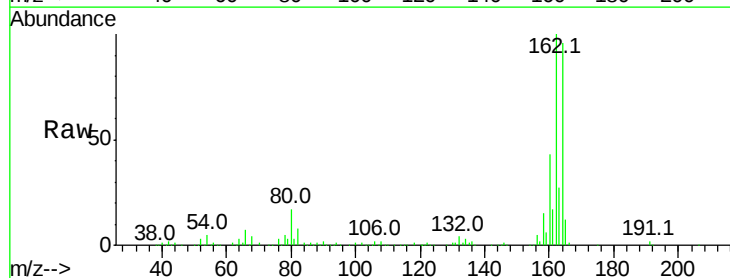


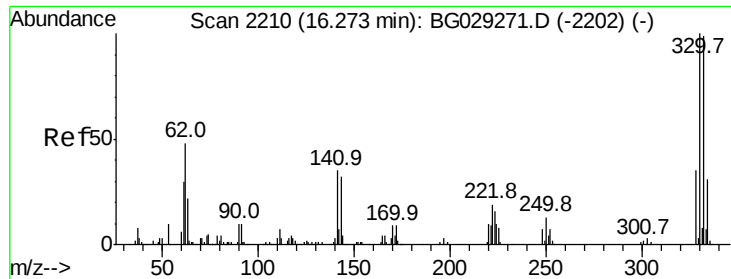




#41
 2,4,6-Tribromophenol
 Concen: 100.386 ng
 RT: 16.26 min Scan# 2207
 Delta R.T. -0.00 min
 Lab File: BG030653.D
 Acq: 2 Nov 2017 3:01

Instrument :
 BNA_G
 ClientSampleId :
 102517-TIDO-F-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.2	77.0	115.6
141	32.6	25.2	37.8

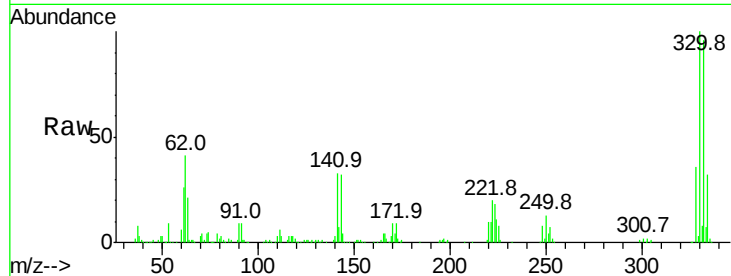


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

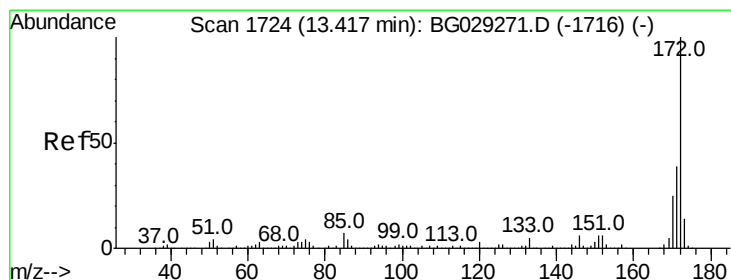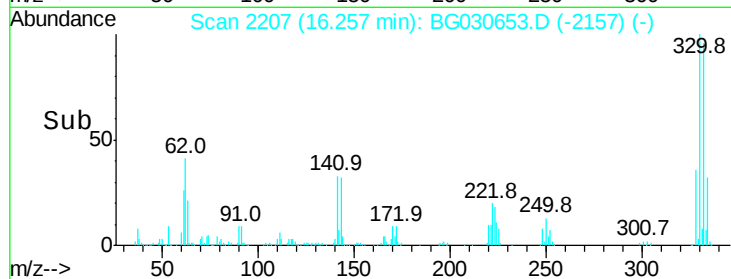
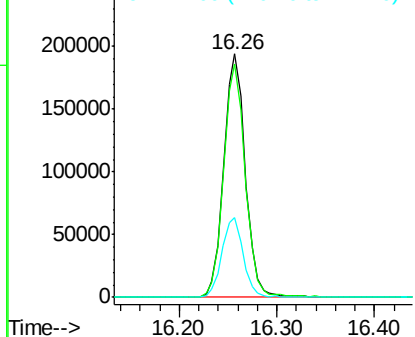



#44
 2-Fluorobiphenyl
 Concen: 96.278 ng
 RT: 13.40 min Scan# 1721
 Delta R.T. 0.00 min
 Lab File: BG030653.D
 Acq: 2 Nov 2017 3:01

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.1	30.0	45.0
170	25.7	19.5	29.3

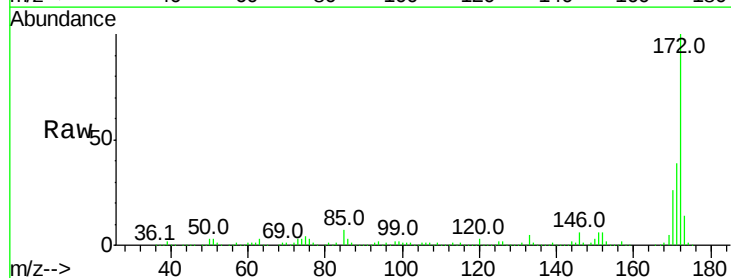

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

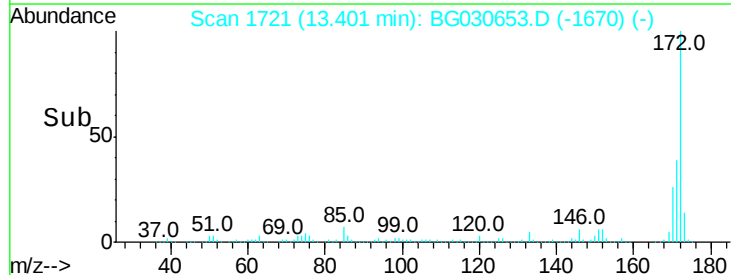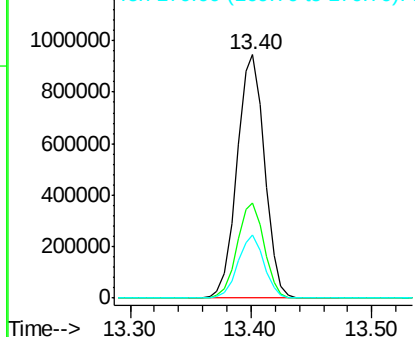


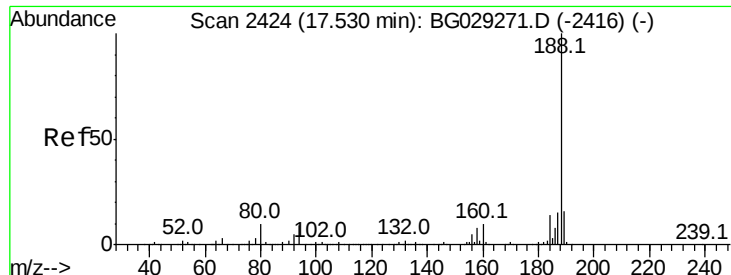




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.51 min Scan# 2420
Delta R.T. -0.00 min
Lab File: BG030653.D
Acq: 2 Nov 2017 3:01

Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B

Tot Ion:188 Resp: 519165
Ion Ratio Lower Upper
188 100
94 7.9 6.9 10.3
80 9.3 7.7 11.5

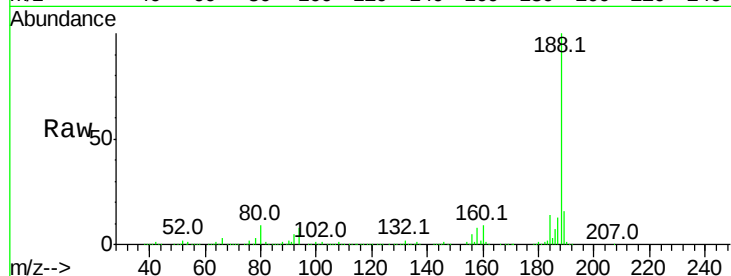


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

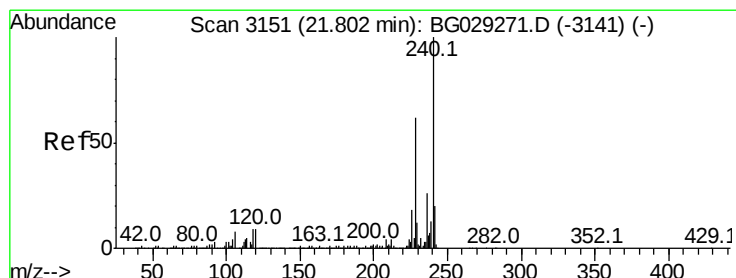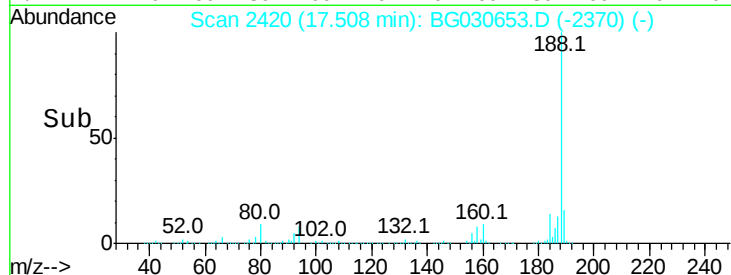
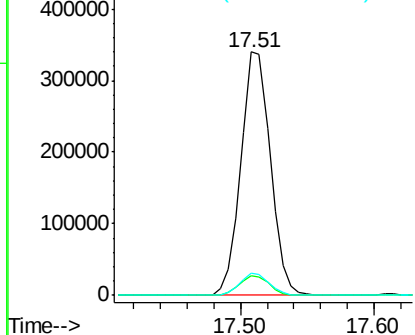



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.79 min Scan# 3148
Delta R.T. -0.00 min
Lab File: BG030653.D
Acq: 2 Nov 2017 3:01

Tgt Ion:240 Resp: 558956
Ion Ratio Lower Upper
240 100
120 8.5 6.8 10.2
236 26.3 20.9 31.3

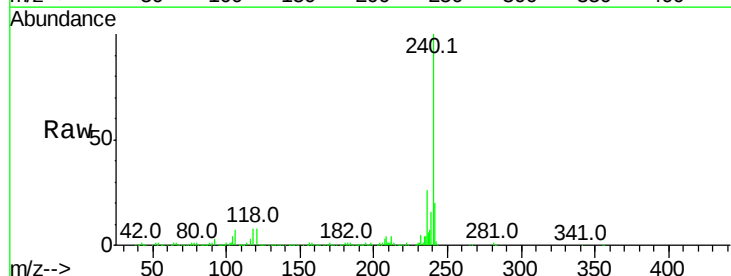

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

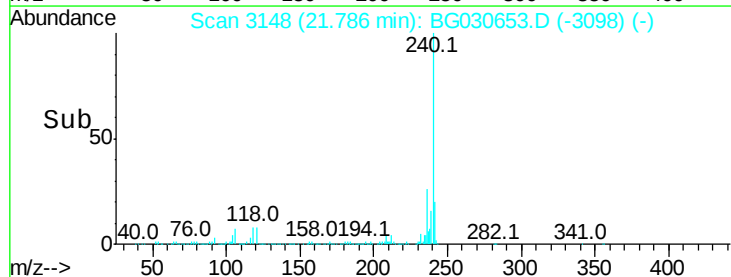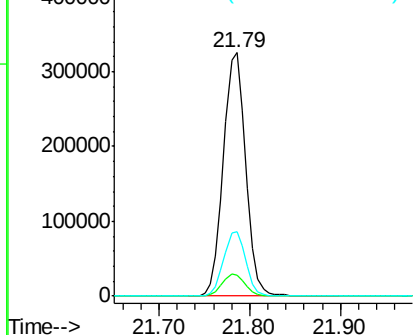

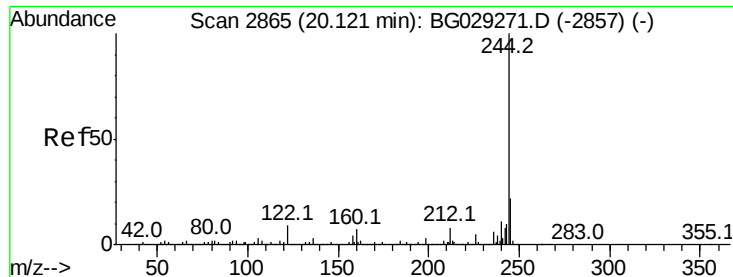

#78

Terphenyl-d14

Concen: 92.681 ng

RT: 20.11 min Scan# 2862

Delta R.T. 0.00 min

Lab File: BG030653.D

Acq: 2 Nov 2017 3:01

Instrument :


BNA_G

ClientSampleId :

102517-TIDO-F-U-B

Tot Ion:244 Resp: 2277189




Ion	Ratio	Lower	Upper
244	100		
212	8.5	5.8	8.8
122	10.3	7.0	10.4

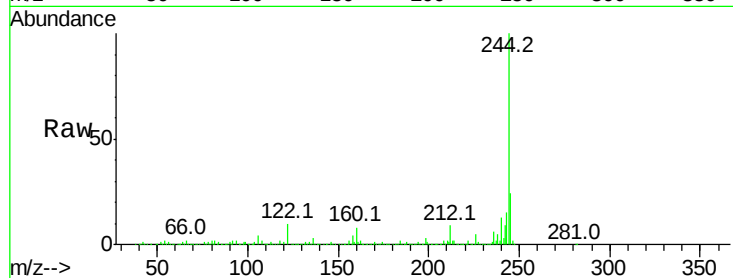

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

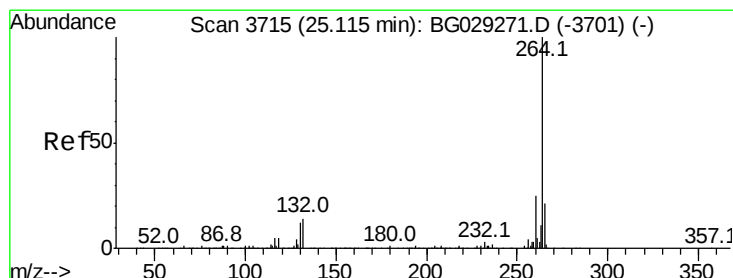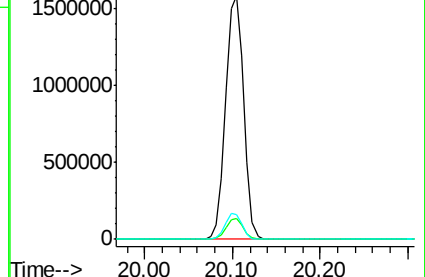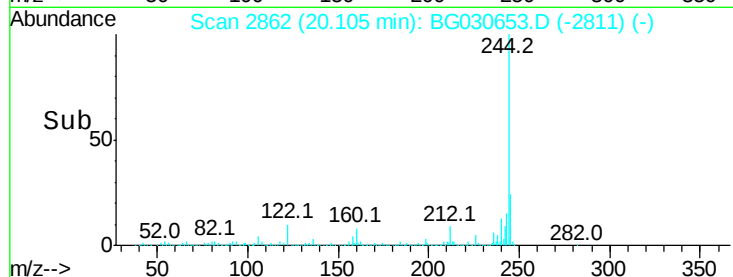

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.09 min Scan# 3710


Delta R.T. -0.01 min

Lab File: BG030653.D

Acq: 2 Nov 2017 3:01

Tgt Ion:264 Resp: 561407

Ion	Ratio	Lower	Upper
264	100		
260	24.0	17.4	26.0
265	21.1	17.7	26.5

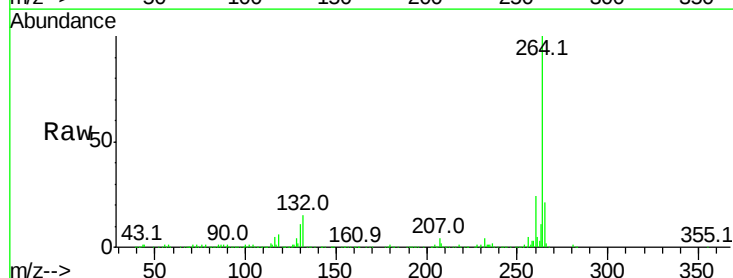

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

