

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110117\
 Data File : BG030653.D
 Acq On : 2 Nov 2017 3:01
 Operator : SJ/JU
 Sample : I6205-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 102517-TIDO-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.240	327	332	339	rBV	78678	121097	1.85%	0.465%
2	5.716	407	413	422	rBV	427870	693320	10.62%	2.661%
3	7.314	678	685	700	rBV	285980	525072	8.04%	2.015%
4	7.690	741	749	762	rBV	804147	1379757	21.13%	5.295%
5	8.160	822	829	836	rBV	242527	414414	6.35%	1.590%
6	8.484	876	884	896	rVB	1088021	1923886	29.46%	7.383%
7	9.324	1018	1027	1041	rBV	874793	1587506	24.31%	6.092%
8	10.975	1300	1308	1316	rBV	356908	659477	10.10%	2.531%
9	13.401	1713	1721	1733	rBV	2817433	4400434	67.38%	16.887%
10	14.218	1854	1860	1866	rBV	43297	67634	1.04%	0.260%
11	14.776	1948	1955	1963	rVB2	641838	1093283	16.74%	4.195%
12	16.045	2166	2171	2176	rBV	64619	85436	1.31%	0.328%
13	16.116	2178	2183	2189	rVB	69486	98554	1.51%	0.378%
14	16.257	2200	2207	2222	rBV	1462669	2236024	34.24%	8.581%
15	17.508	2414	2420	2431	rBV2	821448	1269771	19.44%	4.873%
16	20.105	2855	2862	2870	rBV	4758733	6530418	100.00%	25.060%
17	21.786	3141	3148	3157	rBV	871649	1490227	22.82%	5.719%
18	25.088	3700	3710	3726	rBV2	490336	1482503	22.70%	5.689%


Sum of corrected areas: 26058813

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110117\
Data File : BG030653.D
Acq On : 2 Nov 2017 3:01
Operator : SJ/JU
Sample : I6205-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

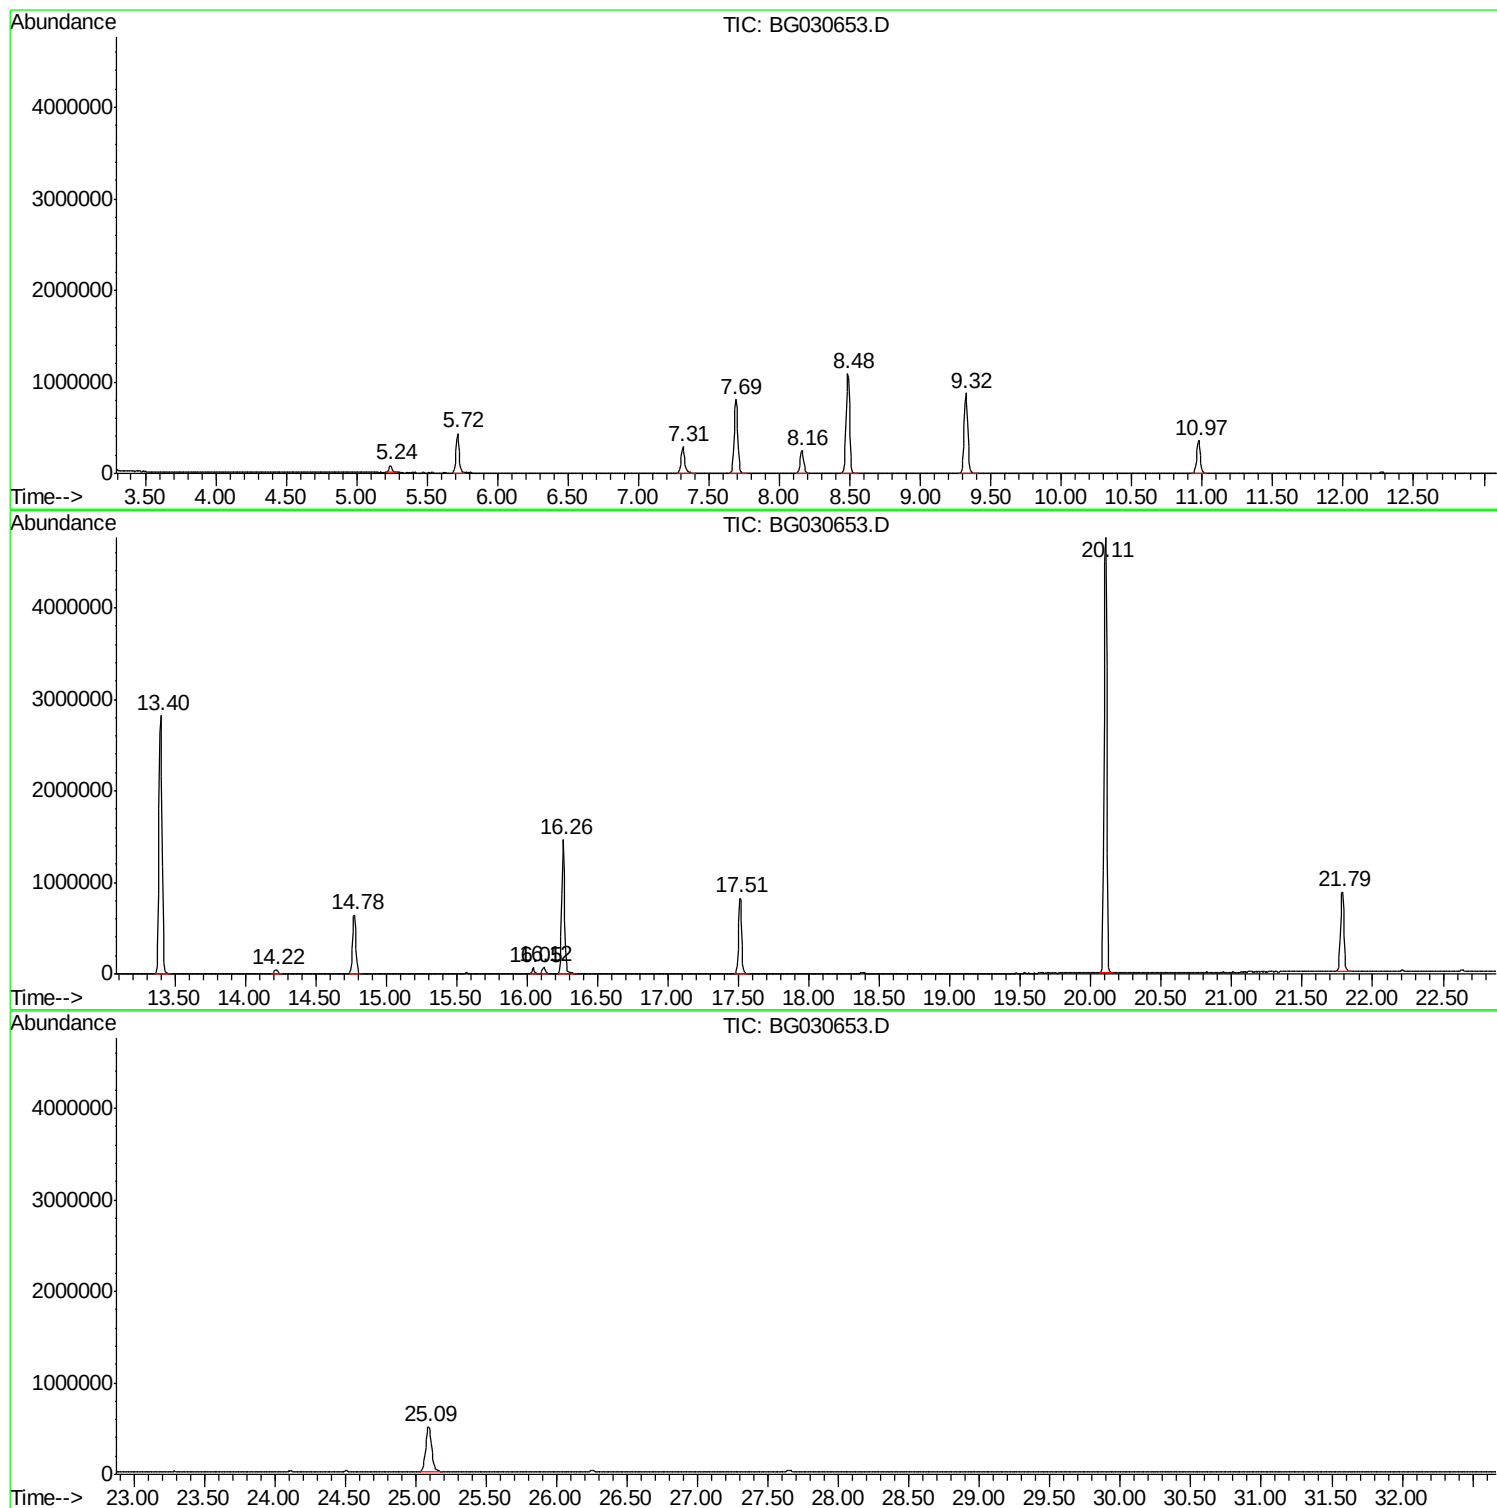

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG110117\
Data File : BG030653.D
Acq On : 2 Nov 2017 3:01
Operator : SJ/JU
Sample : I6205-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.24 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.24	5.84 ng	121097	1,4-Dichlorobenzene-d4	8.16

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hydrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	28
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	25
4			4-Hydroxy-3-hexanone	116	C6H12O2	004984-85-4	23
5			Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	17

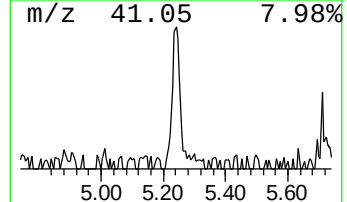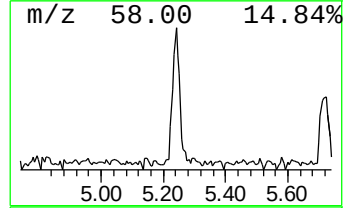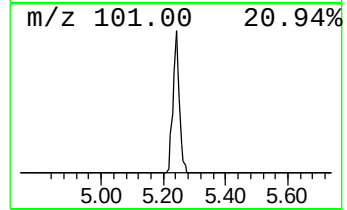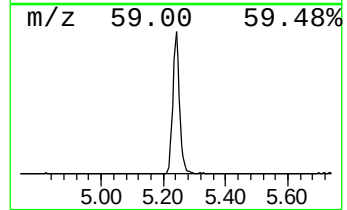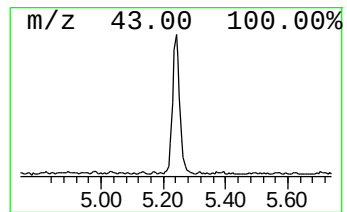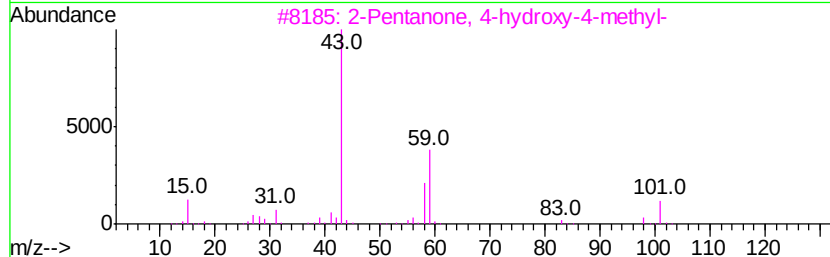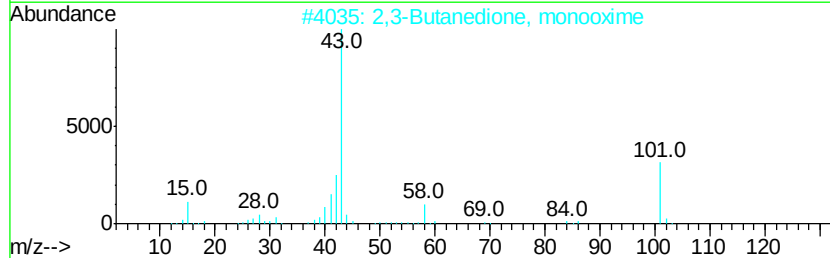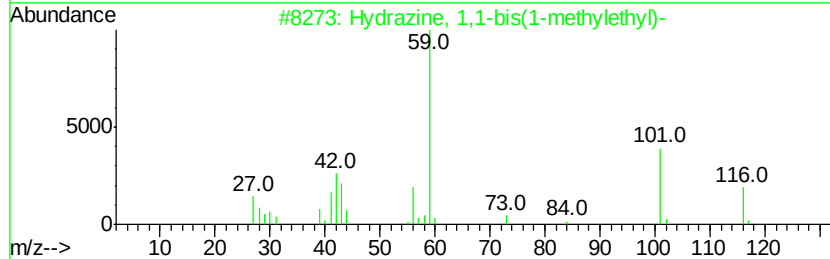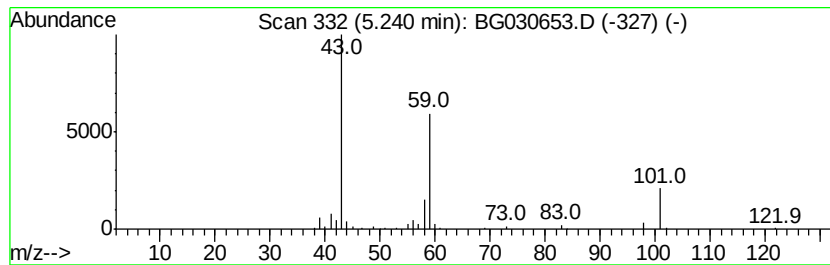

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA G\DATA\BG110117\
Data File : BG030653.D
Acq On : 2 Nov 2017 3:01
Operator : SJ/JU
Sample : I6205-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.69 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	66.59 ng	1379760	1,4-Dichlorobenzene-d4	8.16

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

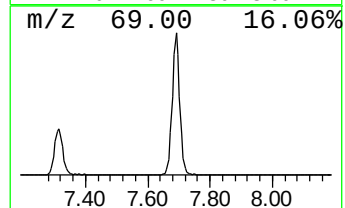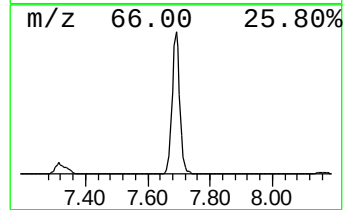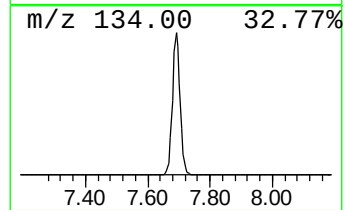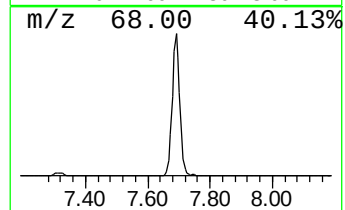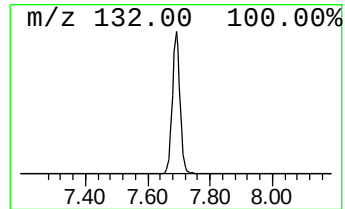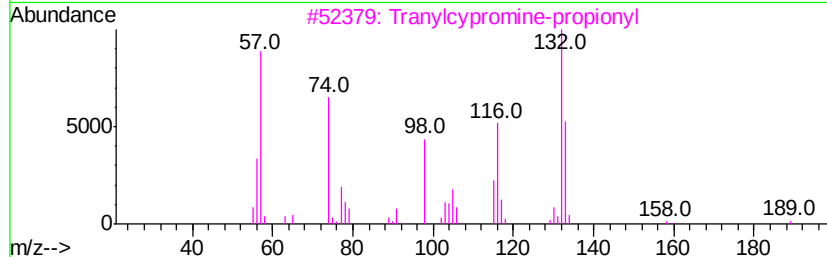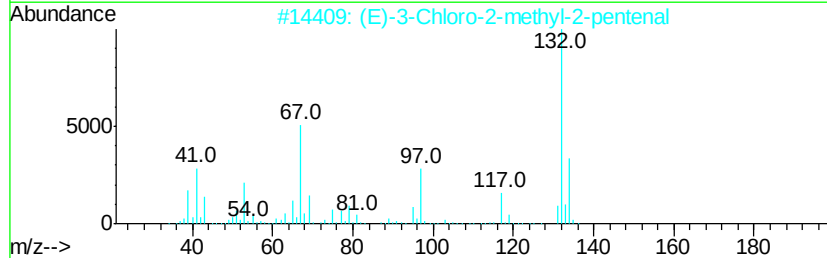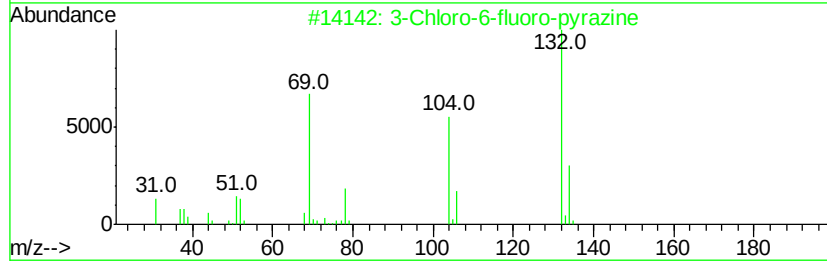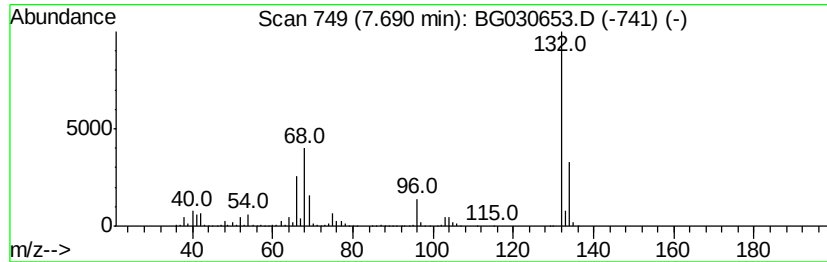

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG110117\
Data File : BG030653.D
Acq On : 2 Nov 2017 3:01
Operator : SJ/JU
Sample : I6205-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
102517-TIDO-F-U-B

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.24	5.24	5.8	ng	121097	1	8.16	414414	20.0
unknown7.69	7.69	66.6	ng	1379760	1	8.16	414414	20.0