


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG110117\
 Data File : BG030625.D
 Acq On : 1 Nov 2017 8:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 01 17:41:24 2017

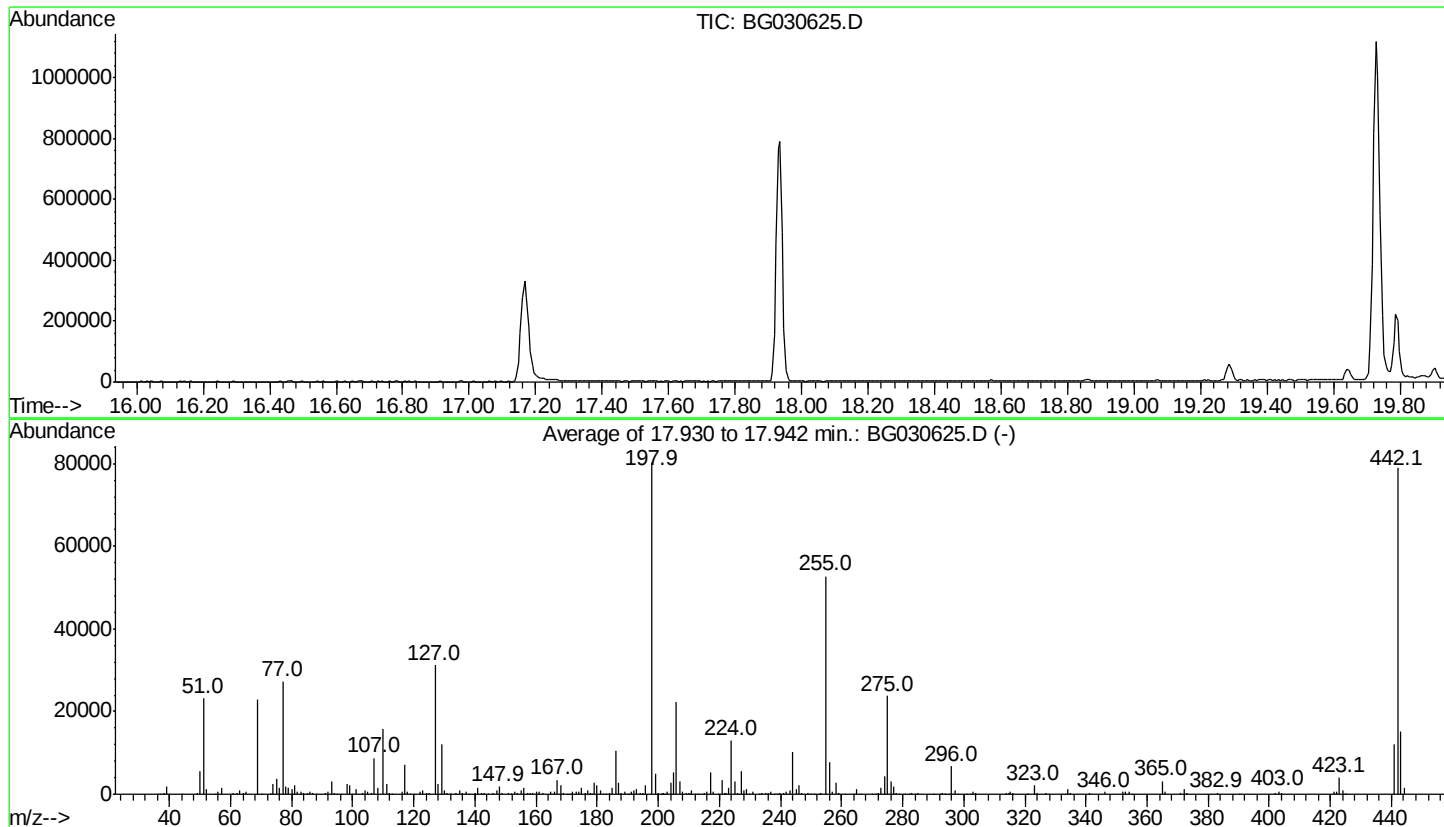

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	23098	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.6	22979	PASS
70	69	0.00	2	0.5	126	PASS
127	198	10	80	39.0	31266	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80248	PASS
199	198	5	9	6.3	5095	PASS
275	198	10	60	29.6	23722	PASS
365	198	1	100	3.9	3116	PASS
441	442	0.01	24	15.2	12064	PASS
442	198	50	100	98.6	79138	PASS
443	442	15	24	19.4	15330	PASS