
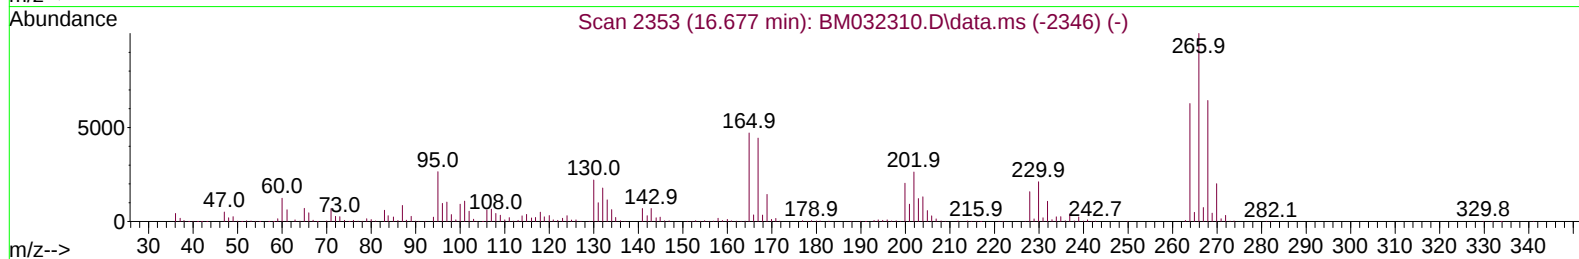
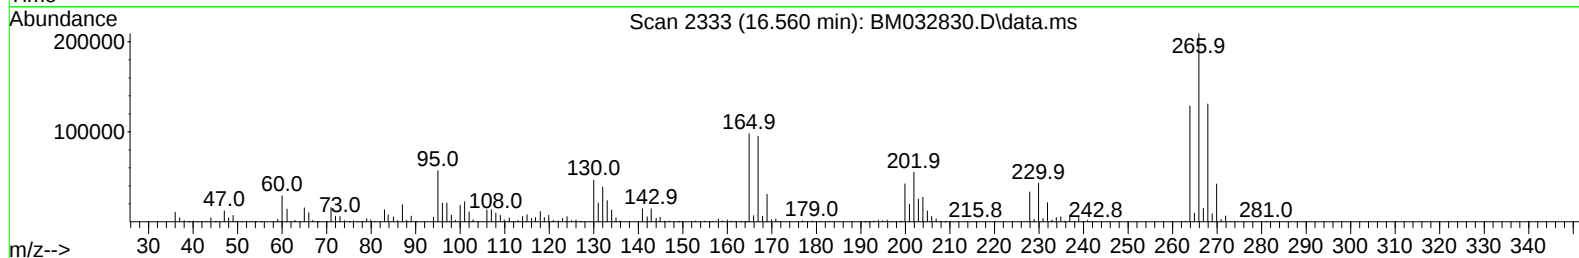


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
Data File : BM032830.D
Acq On : 01 Nov 2021 12:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 14:25:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 23 01:22:28 2021
Response via : Initial Calibration

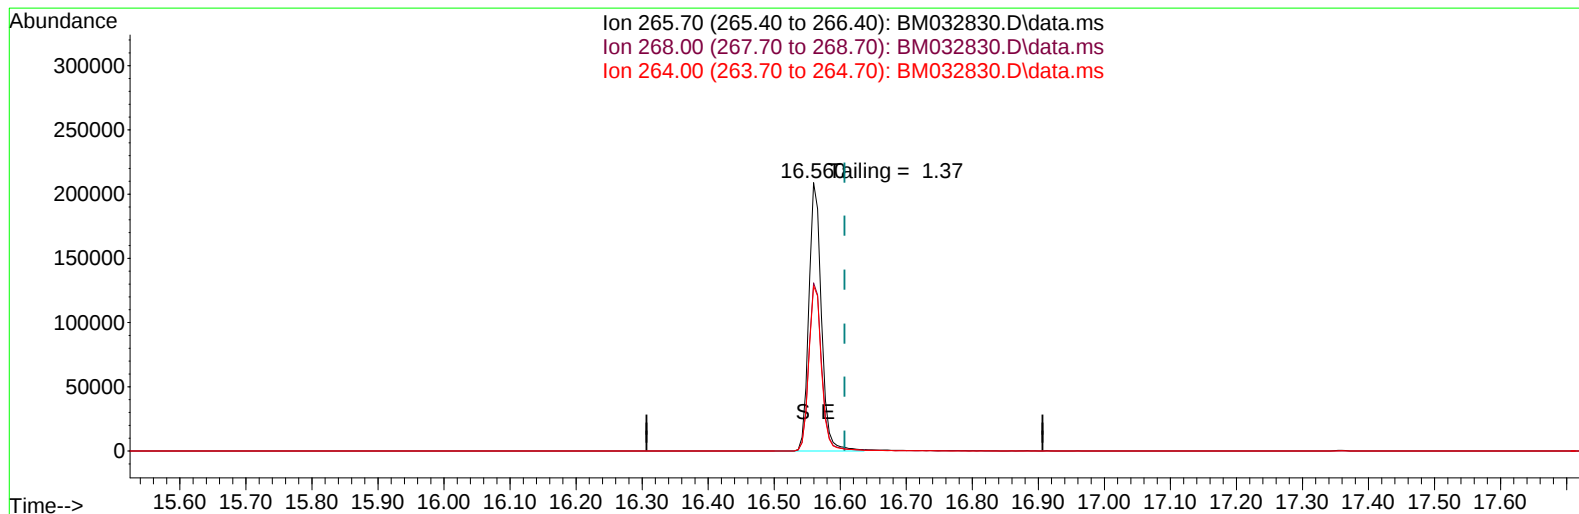

TIC: BM032830.D\data.ms

(70) Pentachlorophenol (C)

16.560min (-0.047) 0.00 ng

response 277787

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.68
264.00	65.10	61.56
0.00	0.00	0.00