
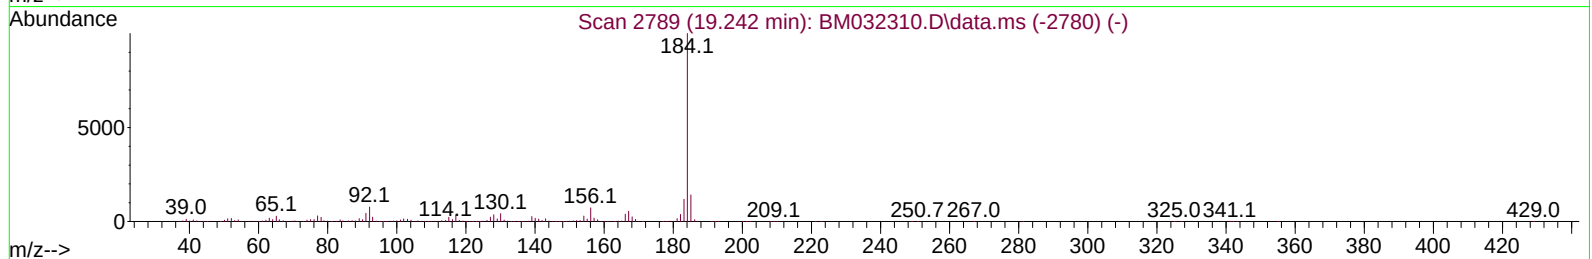
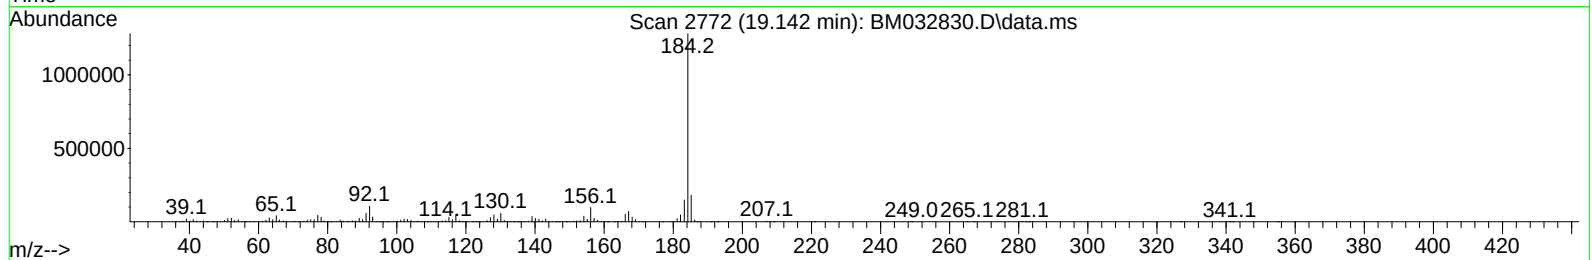


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110121\
Data File : BM032830.D
Acq On : 01 Nov 2021 12:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 14:25:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM100221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 23 01:22:28 2021
Response via : Initial Calibration

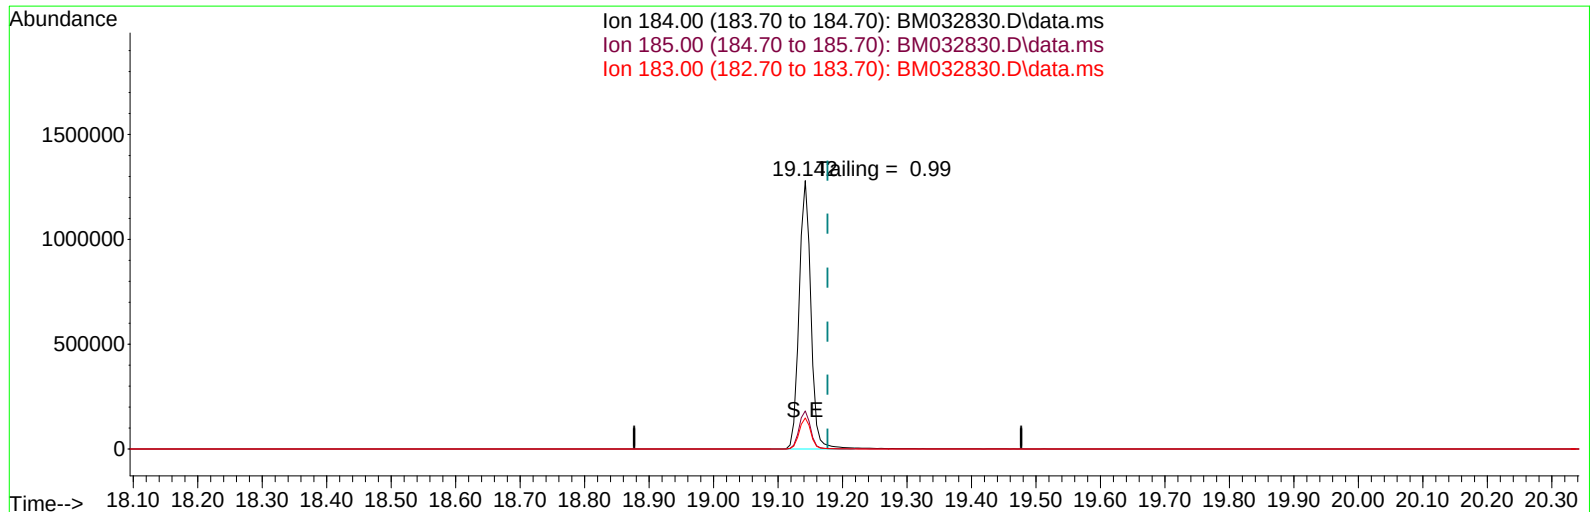

TIC: BM032830.D\data.ms

(77) Benzidine

19.142min (-0.035) 0.00 ng

response 1627768

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.18
183.00	11.20	11.62
0.00	0.00	0.00