
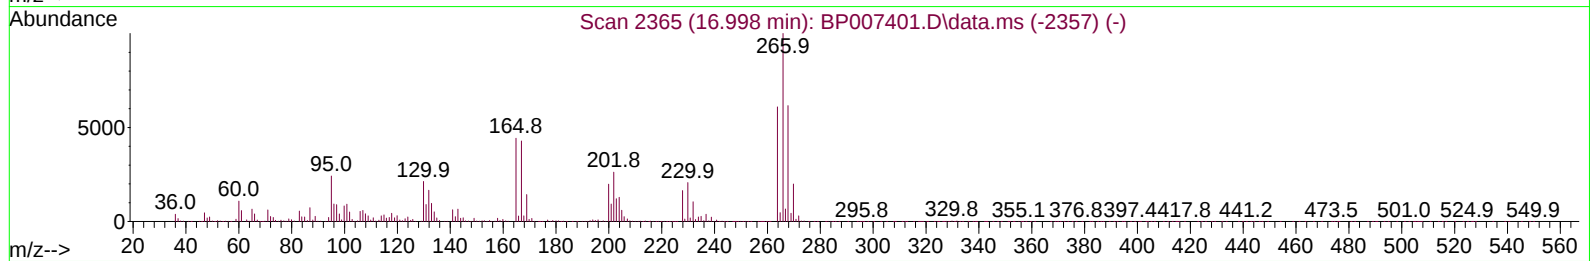
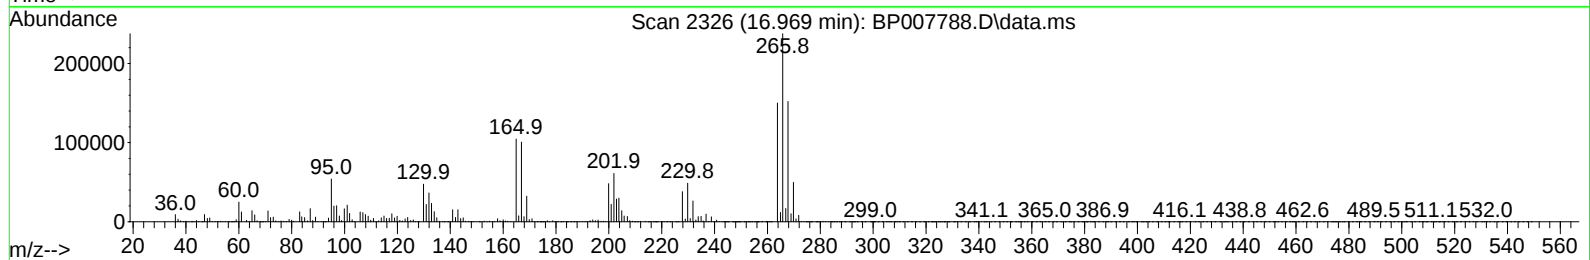


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110121\
Data File : BP007788.D
Acq On : 01 Nov 2021 12:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 14:34:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 13 14:54:20 2021
Response via : Initial Calibration

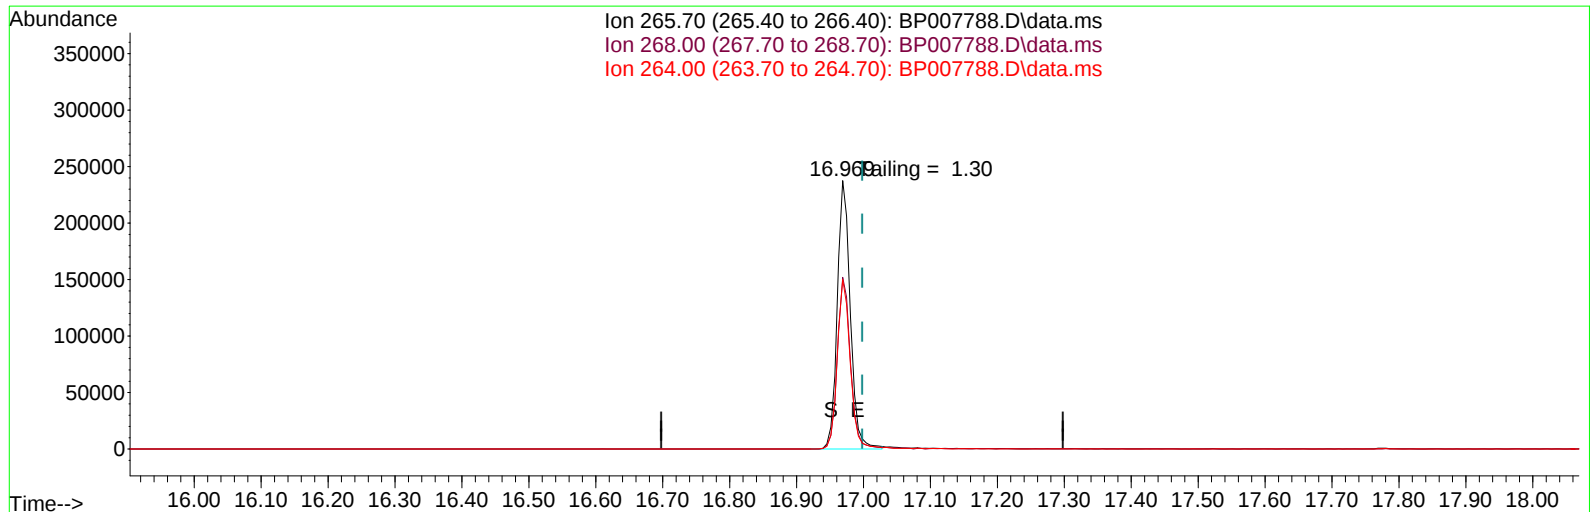

TIC: BP007788.D\data.ms

(70) Pentachlorophenol (C)

16.969min (-0.029) 2876622.33 ng

response 324598

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.98
264.00	60.90	63.15
0.00	0.00	0.00