
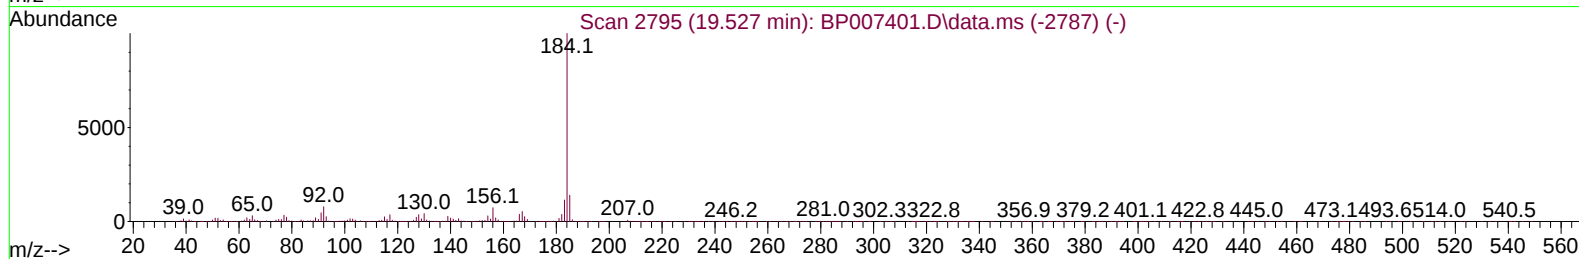
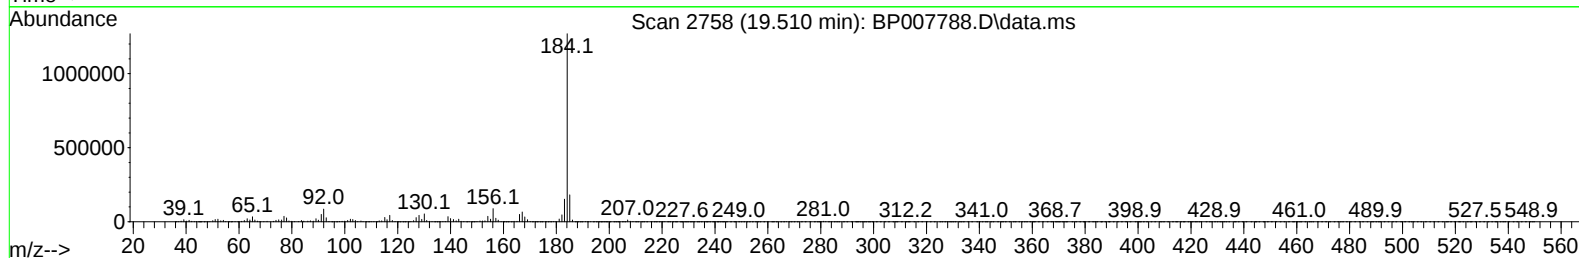


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110121\
 Data File : BP007788.D
 Acq On : 01 Nov 2021 12:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 01 14:34:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 13 14:54:20 2021
 Response via : Initial Calibration

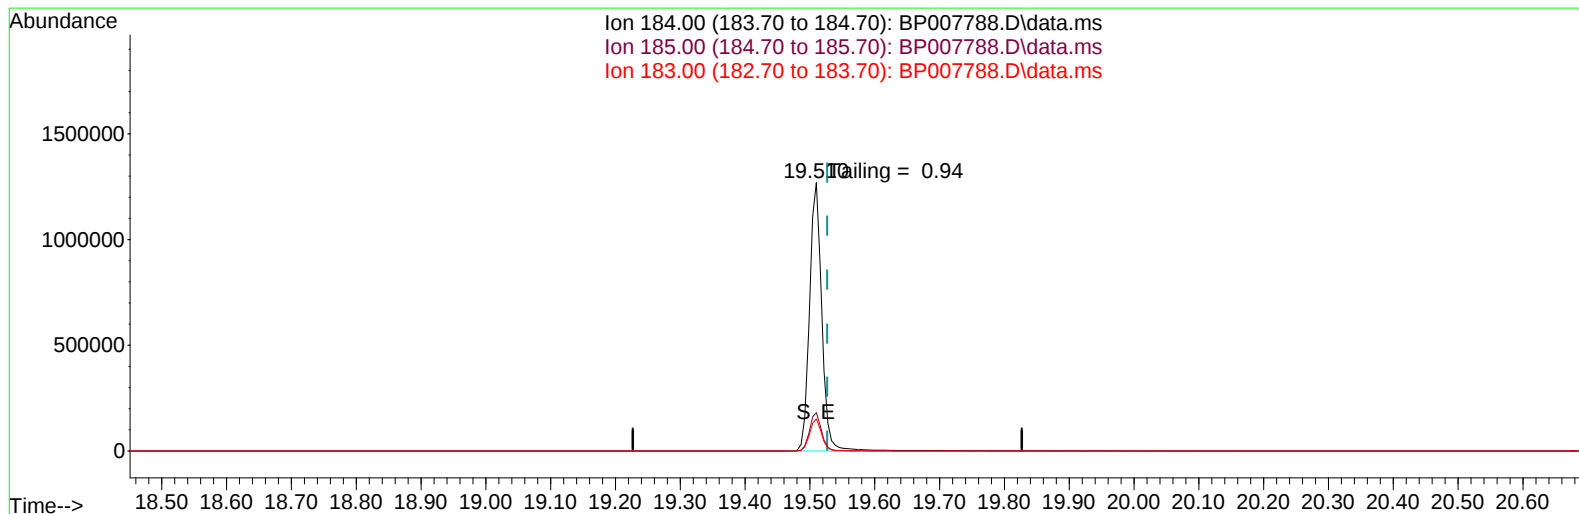

TIC: BP007788.D\data.ms

(77) Benzidine**19.510min (-0.017) 594839.03 ng****response 1678411**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.34
183.00	11.40	11.98
0.00	0.00	0.00