
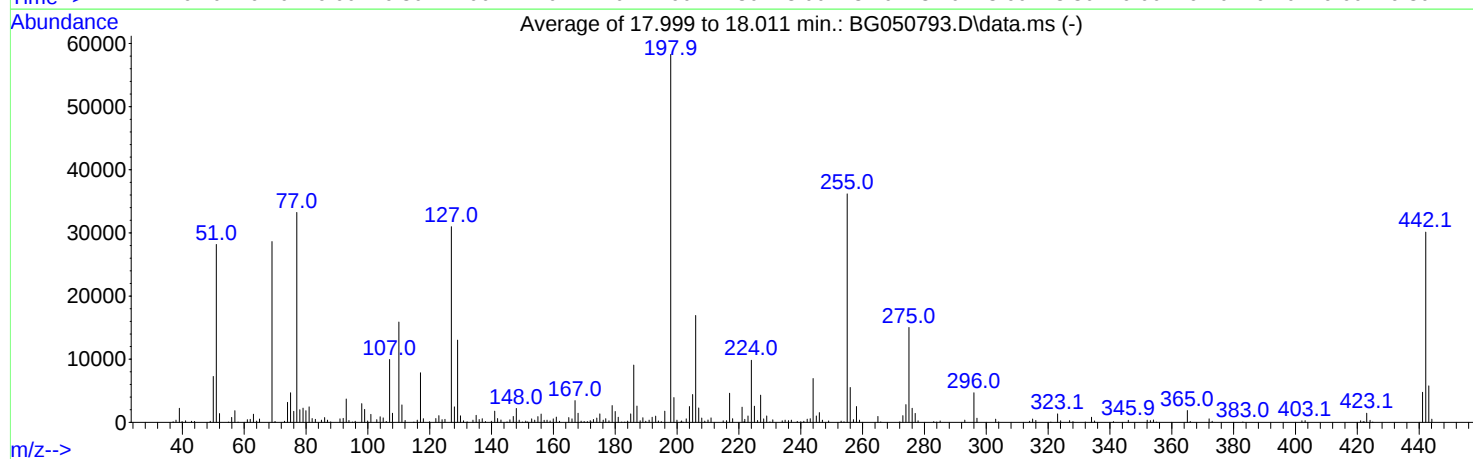


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110121\
 Data File : BG050793.D
 Acq On : 1 Nov 2021 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 01 12:35:42 2021

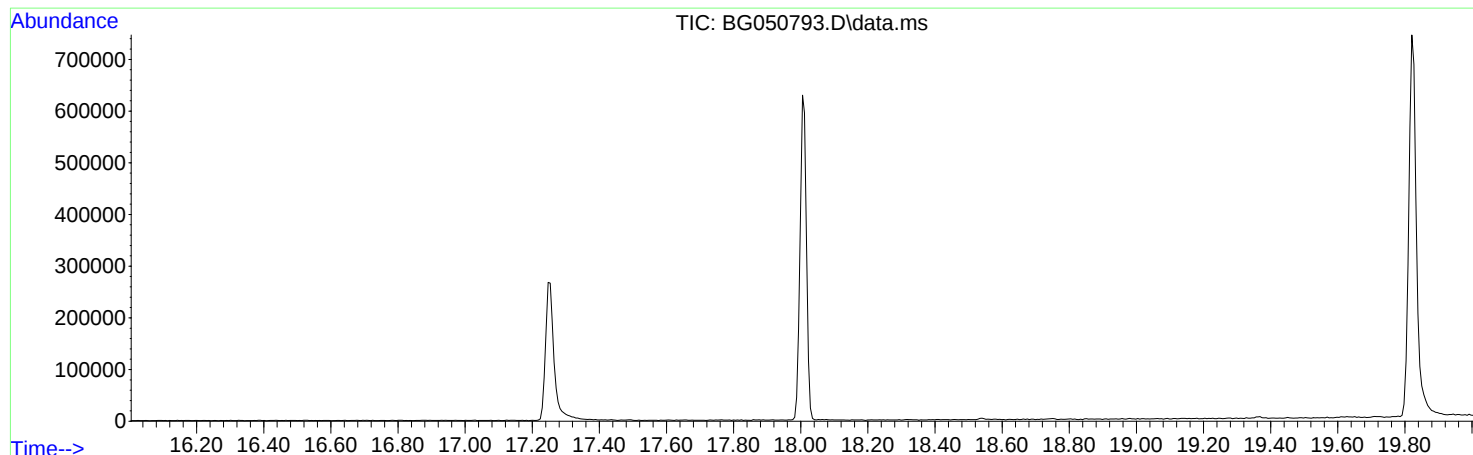




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	28168	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.2	28640	PASS
70	69	0.00	2	0.5	142	PASS
127	198	10	80	53.2	30979	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58253	PASS
199	198	5	9	6.7	3917	PASS
275	198	10	60	25.8	15035	PASS
365	198	1	100	3.2	1868	PASS
441	198	0.01	100	8.2	4753	PASS
442	442	50	100	100.0	30139	PASS
443	442	15	24	19.2	5775	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110121\
Data File : BG050793.D
Acq On : 1 Nov 2021 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 01 11:14:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

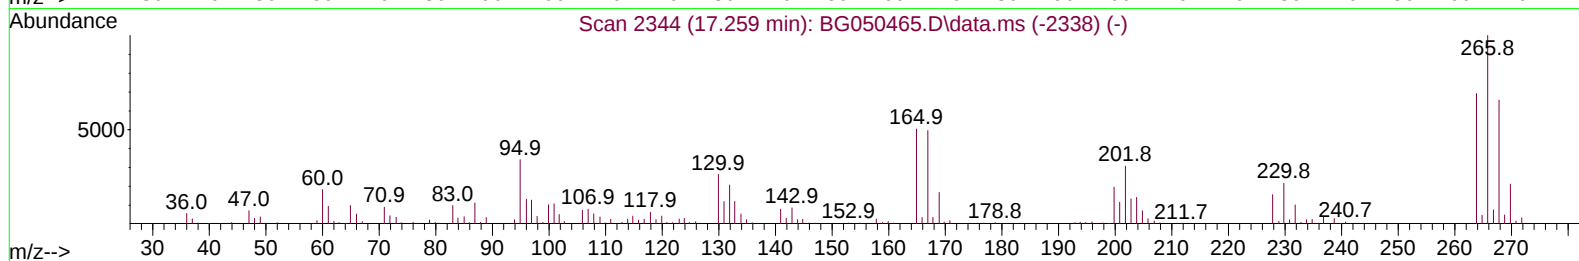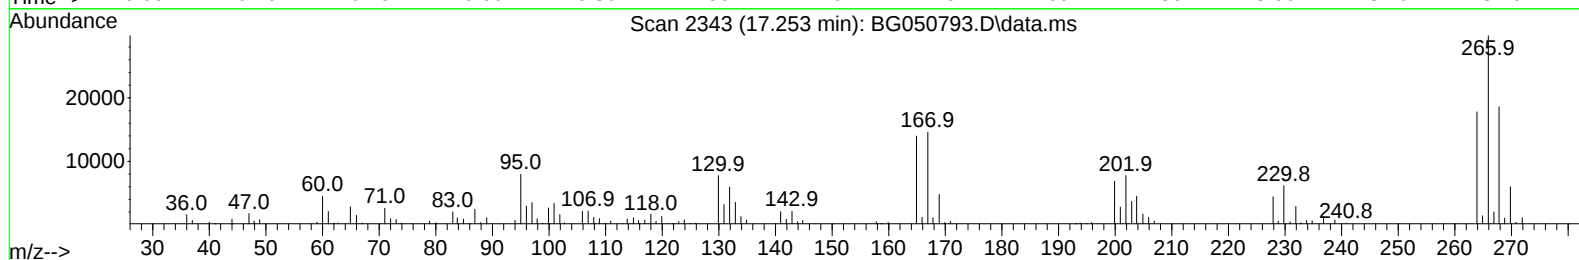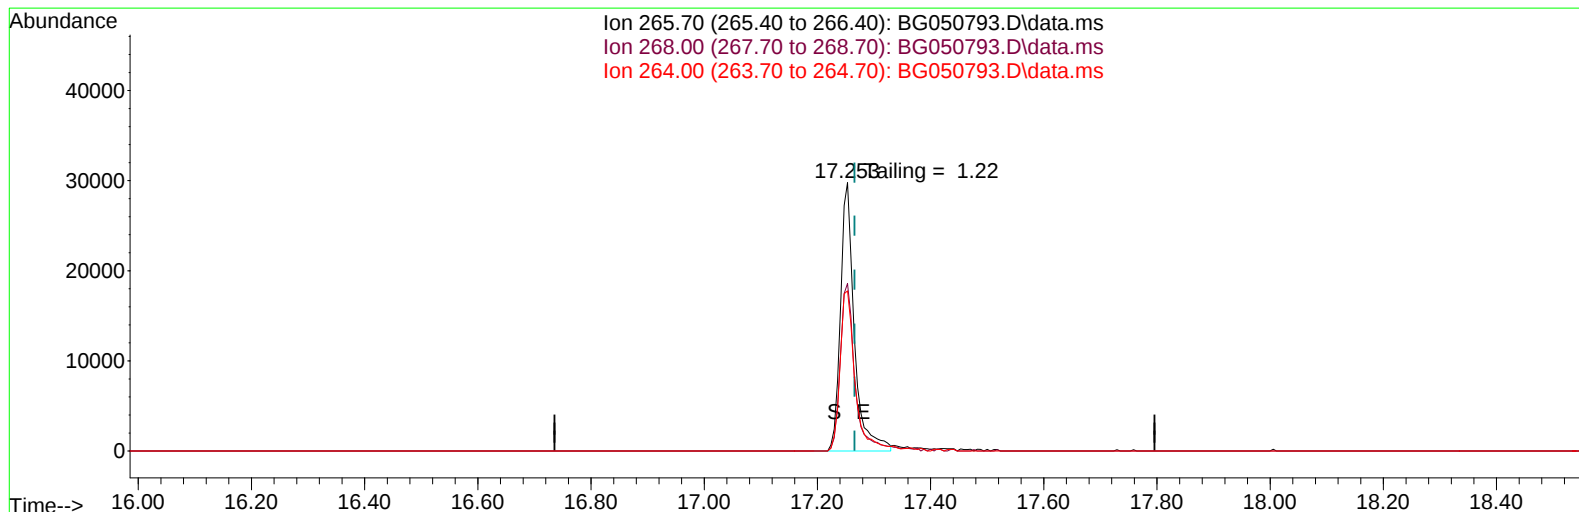

TIC: BG050793.D\data.ms

(70) Pentachlorophenol (C)

17.253min (-0.012) 29539.62 ng




response 52363

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.42
264.00	61.30	59.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110121\
Data File : BG050793.D
Acq On : 1 Nov 2021 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 01 11:14:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

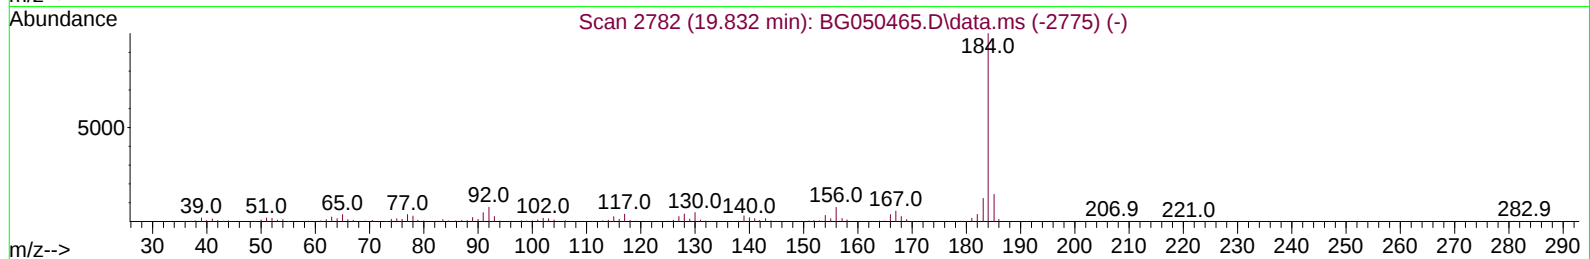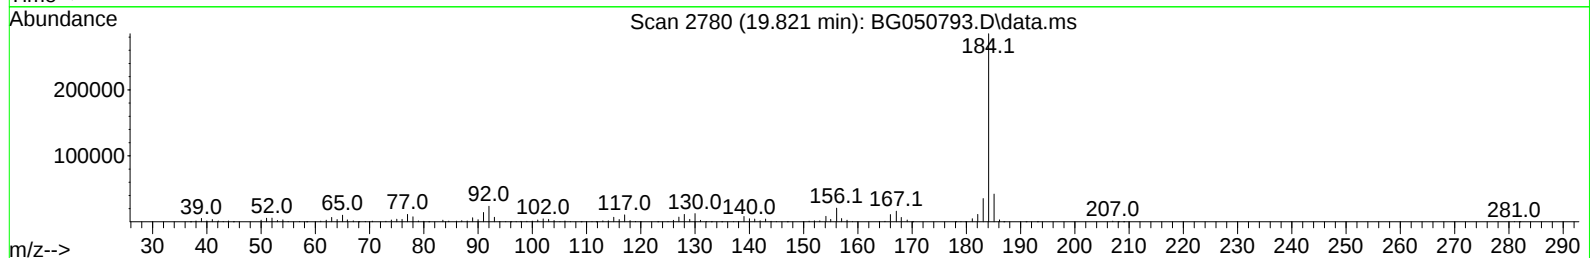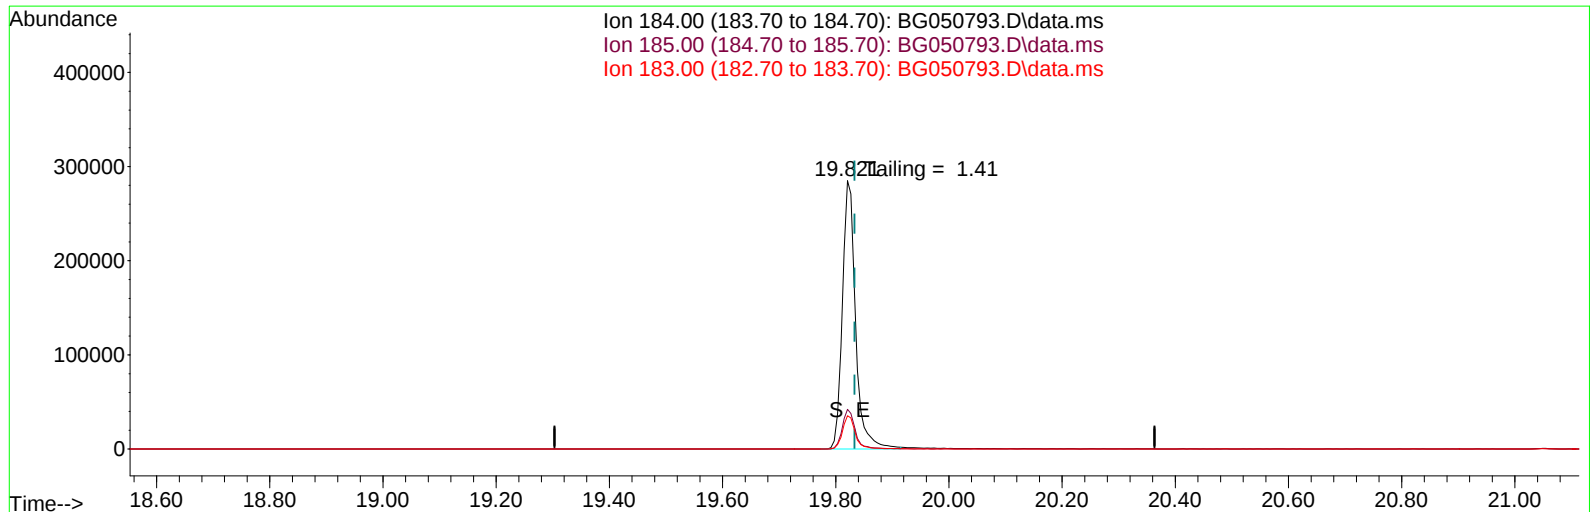

TIC: BG050793.D\data.ms

(77) Benzidine

19.821min (-0.012) 0.00 ng

response 464569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.78
183.00	11.70	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/1/2021	BNA_G	BG050793.D
Compound Name	Response	Retention Time
DDT	175468	21.05
DDD	14676	20.6
DDE	177	20.09
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14853	190321	7.80

Instrument :
BNA_G
ClientSampleId :
DFTPP