
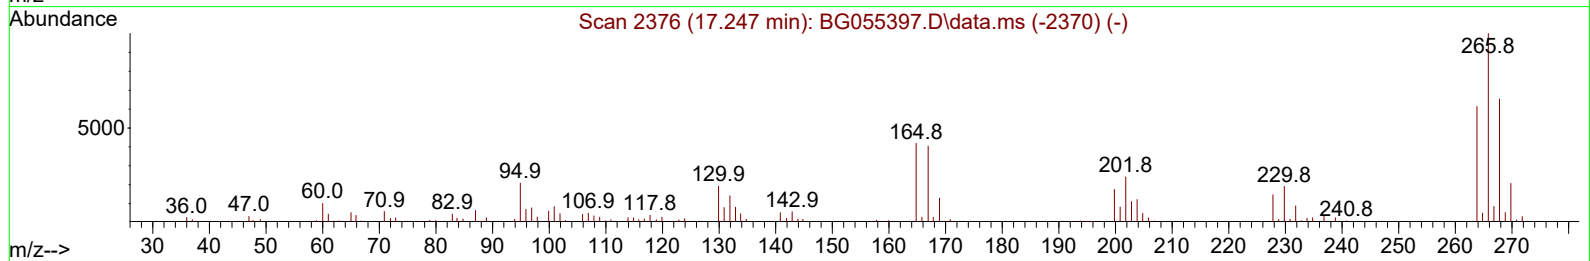
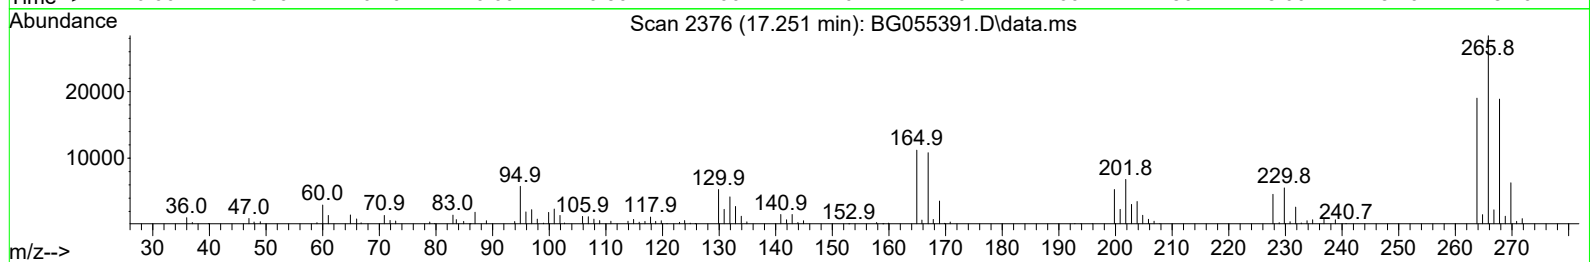


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110122\
Data File : BG055391.D
Acq On : 1 Nov 2022 12:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 06:53:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

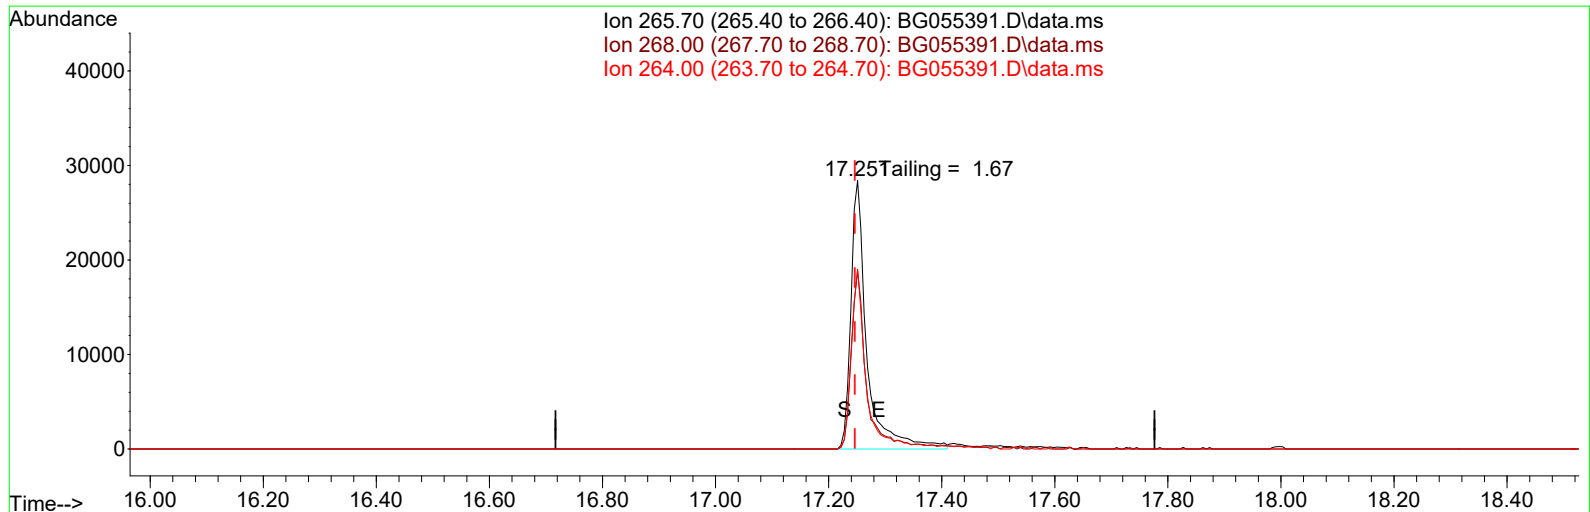

TIC: BG055391.D\data.ms

(70) Pentachlorophenol (C)




17.251min (+ 0.004) 33671.03 ng

response 56111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	66.50
264.00	61.50	66.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG110122\
Data File : BG055391.D
Acq On : 1 Nov 2022 12:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 06:53:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 02 05:05:12 2022
Response via : Initial Calibration

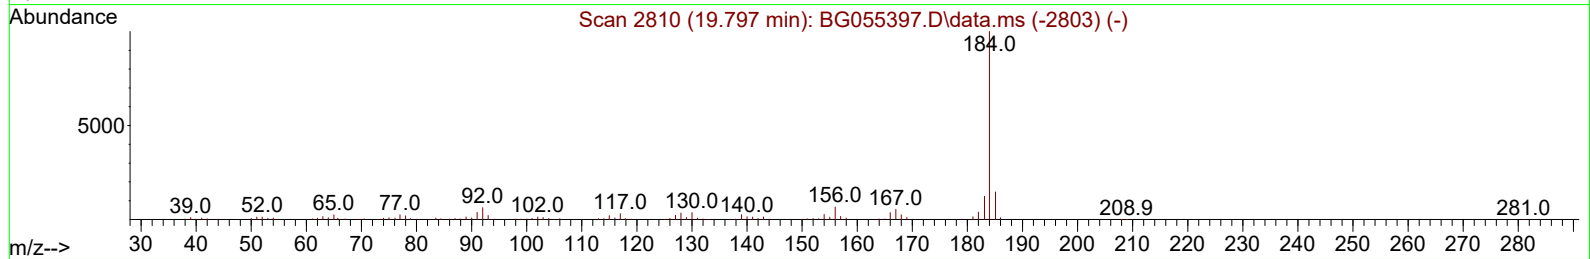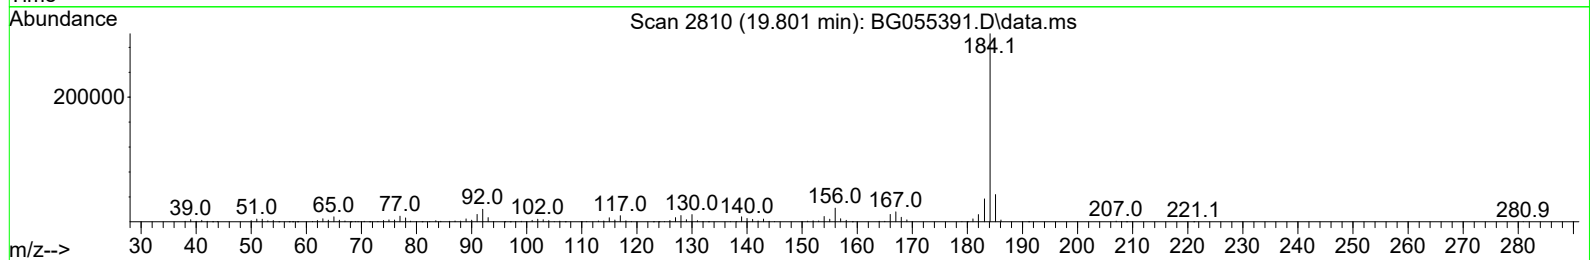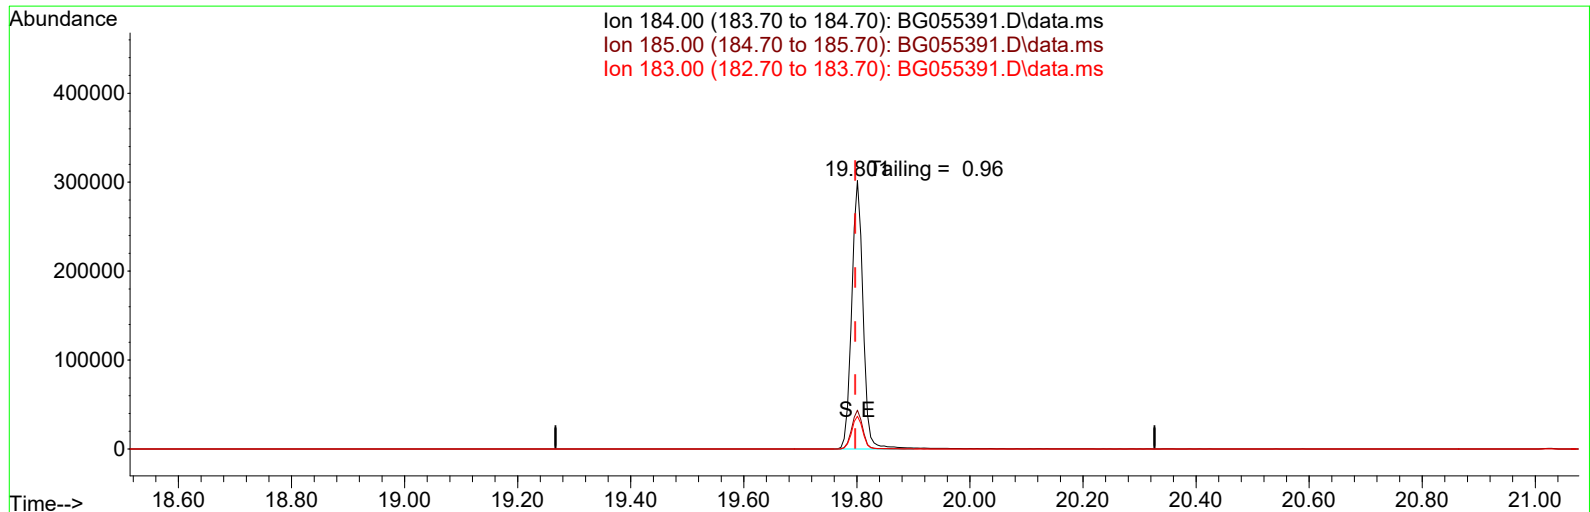

TIC: BG055391.D\data.ms

(77) Benzidine**19.801min (+ 0.004) 60656.94 ng****response 423050**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.51
183.00	12.30	12.23
0.00	0.00	0.00